
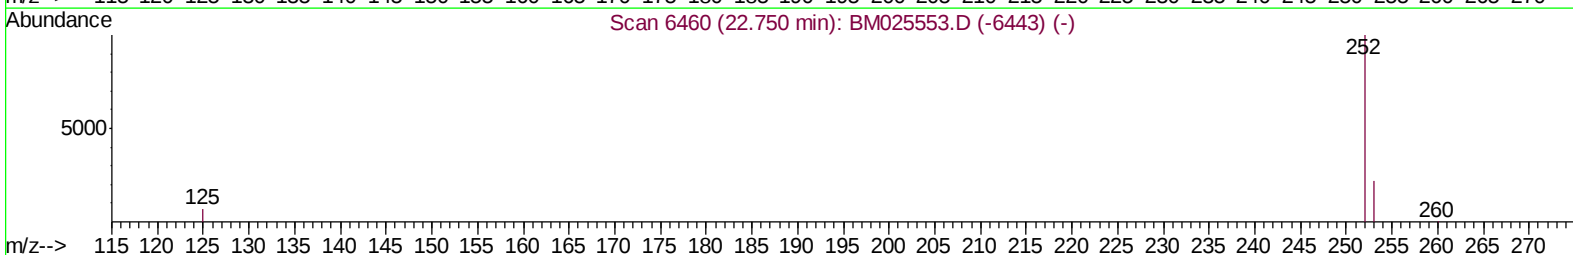
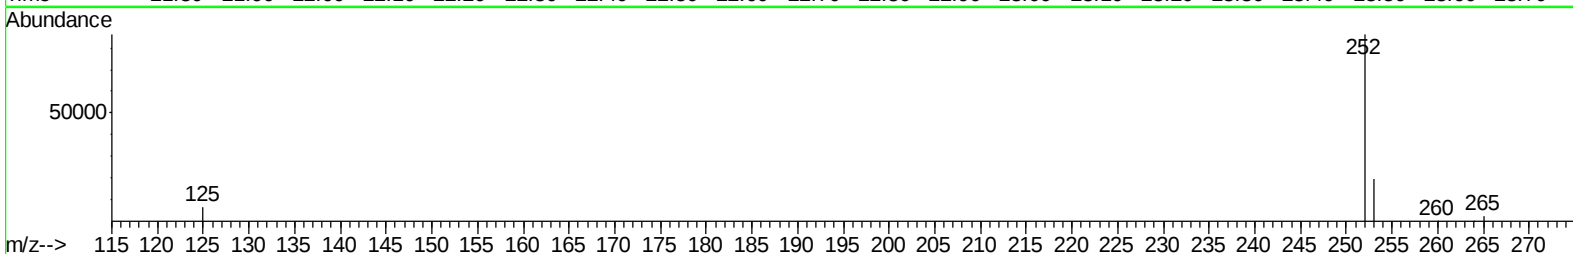


Data File : BM025564.D
Acq On : 14 Mar 2020 05:38
Operator : CG/JU
Sample : L1786-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Mar 16 06:49:27 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 16 06:44:28 2020
Response via : Initial Calibration

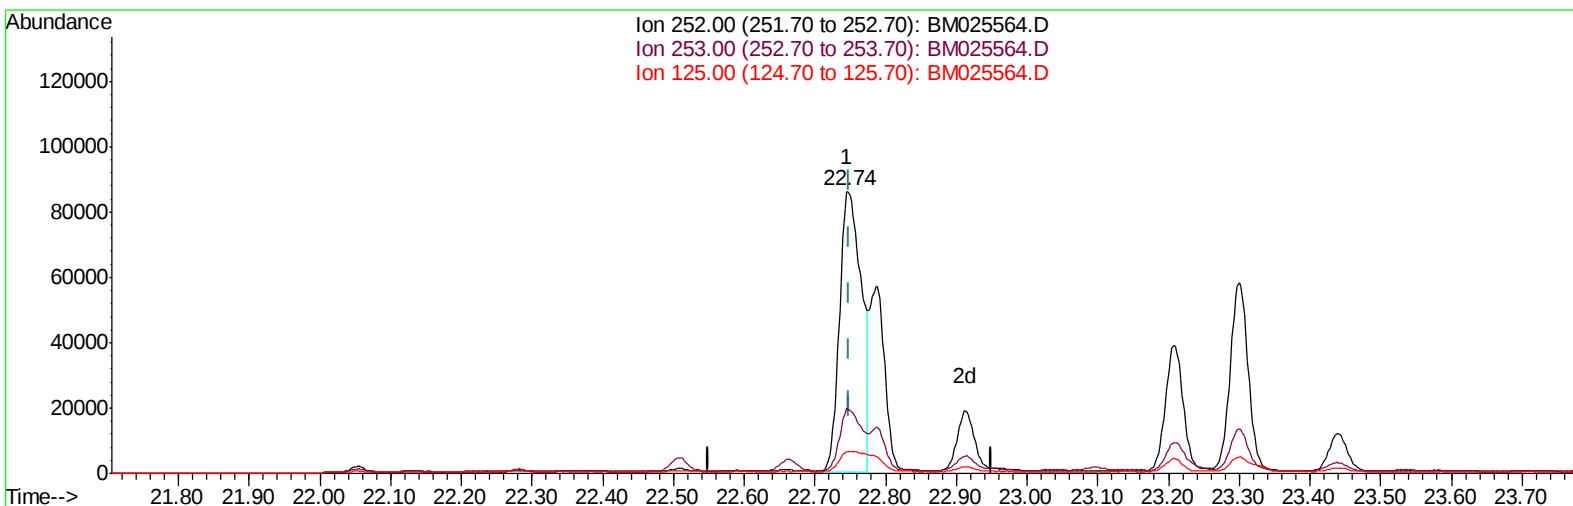

TIC: BM025564.D

(21) Benzo(b)fluoranthene

22.745min (-0.005) 2.84ng/ul m

response 185042

Ion	Exp%	Act%
252.00	100	100
253.00	25.10	23.02
125.00	8.80	7.93
0.00	0.00	0.00