


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031320\
Data File : BM025543.D
Acq On : 13 Mar 2020 16:21
Operator : CG/JU
Sample : PB127314BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK14

Manual Integrations
APPROVED

mohammad
3/16/2020 1:52:05 PM

Quant Time: Mar 13 16:59:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 13 16:53:43 2020
Response via : Initial Calibration

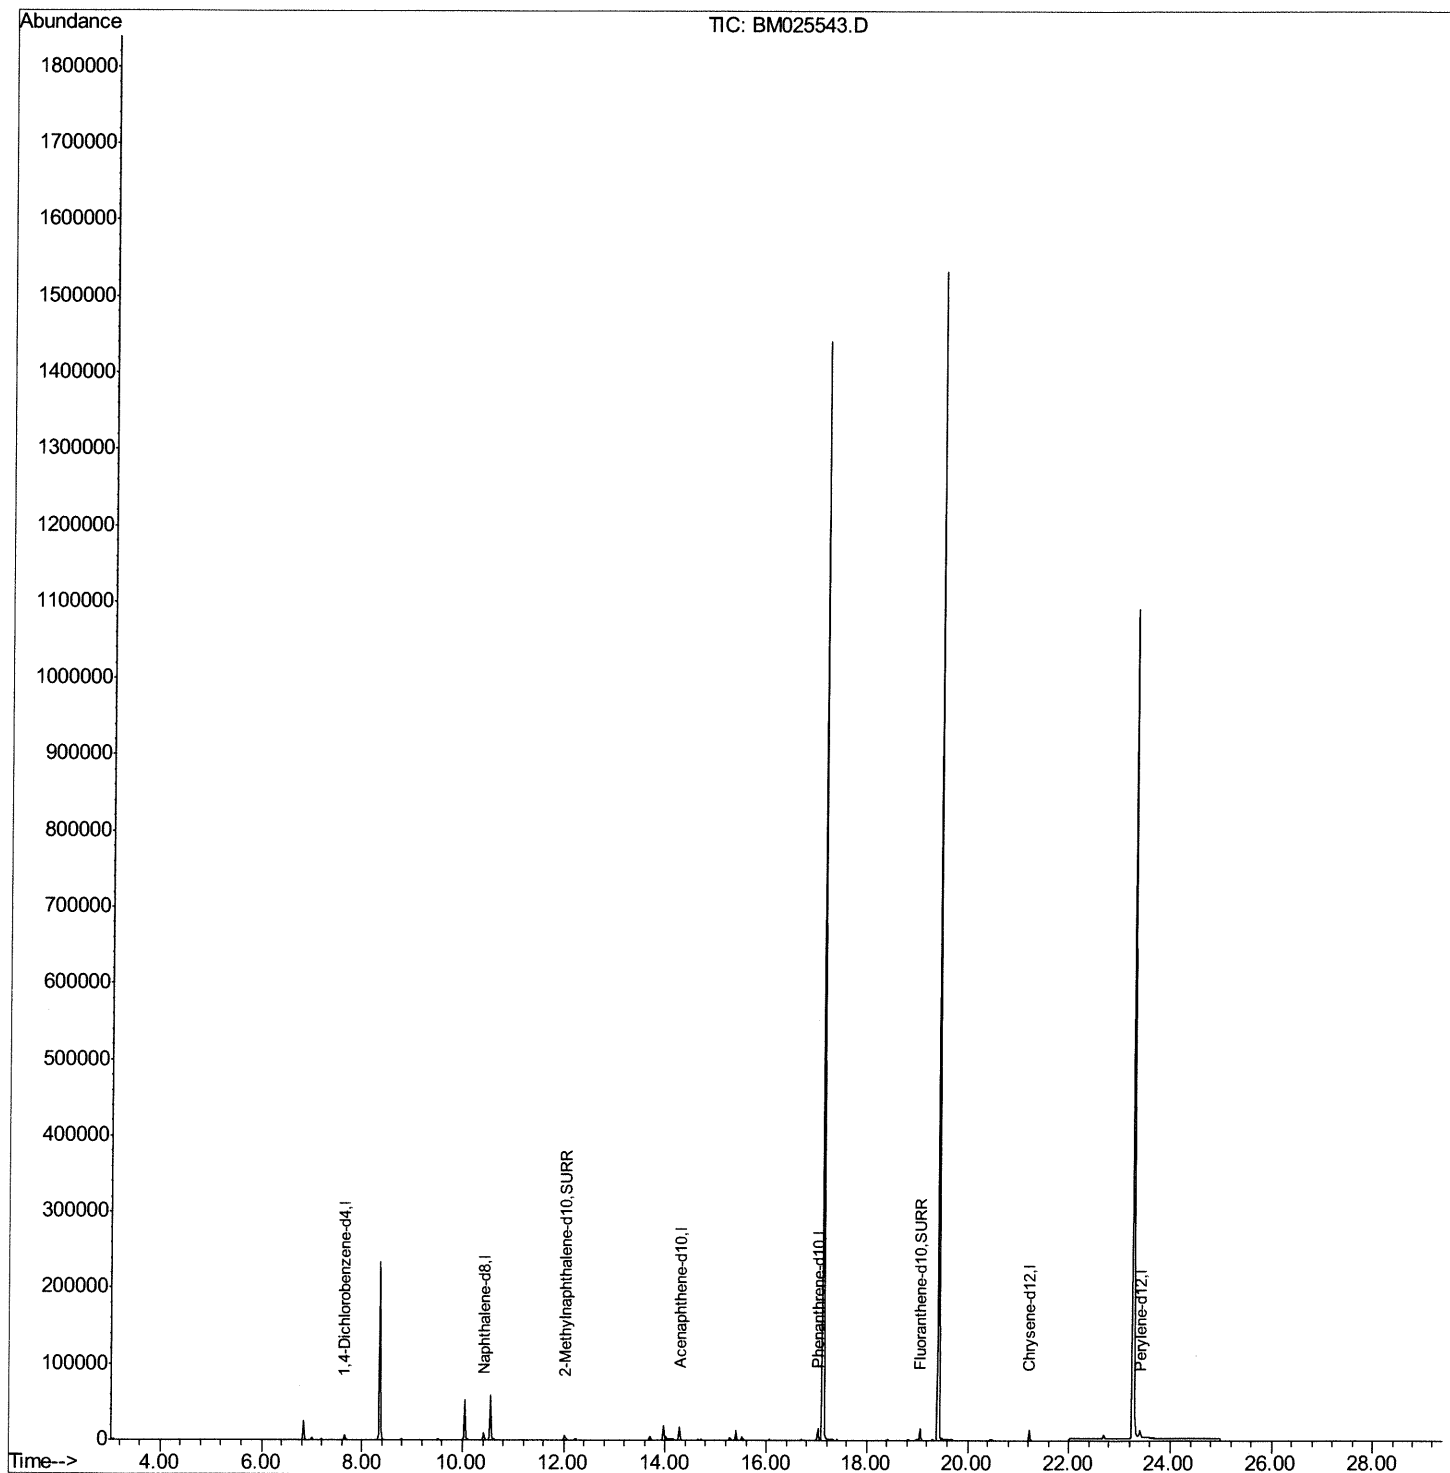

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031320\
 Data File : BM025543.D
 Acq On : 13 Mar 2020 16:21
 Operator : CG/JU
 Sample : PB127314BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK14

Manual Integrations
 APPROVED

mohammad
 3/16/2020 1:52:05 PM

Quant Time: Mar 13 16:56:29 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 13 16:53:43 2020
 Response via : Initial Calibration

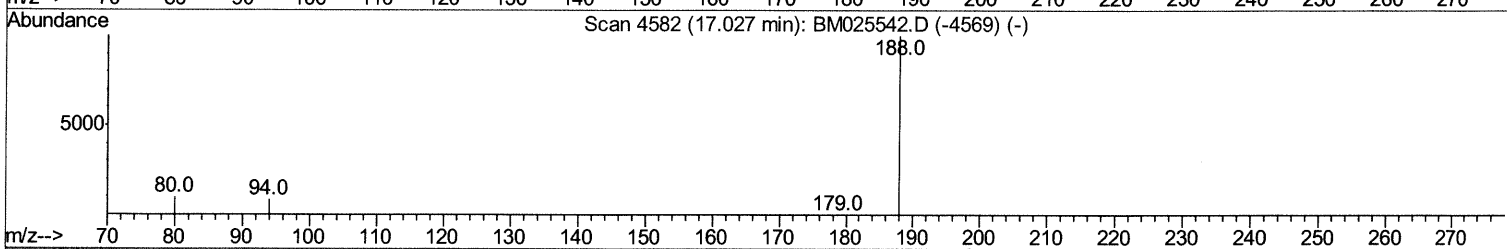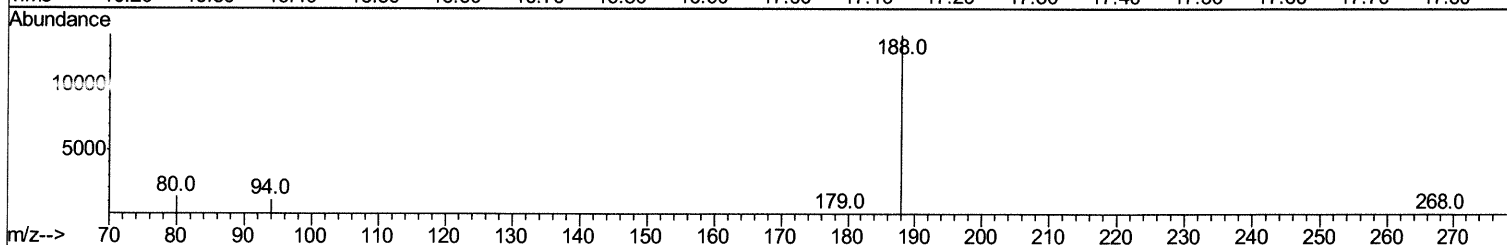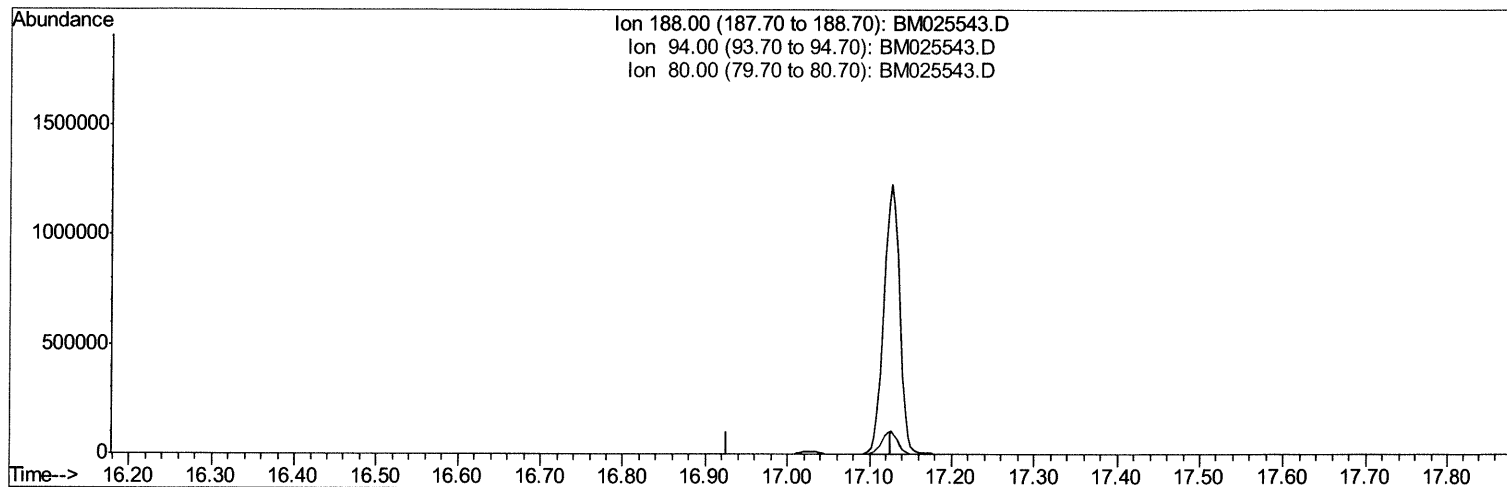

TIC: BM025543.D

(10) Phenanthrene-d10 (I)

17.027min (-17.027) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.10	0.00#
80.00	8.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031320\
Data File : BM025543.D
Acq On : 13 Mar 2020 16:21
Operator : CG/JU
Sample : PB127314BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK14

Manual Integrations
APPROVED

mohammad
3/16/2020 1:52:05 PM

Quant Time: Mar 13 16:56:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 13 16:53:43 2020
Response via : Initial Calibration

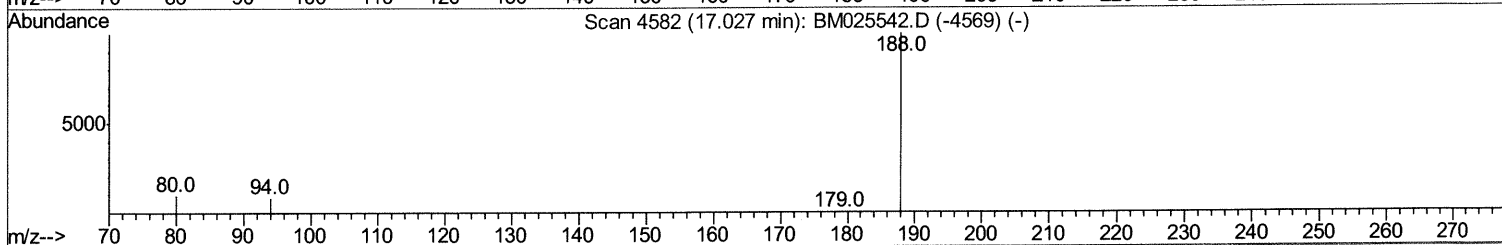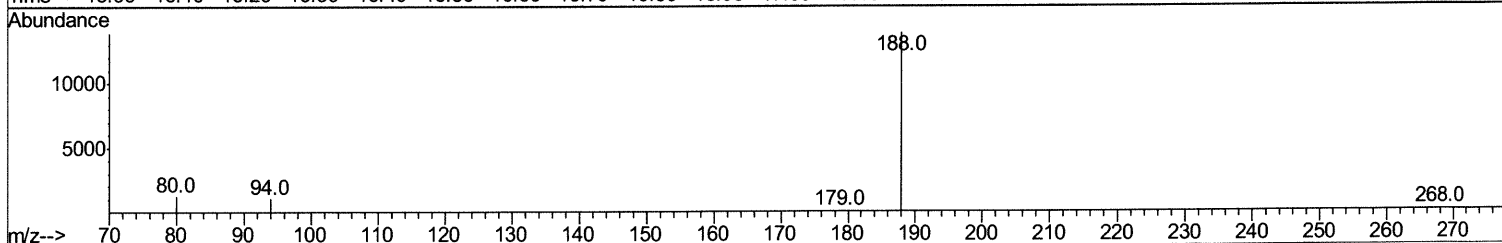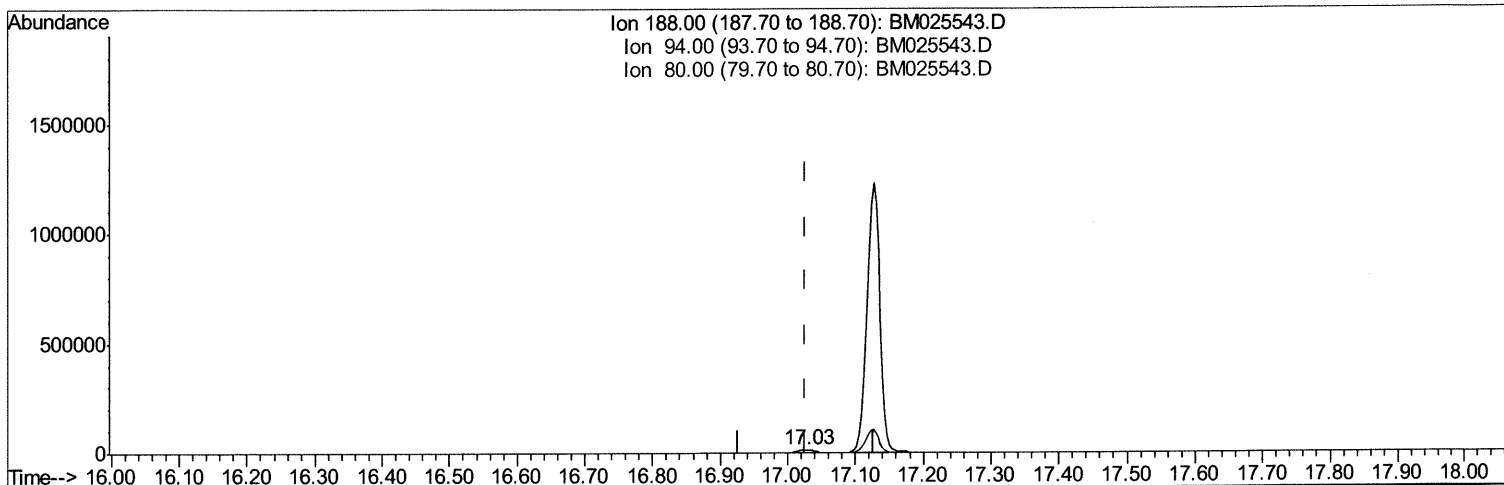

TIC: BM025543.D

(10) Phenanthrene-d10 (I)

17.029min (+0.002) 0.40ng/ul m 5u03/16/20

response 19510

Ion	Exp%	Act%
188.00	100	100
94.00	7.10	7.74
80.00	8.70	9.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031320\
Data File : BM025543.D
Acq On : 13 Mar 2020 16:21
Operator : CG/JU
Sample : PB127314BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK14

Manual Integrations
APPROVED

mohammad
3/16/2020 1:52:05 PM

Quant Time: Mar 13 16:59:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 13 16:53:43 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	2923	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	12506	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.28	164	9324	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.03	188	19510m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.22	240	12731	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	13529	0.40	ng/ul	0.00

3/16/20

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.02	152	8069	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	17305	0.32	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed