

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
 Data File : BM039002.D
 Acq On : 13 Mar 2023 22:42
 Operator : CG/JU
 Sample : PB151312BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK312

Quant Time: Mar 14 01:44:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 13 16:25:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.987	152	349443	20.000	ng/ul	0.00
20) Naphthalene-d8	10.798	136	1552116	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.622	164	991624	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.369	188	2069532	20.000	ng/ul	0.00
79) Chrysene-d12	21.545	240	1556916	20.000	ng/ul	0.00
88) Perylene-d12	23.992	264	1400517	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	70839	7.069	ng/uL	0.00
4) Pyridine-d5	3.793	84	826242	29.150	ng/ul	0.00
7) Phenol-d5	7.140	99	1124368	33.425	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.310	67	749391	34.471	ng/ul	0.00
11) 2-Chlorophenol-d4	7.510	132	872996	34.862	ng/ul	0.00
15) 4-Methylphenol-d8	8.693	113	872694	33.161	ng/ul	0.00
21) Nitrobenzene-d5	9.152	128	453829	34.975	ng/ul	0.00
24) 2-Nitrophenol-d4	9.875	143	475943	36.405	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.416	165	793734	33.166	ng/ul	0.00
31) 4-Chloroaniline-d4	10.934	131	837270	21.631	ng/ul	0.00
46) Dimethylphthalate-d6	14.034	166	2661984	35.443	ng/ul	0.00
49) Acenaphthylene-d8	14.316	160	3005072	34.450	ng/ul	0.00
54) 4-Nitrophenol-d4	14.810	143	464979	29.713	ng/ul	0.00
60) Fluorene-d10	15.616	176	2310663	35.260	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.728	200	354943	27.079	ng/ul	0.00
73) Anthracene-d10	17.469	188	3559189	35.670	ng/ul	0.00
81) Pyrene-d10	19.757	212	3794495	41.627	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.839	264	2649905	36.856	ng/ul	0.00


Target Compounds					Qvalue	
17) N-Nitroso-di-n-propyla...	8.693	70	22595	1.006	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039002.D
Acq On : 13 Mar 2023 22:42
Operator : CG/JU
Sample : PB151312BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK312


Quant Time: Mar 14 01:44:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 13 16:25:27 2023
Response via : Initial Calibration

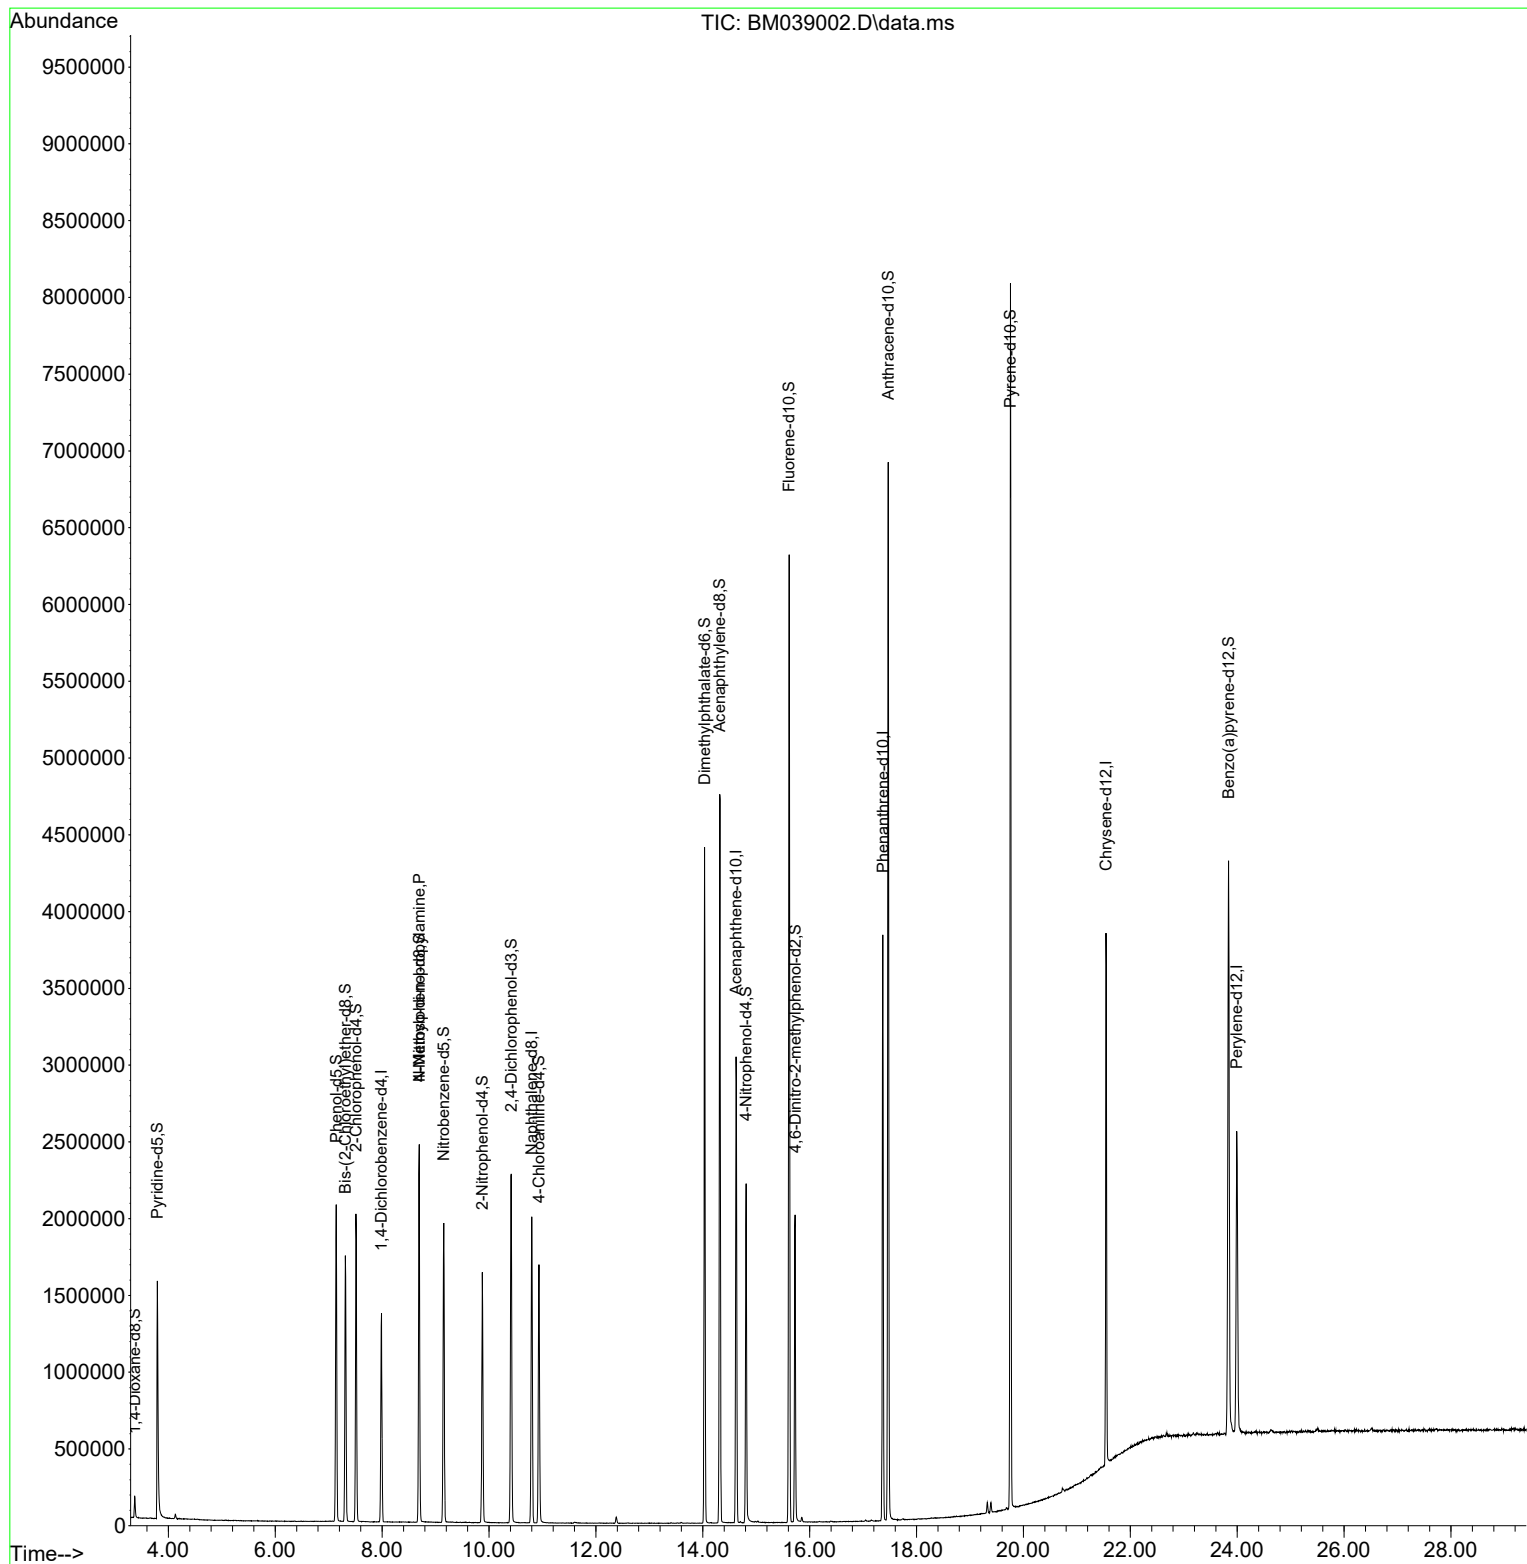

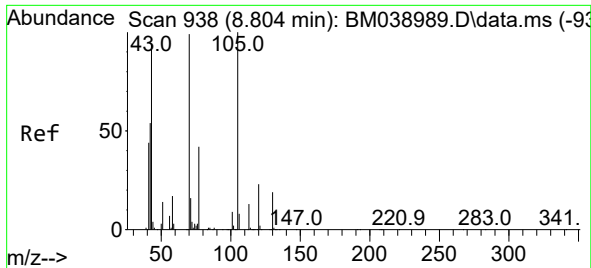

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.006 ng/ul
 RT: 8.693 min Scan# 91
 Delta R.T. -0.111 min
 Lab File: BM039002.D
 Acq: 13 Mar 2023 22:42

Instrument :
 BNA_M
 ClientSampleId :
 SBLK312

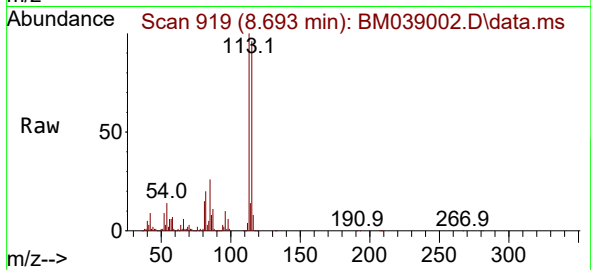

Tgt Ion: 70 Resp: 22595
 Ion Ratio Lower Upper
 70 100
 42 356.0 44.7 67.1#
 101 0.0 7.3 10.9#
 130 0.0 15.5 23.3#

