

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
 Data File : BM038993.D
 Acq On : 13 Mar 2023 17:00
 Operator : CG/JU
 Sample : PB151296BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK296

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038993.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	23	rVB	102559	147572	1.92%	0.180%
2	3.793	83	86	108	rBV	961723	1493803	19.45%	1.820%
3	4.128	140	143	149	rVB	25570	36805	0.48%	0.045%
4	7.139	648	655	667	rBV	1387596	2094052	27.26%	2.552%
5	7.310	678	684	695	rBV	1140723	1795945	23.38%	2.189%
6	7.516	711	719	729	rBV	1308604	2084341	27.14%	2.540%
7	7.986	791	799	806	rBV	1214934	1885699	24.55%	2.298%
8	8.692	912	919	931	rBV	1653456	2581914	33.61%	3.146%
9	9.151	989	997	1005	rBV	1326023	2116563	27.56%	2.579%
10	9.875	1112	1120	1129	rBV	1032421	1693348	22.05%	2.064%
11	10.416	1203	1212	1221	rBV	1558000	2526341	32.89%	3.079%
12	10.798	1269	1277	1286	rVB	1768408	2881254	37.51%	3.511%
13	10.933	1293	1300	1311	rBV	870894	1463018	19.05%	1.783%
14	12.380	1539	1546	1554	rVB2	27362	46768	0.61%	0.057%
15	14.033	1820	1827	1840	rBV	3071112	3971258	51.70%	4.840%
16	14.321	1868	1876	1886	rBV	3234417	4752275	61.87%	5.791%
17	14.627	1920	1928	1935	rBV	2697108	3994949	52.01%	4.868%
18	14.810	1952	1959	1974	rBV	1511368	2159079	28.11%	2.631%
19	15.615	2089	2096	2104	rBV	4321612	6000836	78.12%	7.313%
20	15.727	2108	2115	2128	rVV	1296258	1757290	22.88%	2.142%
21	15.851	2132	2136	2141	rVB2	17279	26332	0.34%	0.032%
22	17.045	2336	2339	2343	rBV6	4866	7999	0.10%	0.010%
23	17.368	2387	2394	2401	rBV	3545399	4846402	63.09%	5.906%
24	17.468	2404	2411	2429	rVV	4819773	6646376	86.53%	8.100%
25	17.751	2454	2459	2462	rBV5	5887	10559	0.14%	0.013%
26	19.321	2723	2726	2733	rVB	49059	70112	0.91%	0.085%
27	19.392	2734	2738	2741	rBV2	53187	69086	0.90%	0.084%
28	19.756	2794	2800	2810	rBV	5753934	7681138	100.00%	9.361%
29	21.550	3100	3105	3112	rBV	4060126	5133140	66.83%	6.255%
30	23.838	3487	3494	3503	rBV2	3724824	6999674	91.13%	8.530%
31	23.997	3514	3521	3533	rVB2	2575491	5084514	66.19%	6.196%




Sum of corrected areas: 82058442

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM038993.D
Acq On : 13 Mar 2023 17:00
Operator : CG/JU
Sample : PB151296BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK296

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

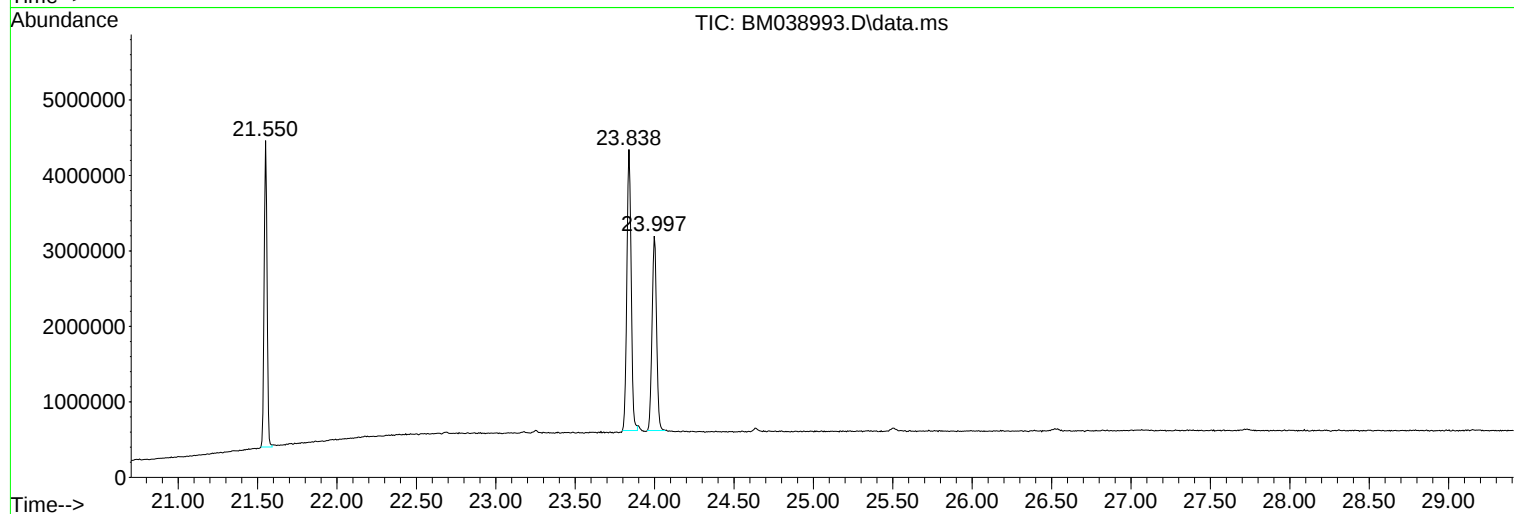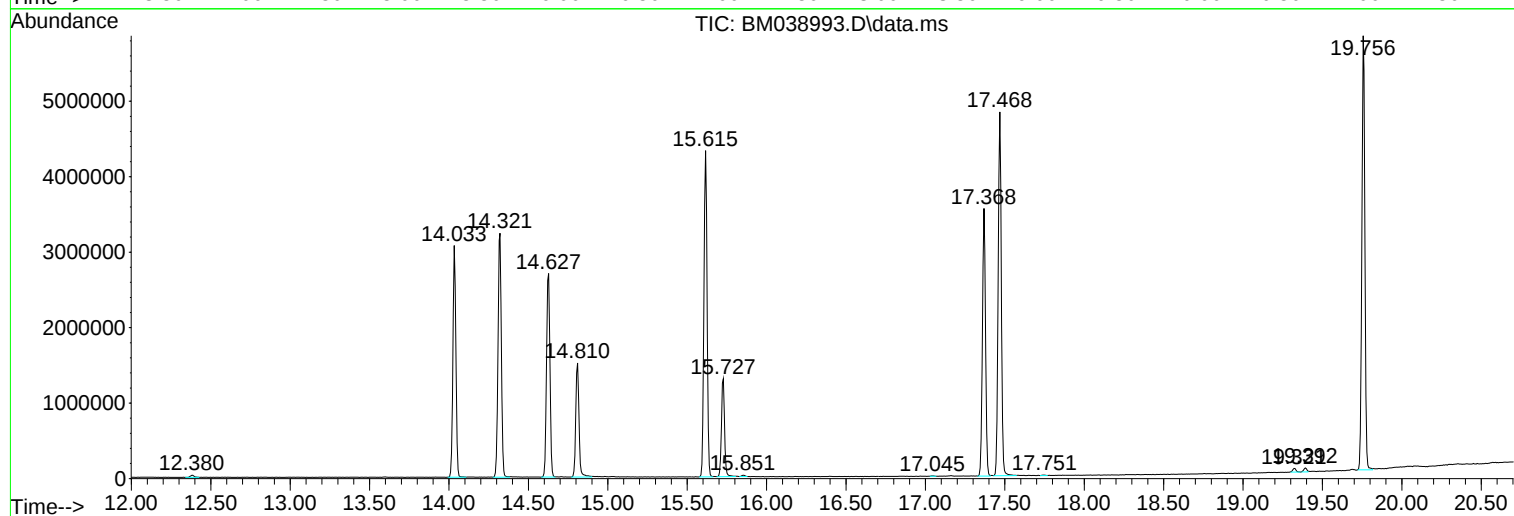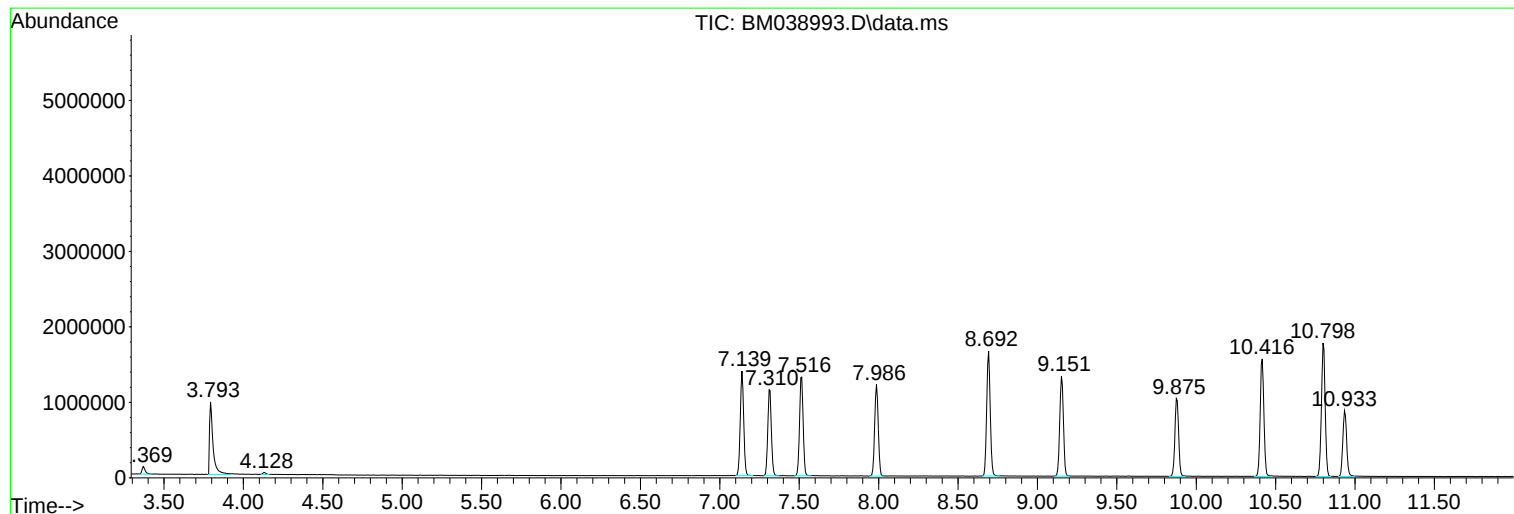

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM038993.D
Acq On : 13 Mar 2023 17:00
Operator : CG/JU
Sample : PB151296BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK296

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM038993.D
Acq On : 13 Mar 2023 17:00
Operator : CG/JU
Sample : PB151296BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK296

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc