

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
 Data File : BM038995.D
 Acq On : 13 Mar 2023 18:16
 Operator : CG/JU
 Sample : PB151297BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK297

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038995.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	10	15	24	rVB	124180	178699	1.86%	0.178%
2	3.793	84	86	106	rBV	1570762	2360419	24.51%	2.355%
3	4.134	140	144	151	rVB	29341	47087	0.49%	0.047%
4	7.140	648	655	665	rBV	1882662	2807541	29.15%	2.801%
5	7.316	678	685	698	rVB	1568467	2390120	24.82%	2.385%
6	7.516	712	719	729	rVB	1822751	2826001	29.34%	2.820%
7	7.987	787	799	807	rBV	1340668	2047809	21.26%	2.043%
8	8.693	911	919	928	rBV	2225370	3441241	35.73%	3.434%
9	9.151	988	997	1007	rBV	1753022	2832354	29.41%	2.826%
10	9.875	1113	1120	1128	rBV	1378996	2269936	23.57%	2.265%
11	10.416	1204	1212	1225	rBV	2090249	3398528	35.28%	3.391%
12	10.798	1269	1277	1288	rVB	1846441	3069865	31.87%	3.063%
13	10.934	1293	1300	1317	rBV	2162642	3585244	37.22%	3.577%
14	12.386	1540	1547	1552	rBV	37353	58377	0.61%	0.058%
15	13.598	1749	1753	1760	rVB6	6795	11660	0.12%	0.012%
16	14.033	1821	1827	1840	rVB	3983210	5327735	55.31%	5.316%
17	14.322	1868	1876	1888	rBV	4280325	6214474	64.52%	6.201%
18	14.627	1919	1928	1936	rBV	2796665	4132089	42.90%	4.123%
19	14.810	1952	1959	1978	rBV	1963405	2791786	28.99%	2.786%
20	15.039	1993	1998	2000	rBV6	9131	11709	0.12%	0.012%
21	15.616	2089	2096	2103	rBV	5583409	7699469	79.94%	7.683%
22	15.727	2108	2115	2130	rVV	1872915	2484331	25.79%	2.479%
23	15.857	2132	2137	2141	rVB2	22968	36149	0.38%	0.036%
24	17.368	2388	2394	2404	rBV	3550975	4824192	50.09%	4.814%
25	17.468	2404	2411	2424	rBV	6447234	8602074	89.31%	8.583%
26	19.321	2722	2726	2731	rVB2	62608	83633	0.87%	0.083%
27	19.392	2734	2738	2745	rVV	62209	86043	0.89%	0.086%
28	19.757	2794	2800	2812	rBV	7288470	9631740	100.00%	9.611%
29	21.551	3100	3105	3116	rBV	3703729	4714353	48.95%	4.704%
30	23.839	3487	3494	3510	rVB2	4135076	7991957	82.98%	7.974%
31	23.997	3514	3521	3533	rVB2	2116271	4263387	44.26%	4.254%




Sum of corrected areas: 100220002

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM038995.D
Acq On : 13 Mar 2023 18:16
Operator : CG/JU
Sample : PB151297BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK297

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

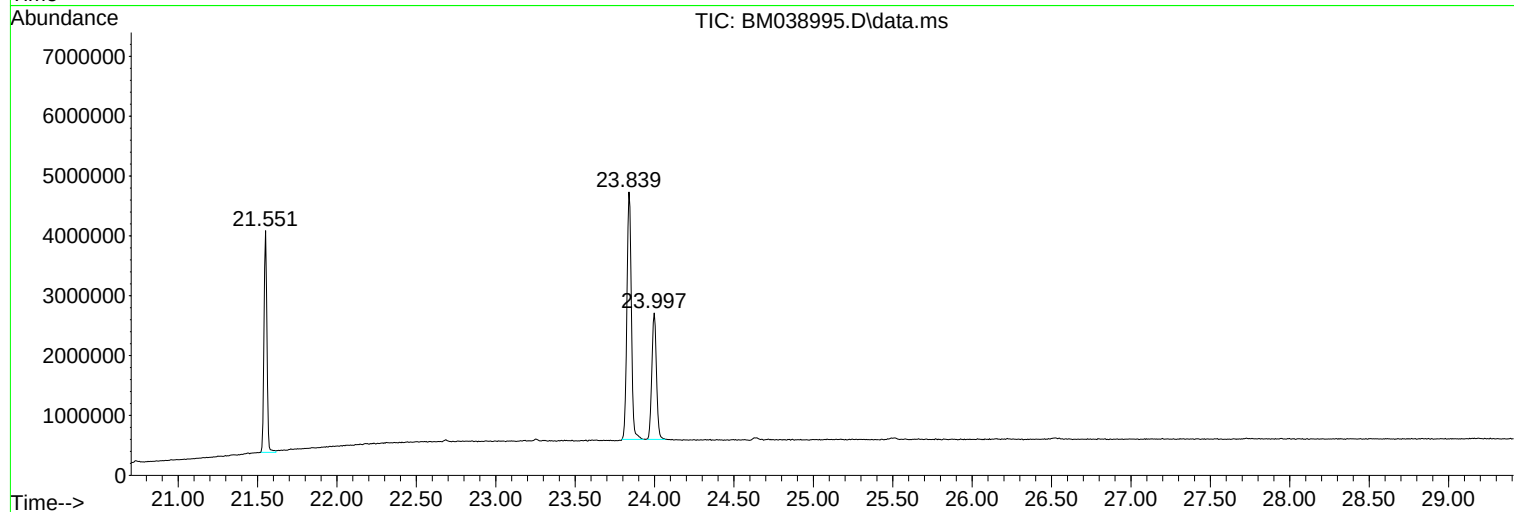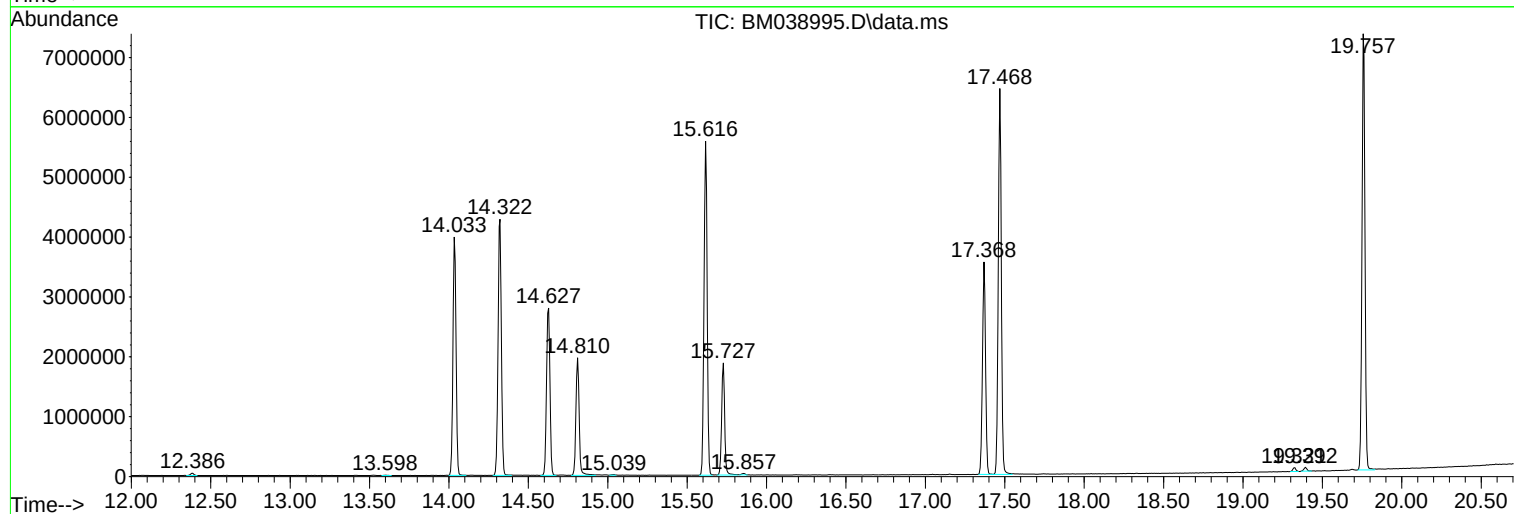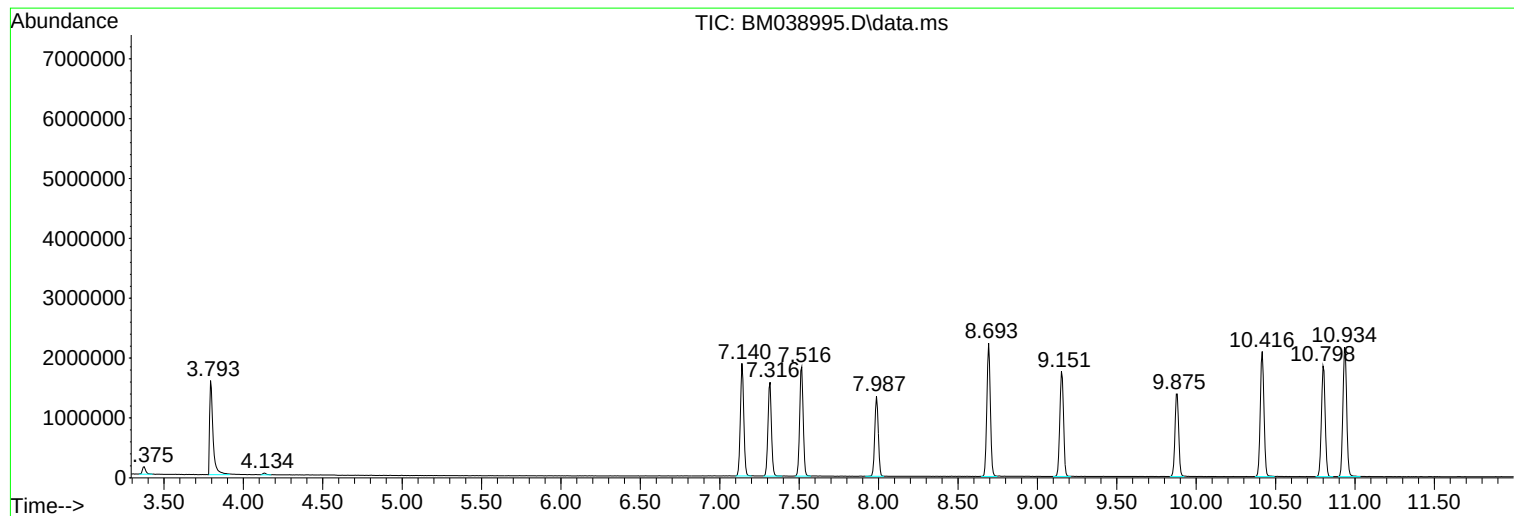

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM038995.D
Acq On : 13 Mar 2023 18:16
Operator : CG/JU
Sample : PB151297BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK297

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM038995.D
Acq On : 13 Mar 2023 18:16
Operator : CG/JU
Sample : PB151297BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK297

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc