

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
 Data File : BM039000.D
 Acq On : 13 Mar 2023 21:26
 Operator : CG/JU
 Sample : 01804-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039000.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	21	rVB	74594	108172	1.12%	0.125%
2	3.799	84	87	109	rBV	333028	527506	5.46%	0.611%
3	4.034	122	127	133	rVB2	37125	58448	0.60%	0.068%
4	4.128	139	143	151	rVB	29064	42728	0.44%	0.049%
5	4.234	156	161	167	rVB5	23819	37648	0.39%	0.044%
6	5.063	298	302	310	rVB4	19158	37061	0.38%	0.043%
7	6.363	519	523	527	rVB3	18077	28430	0.29%	0.033%
8	7.140	648	655	664	rVB	261219	414535	4.29%	0.480%
9	7.310	677	684	693	rVB	1372153	2060695	21.32%	2.386%
10	7.510	711	718	726	rBV	1113976	1718125	17.77%	1.989%
11	7.610	730	735	738	rVB6	6894	10507	0.11%	0.012%
12	7.987	792	799	806	rBV	1342474	2083018	21.55%	2.412%
13	8.692	912	919	929	rBV	798277	1265646	13.09%	1.465%
14	9.151	989	997	1006	rBV	1547739	2480077	25.65%	2.872%
15	9.569	1063	1068	1074	rBV3	9012	14570	0.15%	0.017%
16	9.875	1112	1120	1129	rBV	1151672	1854072	19.18%	2.147%
17	10.410	1203	1211	1227	rBV	1554877	2581754	26.70%	2.989%
18	10.798	1269	1277	1290	rBV	1909175	3173661	32.83%	3.675%
19	10.933	1293	1300	1317	rVV	1431916	2369009	24.50%	2.743%
20	11.604	1406	1414	1418	rBV10	7675	21166	0.22%	0.025%
21	12.380	1540	1546	1552	rBV	32480	51114	0.53%	0.059%
22	13.516	1734	1739	1744	rVB2	12891	20950	0.22%	0.024%
23	13.592	1748	1752	1757	rBV5	5590	9756	0.10%	0.011%
24	14.033	1820	1827	1837	rBV	3672932	4849795	50.16%	5.616%
25	14.316	1868	1875	1887	rBV	3826105	5512543	57.02%	6.383%
26	14.621	1920	1927	1935	rBV	2966745	4341913	44.91%	5.027%
27	14.698	1935	1940	1947	rVB10	8756	18136	0.19%	0.021%
28	14.804	1952	1958	1971	rBV	223082	360426	3.73%	0.417%
29	15.033	1992	1997	2002	rVB4	16567	26047	0.27%	0.030%
30	15.616	2089	2096	2103	rBV	5264833	7398077	76.52%	8.566%
31	15.727	2108	2115	2129	rVV	1648627	2310342	23.90%	2.675%
32	15.857	2132	2137	2148	rVB3	27005	53764	0.56%	0.062%
33	16.398	2226	2229	2236	rVB9	5917	11157	0.12%	0.013%
34	17.051	2335	2340	2344	rBV8	6524	12452	0.13%	0.014%
35	17.368	2387	2394	2404	rBV	3722985	5122148	52.98%	5.931%
36	17.468	2404	2411	2424	rBV	6353438	8593478	88.89%	9.950%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
 Data File : BM039000.D
 Acq On : 13 Mar 2023 21:26
 Operator : CG/JU
 Sample : 01804-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
 Title : SVOA CALIBRATION

37	17.745	2454	2458	2460	rBV3	9546	9750	0.10%	0.011%
38	18.262	2542	2546	2550	rBV2	53019	81227	0.84%	0.094%
39	19.321	2722	2726	2730	rBV2	66209	88535	0.92%	0.103%
40	19.392	2734	2738	2745	rVB	64882	93761	0.97%	0.109%
41	19.533	2759	2762	2768	rBV3	52223	76488	0.79%	0.089%
42	19.756	2794	2800	2813	rBV	7295905	9667717	100.00%	11.194%
43	21.550	3100	3105	3114	rBV	3824748	4823637	49.89%	5.585%
44	23.839	3487	3494	3509	rVB2	3871649	7615797	78.78%	8.818%
45	23.997	3514	3521	3533	rVB2	2142511	4328487	44.77%	5.012%




Sum of corrected areas: 86364325

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039000.D
Acq On : 13 Mar 2023 21:26
Operator : CG/JU
Sample : 01804-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

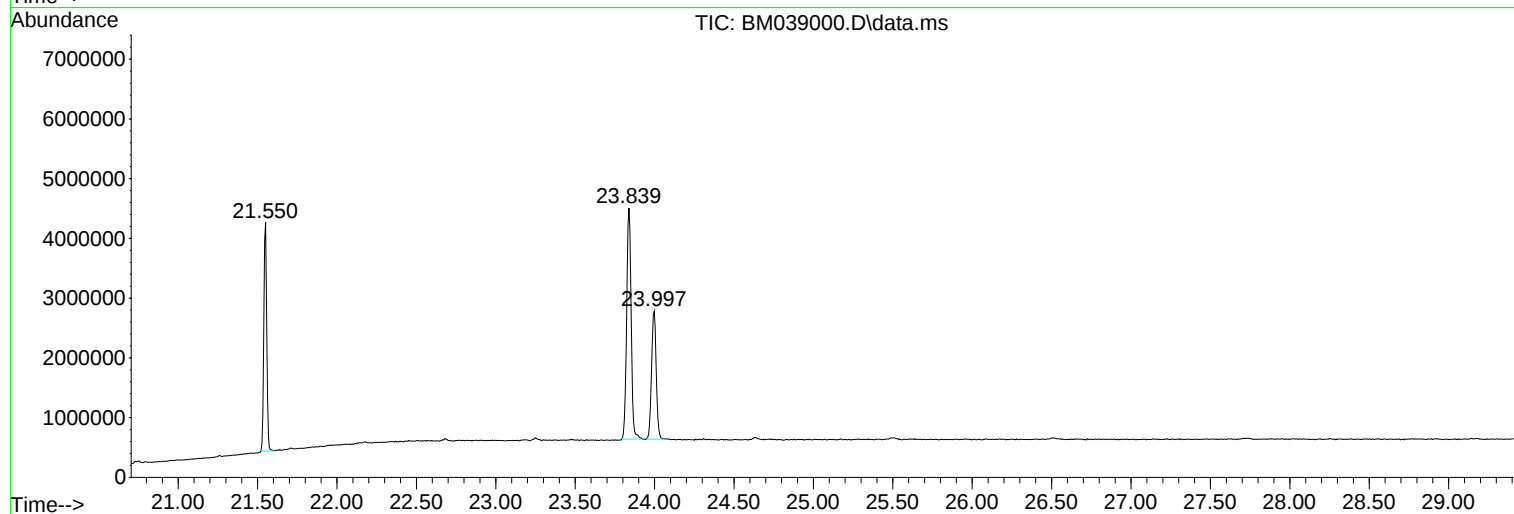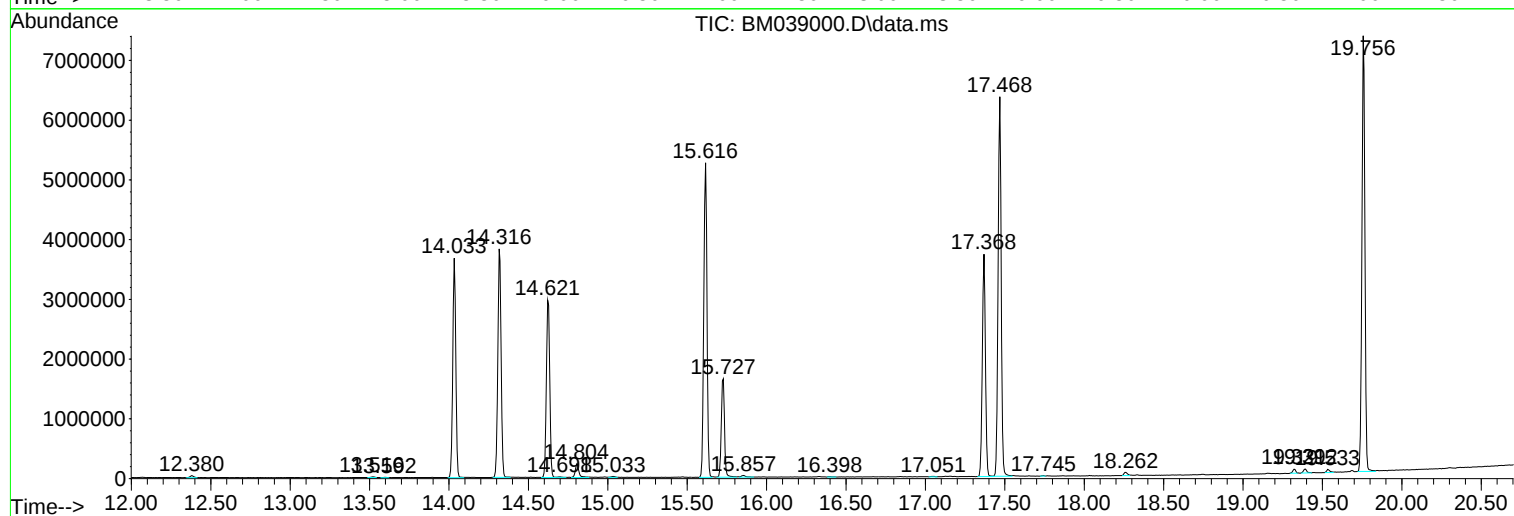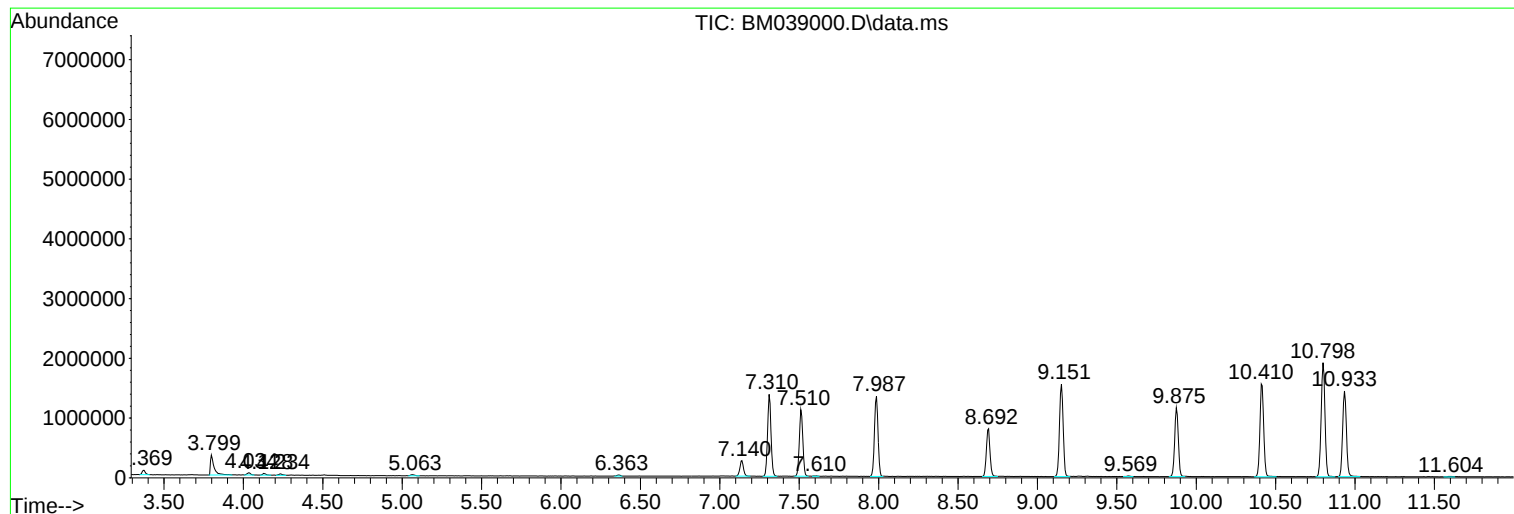

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039000.D
Acq On : 13 Mar 2023 21:26
Operator : CG/JU
Sample : 01804-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039000.D
Acq On : 13 Mar 2023 21:26
Operator : CG/JU
Sample : 01804-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc