

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
 Data File : BM039002.D
 Acq On : 13 Mar 2023 22:42
 Operator : CG/JU
 Sample : PB151312BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK312

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039002.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	10	14	25	rVB	143723	197051	1.97%	0.188%
2	3.793	83	86	106	rBV	1548711	2257134	22.57%	2.152%
3	4.128	140	143	150	rVB	30896	44539	0.45%	0.042%
4	7.140	647	655	666	rBV	2062476	3100639	31.01%	2.956%
5	7.310	677	684	696	rVB	1731111	2643363	26.43%	2.520%
6	7.510	711	718	731	rBV	2003790	3086583	30.87%	2.943%
7	7.987	792	799	806	rVB	1360348	2100567	21.01%	2.003%
8	8.693	911	919	928	rBV	2460232	3843907	38.44%	3.665%
9	9.152	988	997	1005	rBV	1950522	3141365	31.41%	2.995%
10	9.875	1112	1120	1133	rBV	1629867	2541482	25.41%	2.423%
11	10.416	1202	1212	1228	rBV	2273067	3790958	37.91%	3.614%
12	10.798	1269	1277	1286	rVB	1993446	3201743	32.02%	3.052%
13	10.934	1293	1300	1316	rBV	1682127	2720768	27.21%	2.594%
14	11.598	1405	1413	1415	rBV7	6602	11285	0.11%	0.011%
15	12.381	1539	1546	1554	rBV2	40654	70505	0.71%	0.067%
16	14.034	1820	1827	1839	rBV	4402572	5830934	58.31%	5.559%
17	14.316	1868	1875	1890	rBV	4743755	6967272	69.67%	6.642%
18	14.622	1921	1927	1934	rBV	3035306	4399066	43.99%	4.194%
19	14.704	1938	1941	1946	rVB7	7829	10876	0.11%	0.010%
20	14.810	1952	1959	1975	rBV	2208516	3077629	30.78%	2.934%
21	15.034	1993	1997	2002	rVB6	8297	11596	0.12%	0.011%
22	15.616	2089	2096	2104	rBV	6302689	8646864	86.47%	8.244%
23	15.728	2108	2115	2126	rBV	1998578	2679796	26.80%	2.555%
24	15.851	2131	2136	2143	rVB2	29749	52079	0.52%	0.050%
25	16.398	2224	2229	2233	rBV7	7752	14185	0.14%	0.014%
26	17.045	2334	2339	2342	rBV5	9821	15668	0.16%	0.015%
27	17.151	2354	2357	2364	rVB6	7225	12876	0.13%	0.012%
28	17.369	2387	2394	2404	rBV	3816236	5120240	51.20%	4.881%
29	17.469	2404	2411	2427	rVV	6890266	9283862	92.84%	8.851%
30	19.321	2722	2726	2732	rBV2	69591	94424	0.94%	0.090%
31	19.392	2734	2738	2743	rBV	65883	95580	0.96%	0.091%
32	19.757	2794	2800	2810	rBV	7979839	10000198	100.00%	9.534%
33	21.545	3099	3104	3116	rBV	3467839	4617954	46.18%	4.403%
34	23.839	3486	3494	3509	rBV	3724056	7357292	73.57%	7.014%
35	23.992	3514	3520	3531	rVB2	1949798	3851695	38.52%	3.672%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039002.D
Acq On : 13 Mar 2023 22:42
Operator : CG/JU
Sample : PB151312BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK312

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Title : SVOA CALIBRATION




Sum of corrected areas: 104891975

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039002.D
Acq On : 13 Mar 2023 22:42
Operator : CG/JU
Sample : PB151312BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK312

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

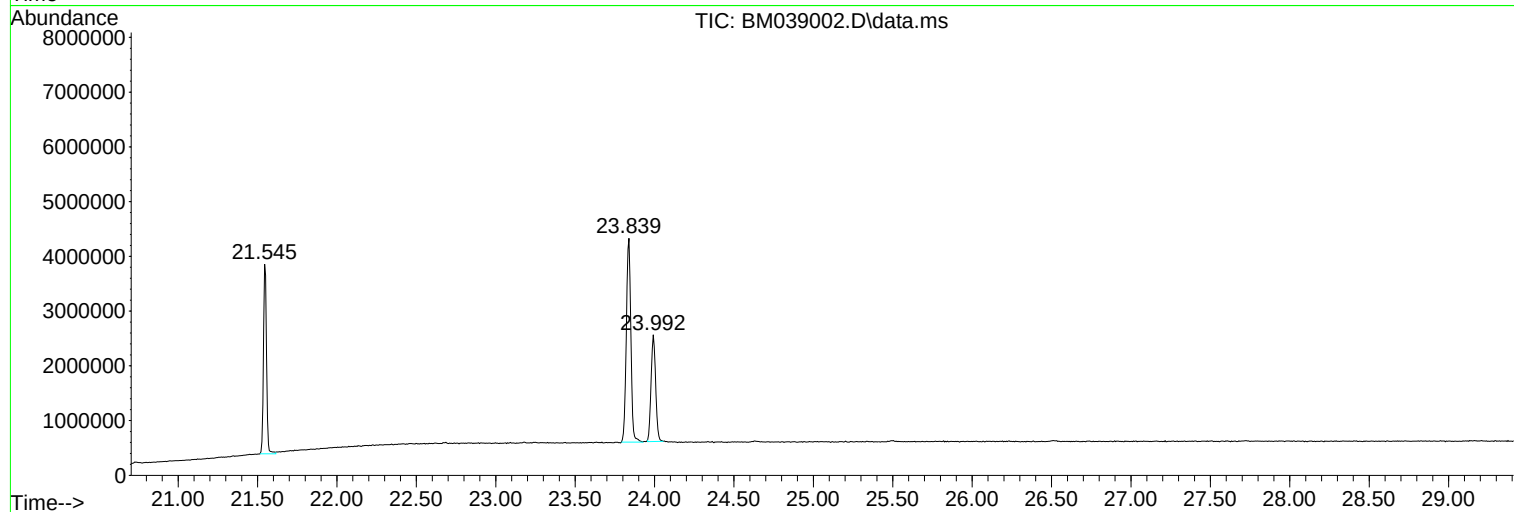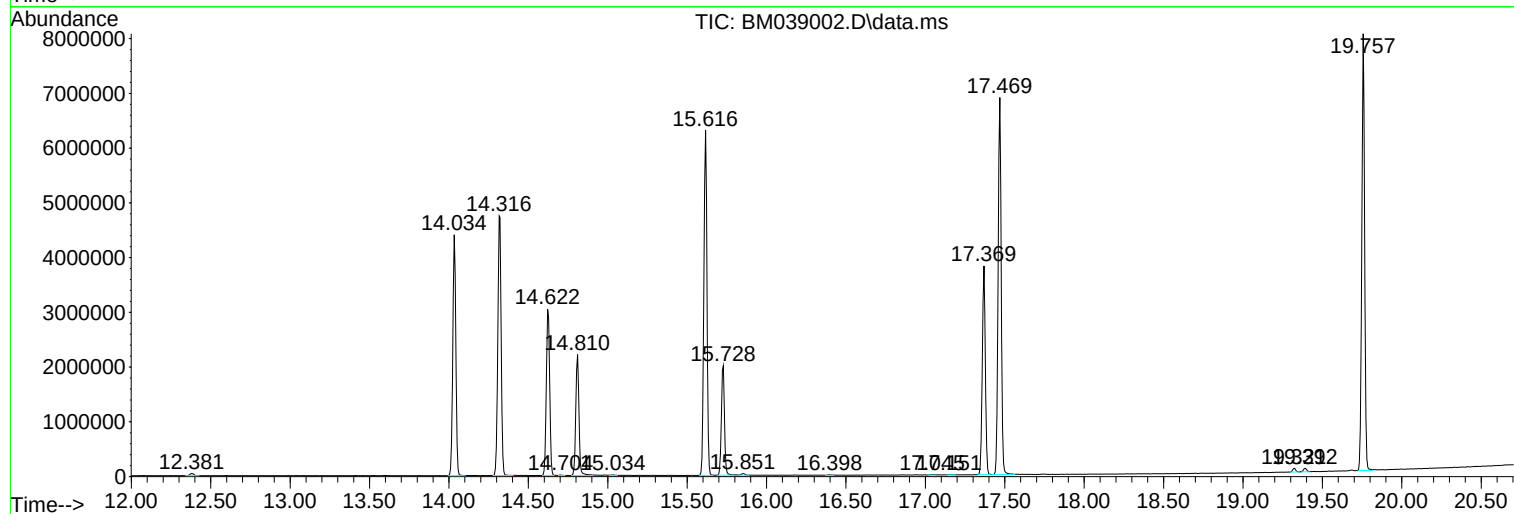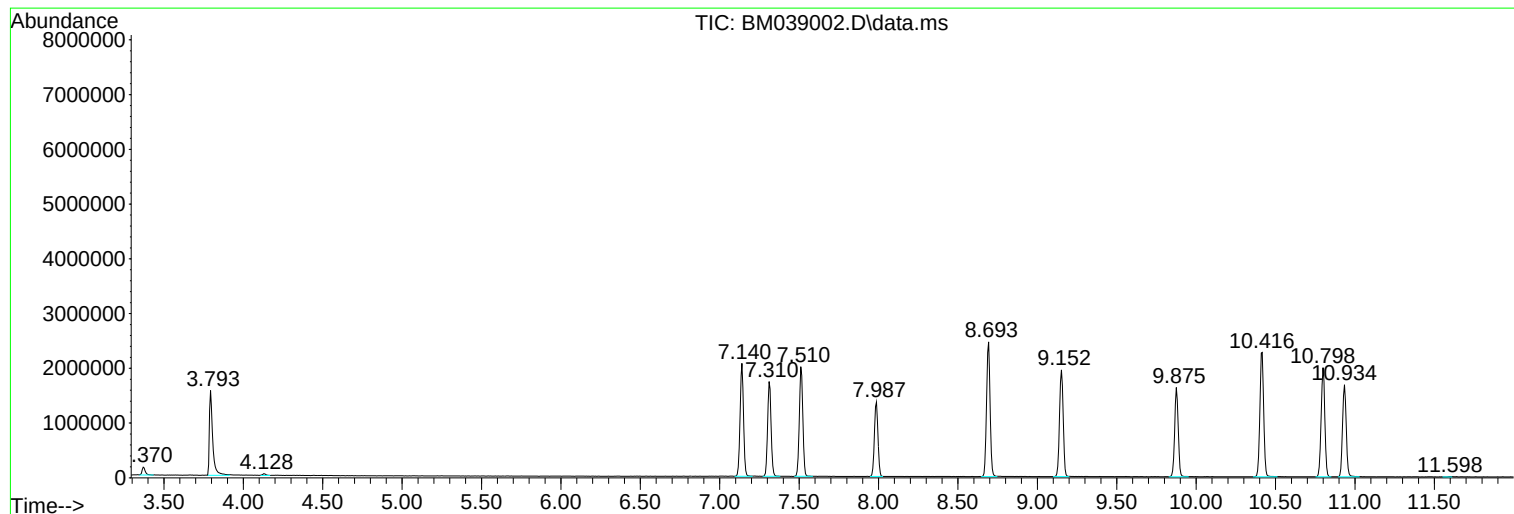

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039002.D
Acq On : 13 Mar 2023 22:42
Operator : CG/JU
Sample : PB151312BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK312

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039002.D
Acq On : 13 Mar 2023 22:42
Operator : CG/JU
Sample : PB151312BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK312

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc