

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
 Data File : BM039003.D
 Acq On : 13 Mar 2023 23:20
 Operator : CG/JU
 Sample : PB151314BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK314

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039003.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	22	rVB	133485	181583	1.84%	0.175%
2	3.793	82	86	112	rBV	1702408	2563923	25.98%	2.466%
3	4.128	140	143	149	rVB	29075	40116	0.41%	0.039%
4	7.140	647	655	666	rBV	1908969	2909290	29.48%	2.798%
5	7.310	677	684	696	rBV	1629846	2471894	25.05%	2.377%
6	7.510	711	718	726	rBV	1913589	2920026	29.59%	2.808%
7	7.987	791	799	807	rBV	1399603	2176038	22.05%	2.093%
8	8.692	911	919	931	rBV	2250159	3557170	36.05%	3.421%
9	9.151	989	997	1007	rBV	1839902	2903346	29.42%	2.792%
10	9.875	1109	1120	1131	rBV	1481102	2349361	23.81%	2.260%
11	10.410	1204	1211	1225	rBV	2152993	3525962	35.73%	3.391%
12	10.798	1269	1277	1287	rVB	2063428	3292509	33.37%	3.167%
13	10.934	1291	1300	1314	rBV	2347697	3850650	39.02%	3.704%
14	12.380	1540	1546	1556	rVB2	41126	65807	0.67%	0.063%
15	14.033	1820	1827	1838	rBV	4107492	5400910	54.74%	5.195%
16	14.316	1868	1875	1887	rBV2	4260869	6425921	65.12%	6.180%
17	14.622	1919	1927	1934	rBV	2993014	4506341	45.67%	4.334%
18	14.704	1937	1941	1946	rVB7	6667	10181	0.10%	0.010%
19	14.810	1952	1959	1977	rBV	2013945	2839733	28.78%	2.731%
20	15.033	1992	1997	2002	rVB9	8832	12357	0.13%	0.012%
21	15.616	2089	2096	2104	rBV	5752151	7912748	80.19%	7.610%
22	15.727	2108	2115	2130	rVV	1851667	2523830	25.58%	2.427%
23	15.851	2131	2136	2142	rVB	25957	44413	0.45%	0.043%
24	17.157	2353	2358	2360	rBV3	8130	11582	0.12%	0.011%
25	17.368	2387	2394	2404	rBV	3854957	5279845	53.51%	5.078%
26	17.468	2404	2411	2424	rBV	6243071	8638250	87.54%	8.308%
27	19.321	2722	2726	2731	rBV	71628	93062	0.94%	0.090%
28	19.392	2734	2738	2742	rVV2	65169	86086	0.87%	0.083%
29	19.756	2794	2800	2814	rBV	7826799	9867328	100.00%	9.490%
30	21.545	3099	3104	3114	rBV	3919432	5091289	51.60%	4.897%
31	23.839	3487	3494	3511	rVB2	4030125	7873171	79.79%	7.572%
32	23.991	3514	3520	3532	rVB2	2214089	4546833	46.08%	4.373%




Sum of corrected areas: 103971555

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039003.D
Acq On : 13 Mar 2023 23:20
Operator : CG/JU
Sample : PB151314BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK314

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

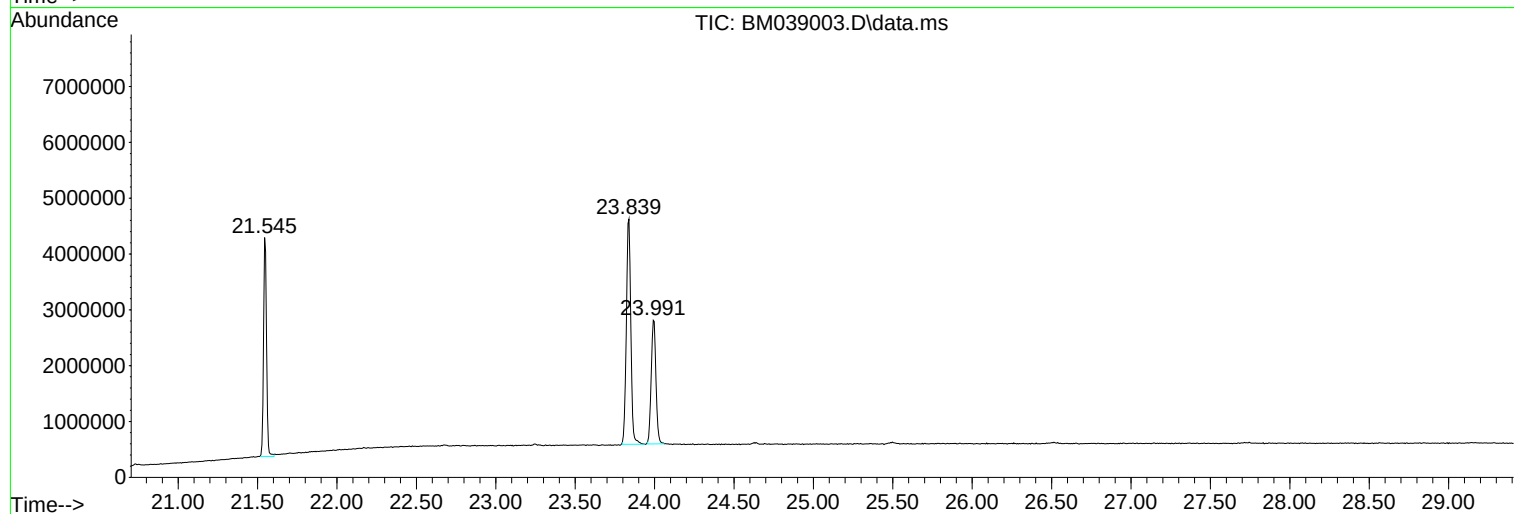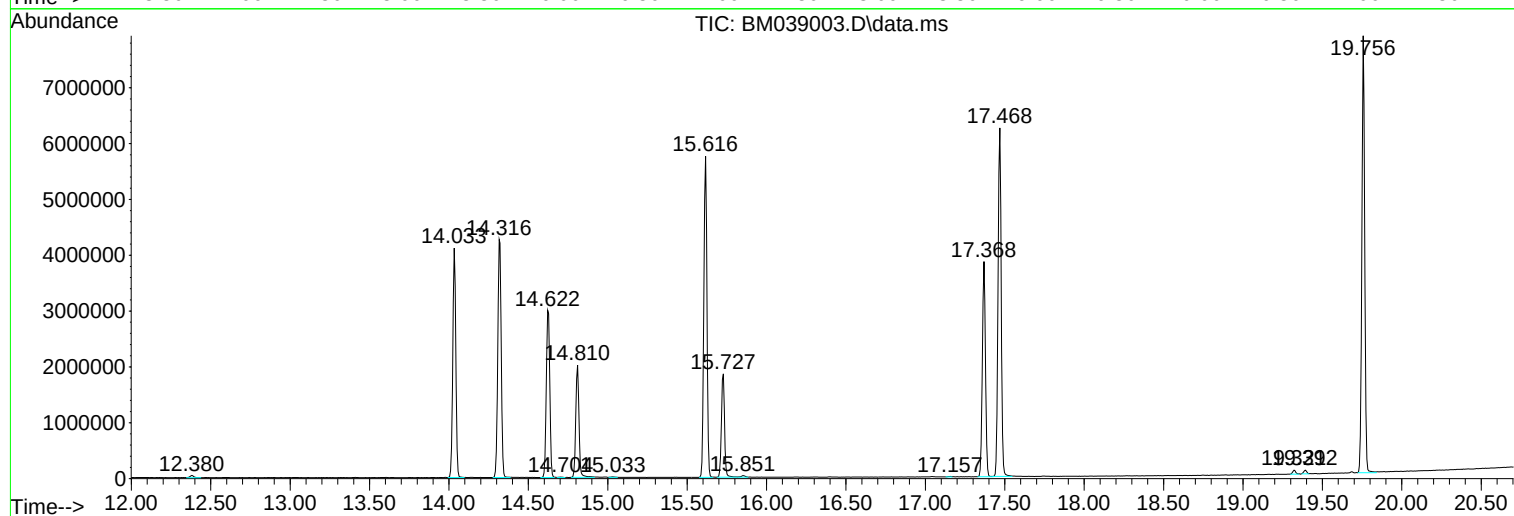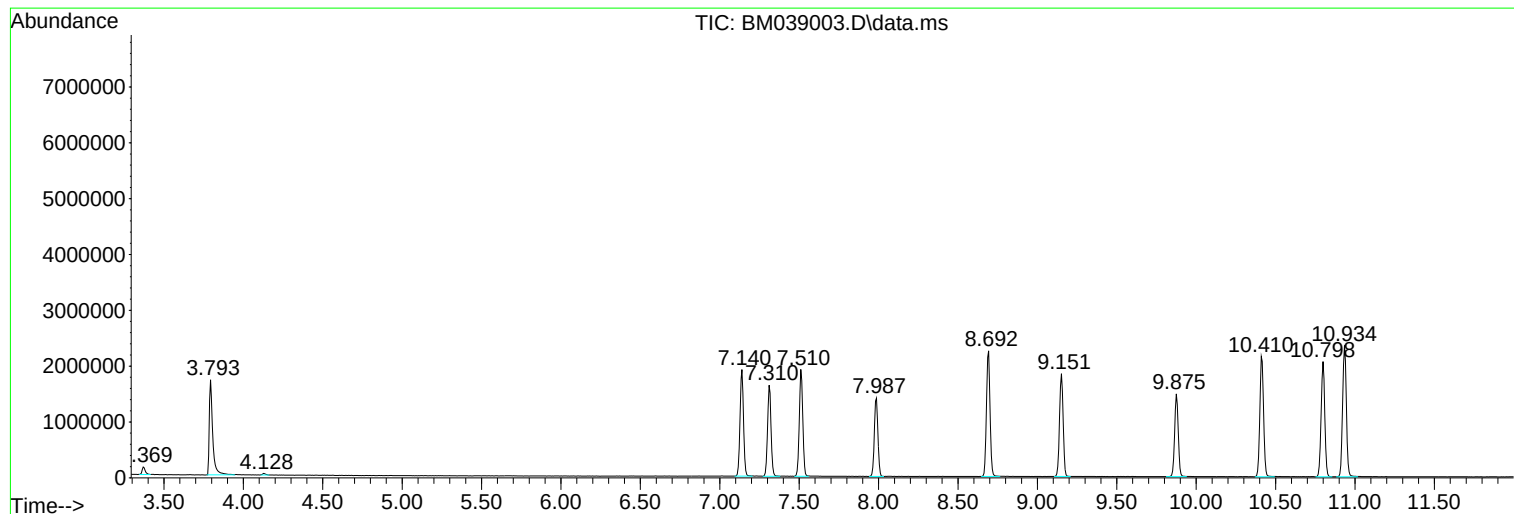

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039003.D
Acq On : 13 Mar 2023 23:20
Operator : CG/JU
Sample : PB151314BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK314

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039003.D
Acq On : 13 Mar 2023 23:20
Operator : CG/JU
Sample : PB151314BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK314

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc