

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
 Data File : BM039005.D
 Acq On : 14 Mar 2023 09:35
 Operator : CG/JU
 Sample : PB151314BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK314

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039005.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	21	rVB	181040	239075	1.69%	0.158%
2	3.793	82	86	113	rBV	2285285	3549482	25.13%	2.351%
3	4.128	139	143	148	rVB	38848	56780	0.40%	0.038%
4	7.134	647	654	665	rBV	2644772	4112767	29.12%	2.725%
5	7.310	677	684	695	rVB	2292945	3468259	24.55%	2.298%
6	7.510	710	718	728	rBV	2679887	4155960	29.42%	2.753%
7	7.981	791	798	806	rVB	1986957	3086988	21.85%	2.045%
8	8.687	910	918	932	rBV	3219996	5106098	36.15%	3.383%
9	9.151	988	997	1006	rBV	2668997	4225551	29.91%	2.799%
10	9.875	1111	1120	1134	rBV	2185370	3447891	24.41%	2.284%
11	10.410	1203	1211	1226	rBV	3160099	5080046	35.96%	3.365%
12	10.798	1268	1277	1286	rBV	2915735	4748514	33.62%	3.146%
13	10.933	1292	1300	1312	rBV	3352704	5547438	39.27%	3.675%
14	11.586	1407	1411	1421	rVB10	6775	15089	0.11%	0.010%
15	12.380	1540	1546	1551	rBV	56910	89789	0.64%	0.059%
16	13.598	1748	1753	1758	rVB6	8926	16764	0.12%	0.011%
17	14.033	1820	1827	1840	rVB	5776634	7877984	55.77%	5.219%
18	14.316	1868	1875	1884	rBV	6608079	9464691	67.00%	6.270%
19	14.621	1920	1927	1936	rBV	4503552	6597795	46.71%	4.371%
20	14.704	1937	1941	1946	rVB8	9783	14775	0.10%	0.010%
21	14.810	1952	1959	1974	rBV	2948017	4163755	29.48%	2.758%
22	15.033	1993	1997	2002	rVB7	13835	22133	0.16%	0.015%
23	15.521	2074	2080	2081	rBV4	14980	24788	0.18%	0.016%
24	15.615	2089	2096	2105	rVB	8407941	11638927	82.40%	7.711%
25	15.727	2109	2115	2126	rBV	3008194	3957163	28.01%	2.622%
26	15.851	2132	2136	2142	rVB2	39085	59935	0.42%	0.040%
27	16.398	2225	2229	2233	rBV4	10027	18292	0.13%	0.012%
28	16.839	2298	2304	2311	rBV3	34710	71999	0.51%	0.048%
29	17.045	2337	2339	2345	rVB6	13576	18284	0.13%	0.012%
30	17.215	2363	2368	2373	rBV2	21572	35404	0.25%	0.023%
31	17.368	2387	2394	2403	rBV	5686873	7696583	54.49%	5.099%
32	17.468	2404	2411	2430	rVV	9049176	12564218	88.95%	8.324%
33	17.745	2455	2458	2466	rVB6	13184	22828	0.16%	0.015%
34	17.921	2485	2488	2492	rVB2	32927	40630	0.29%	0.027%
35	18.262	2542	2546	2553	rBV4	27396	52513	0.37%	0.035%
36	18.868	2646	2649	2652	rBV3	28919	36945	0.26%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039005.D
Acq On : 14 Mar 2023 09:35
Operator : CG/JU
Sample : PB151314BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK314

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Title : SVOA CALIBRATION

37	19.327	2723	2727	2733	rVB2	104107	138963	0.98%	0.092%
38	19.392	2735	2738	2745	rVB	101558	148535	1.05%	0.098%
39	19.762	2795	2801	2811	rBV	10831776	14125537	100.00%	9.358%
40	21.556	3101	3106	3115	rBV	5663810	7349951	52.03%	4.869%
41	23.850	3488	3496	3511	rBV	5685290	11359066	80.42%	7.525%
42	24.009	3516	3523	3536	rVB2	3195242	6498306	46.00%	4.305%




Sum of corrected areas: 150946491

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039005.D
Acq On : 14 Mar 2023 09:35
Operator : CG/JU
Sample : PB151314BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK314

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

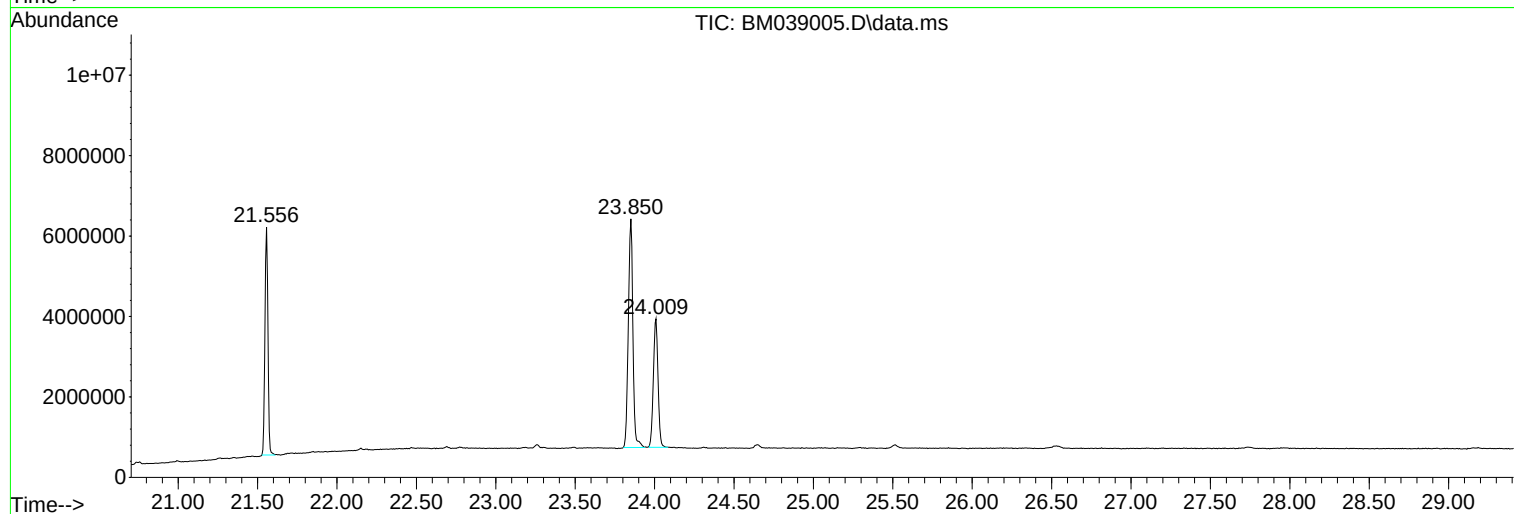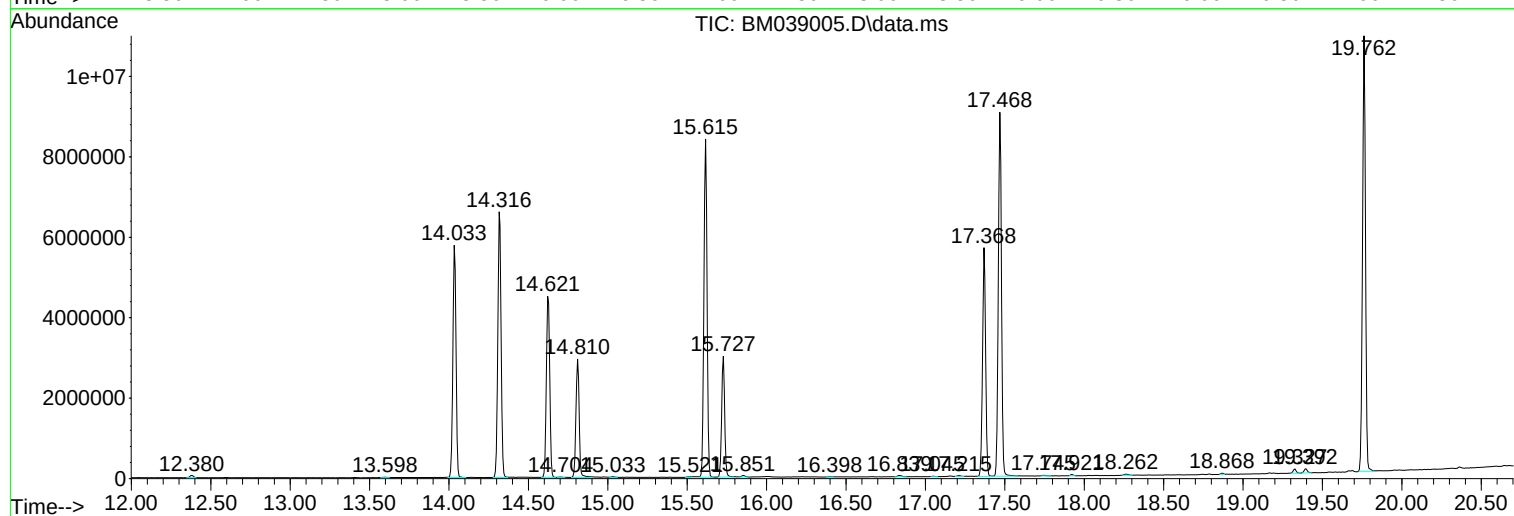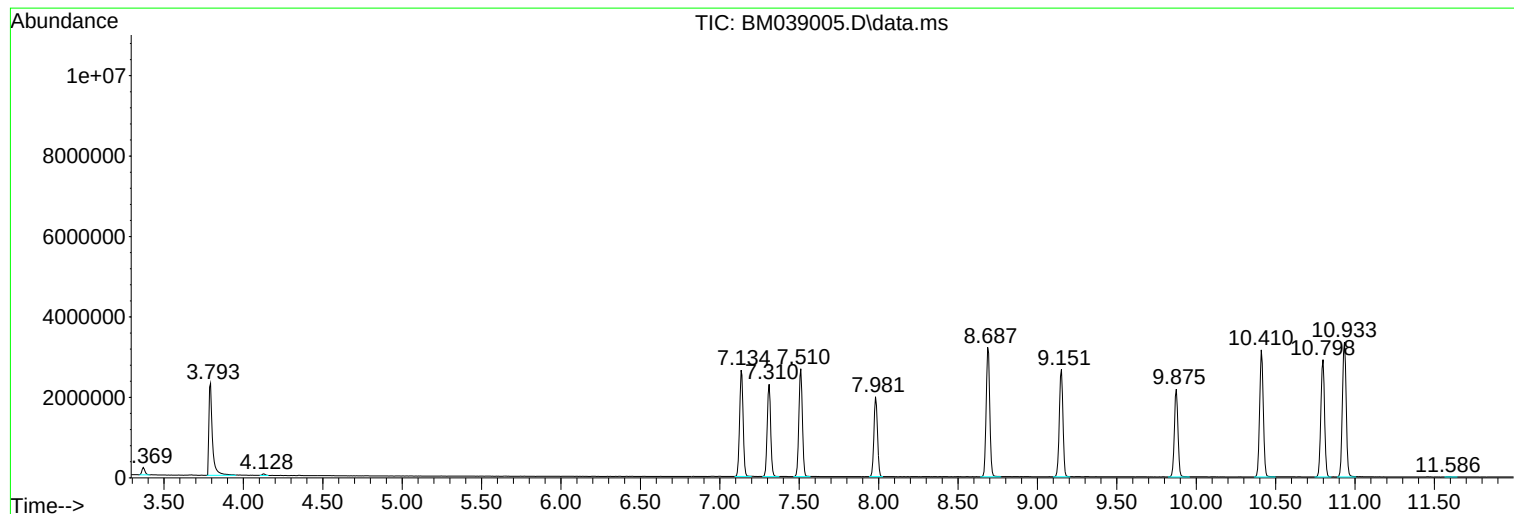

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039005.D
Acq On : 14 Mar 2023 09:35
Operator : CG/JU
Sample : PB151314BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK314

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039005.D
Acq On : 14 Mar 2023 09:35
Operator : CG/JU
Sample : PB151314BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK314

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc