

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
 Data File : BM039009.D
 Acq On : 14 Mar 2023 12:06
 Operator : CG/JU
 Sample : PB151312BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK312

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039009.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	10	14	23	rVB	169832	229220	1.88%	0.179%
2	3.793	83	86	109	rBV	1794358	2696035	22.08%	2.104%
3	4.128	140	143	150	rVB	32373	44866	0.37%	0.035%
4	7.140	648	655	663	rBV	2446568	3708233	30.38%	2.894%
5	7.310	676	684	693	rBV	2103640	3177742	26.03%	2.480%
6	7.510	711	718	731	rBV	2408657	3692806	30.25%	2.882%
7	7.987	791	799	808	rBV	1570633	2493457	20.43%	1.946%
8	8.692	911	919	934	rBV	2964795	4643292	38.04%	3.624%
9	9.151	989	997	1007	rBV	2379018	3788551	31.03%	2.957%
10	9.875	1110	1120	1134	rBV	1963789	3101333	25.40%	2.420%
11	10.410	1204	1211	1225	rBV	2784968	4545624	37.24%	3.548%
12	10.798	1269	1277	1285	rBV	2351074	3871281	31.71%	3.021%
13	10.933	1293	1300	1311	rBV	1981866	3243240	26.57%	2.531%
14	12.380	1541	1546	1553	rVB	48699	80847	0.66%	0.063%
15	14.033	1820	1827	1838	rBV	5207341	6987075	57.24%	5.453%
16	14.321	1868	1876	1886	rBV	5863879	8501960	69.64%	6.635%
17	14.621	1920	1927	1936	rBV	3598042	5361135	43.92%	4.184%
18	14.810	1952	1959	1978	rBV	2711933	3794185	31.08%	2.961%
19	15.033	1993	1997	2004	rVB5	11291	17189	0.14%	0.013%
20	15.615	2089	2096	2104	rBV	7655931	10544102	86.37%	8.229%
21	15.727	2108	2115	2129	rVV	2551968	3382318	27.71%	2.640%
22	15.851	2132	2136	2143	rVB2	34241	53820	0.44%	0.042%
23	16.398	2225	2229	2235	rBV8	8403	15078	0.12%	0.012%
24	17.051	2337	2340	2345	rVB6	8530	12484	0.10%	0.010%
25	17.368	2388	2394	2403	rBV	4557565	6187125	50.68%	4.829%
26	17.468	2404	2411	2428	rVV	8205879	11262163	92.25%	8.790%
27	17.745	2453	2458	2461	rBV5	10696	18696	0.15%	0.015%
28	19.327	2722	2727	2731	rBV2	78612	108081	0.89%	0.084%
29	19.392	2734	2738	2742	rBV	78805	105021	0.86%	0.082%
30	19.762	2795	2801	2811	rBV	9228703	12207670	100.00%	9.528%
31	21.550	3100	3105	3112	rBV	4512854	5662035	46.38%	4.419%
32	23.844	3487	3495	3512	rBV2	4884322	9578211	78.46%	7.475%
33	23.997	3515	3521	3533	rVB2	2492704	5015442	41.08%	3.914%




Sum of corrected areas: 128130317

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039009.D
Acq On : 14 Mar 2023 12:06
Operator : CG/JU
Sample : PB151312BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK312

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

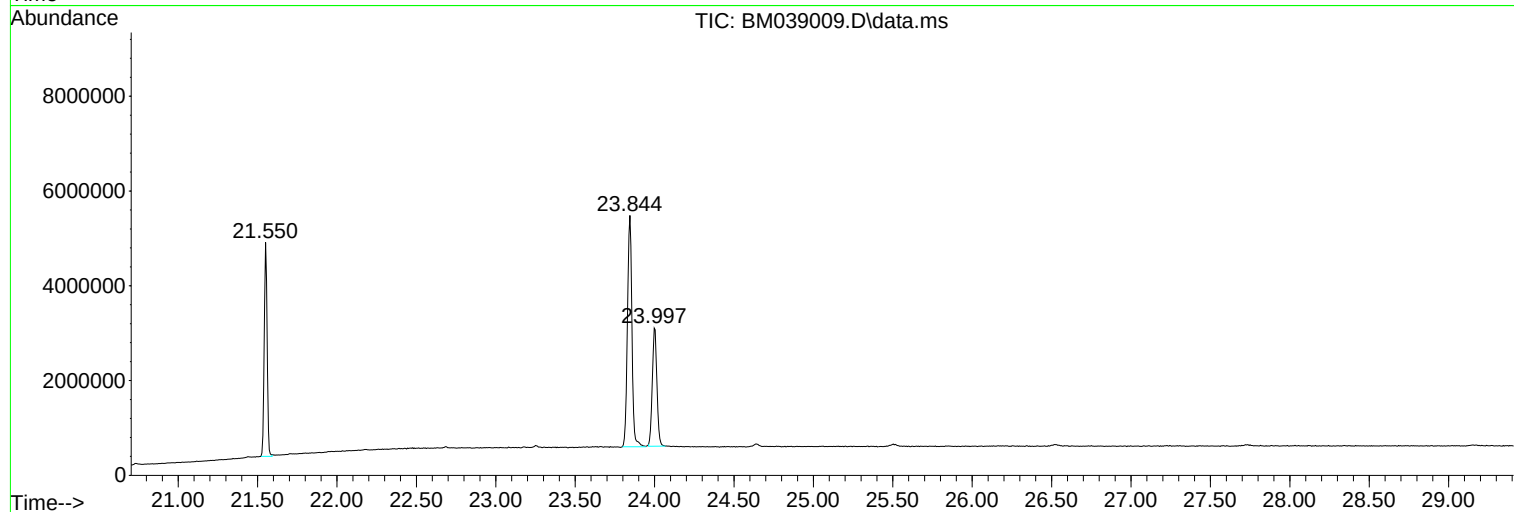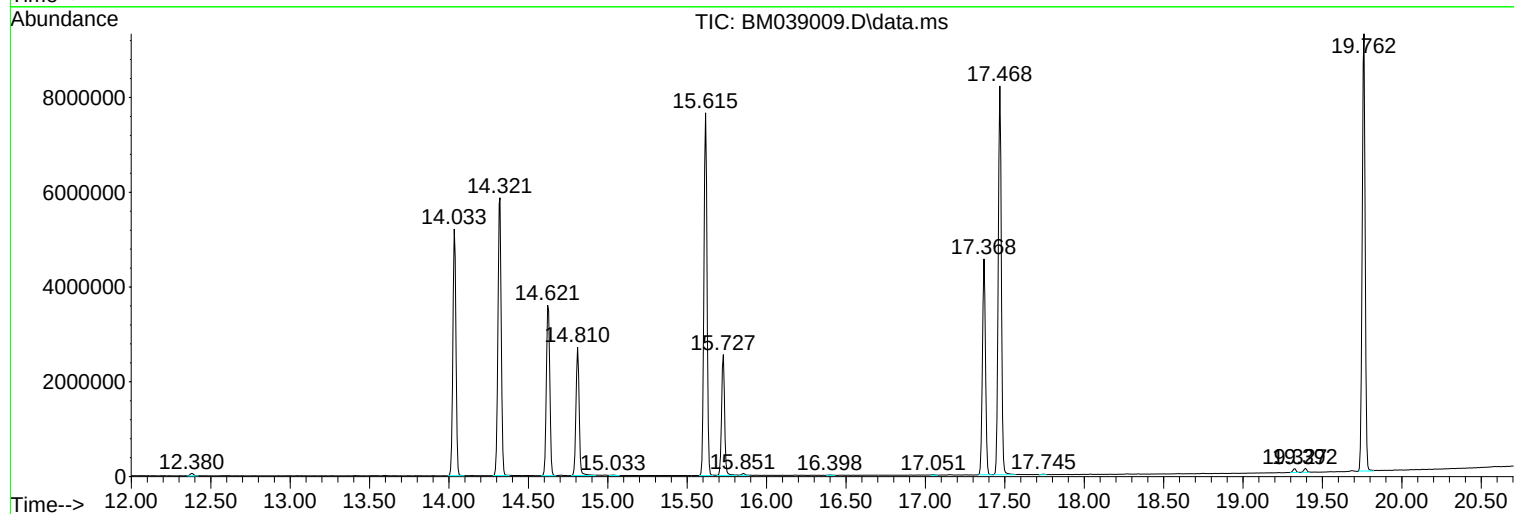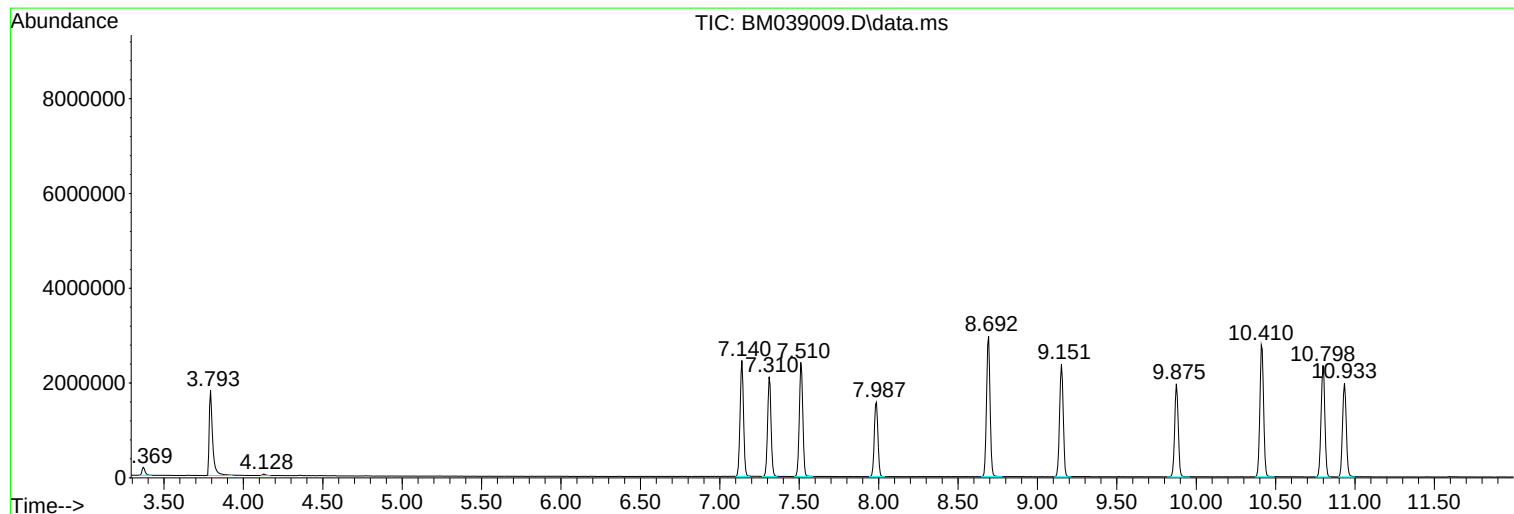

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039009.D
Acq On : 14 Mar 2023 12:06
Operator : CG/JU
Sample : PB151312BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK312

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031323\
Data File : BM039009.D
Acq On : 14 Mar 2023 12:06
Operator : CG/JU
Sample : PB151312BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK312

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc