
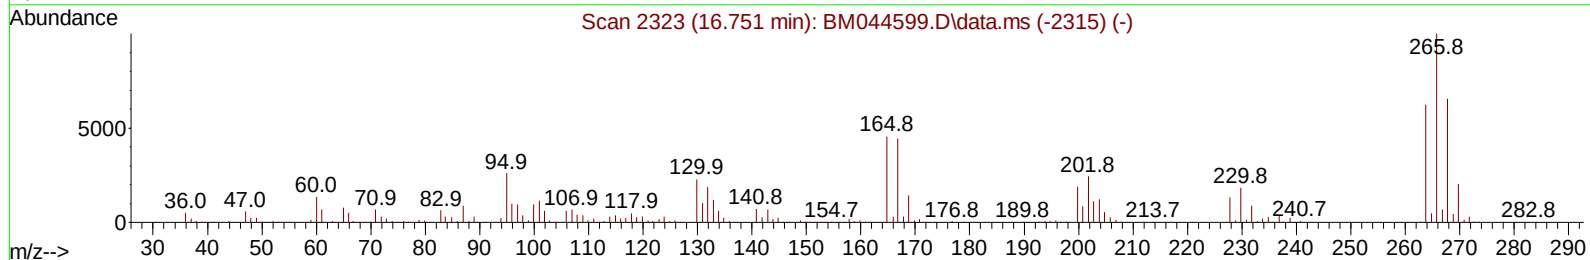
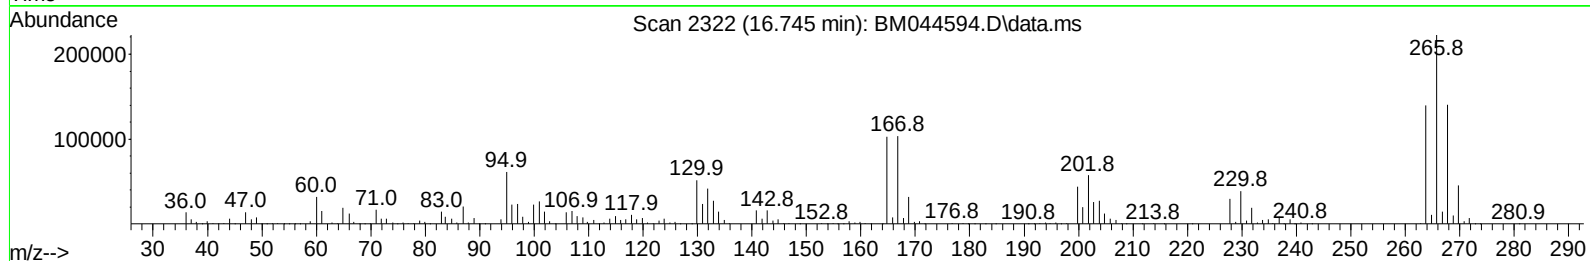


Quant Time: Mar 14 02:09:55 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031324.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 14 02:00:45 2024  
Response via : Initial Calibration

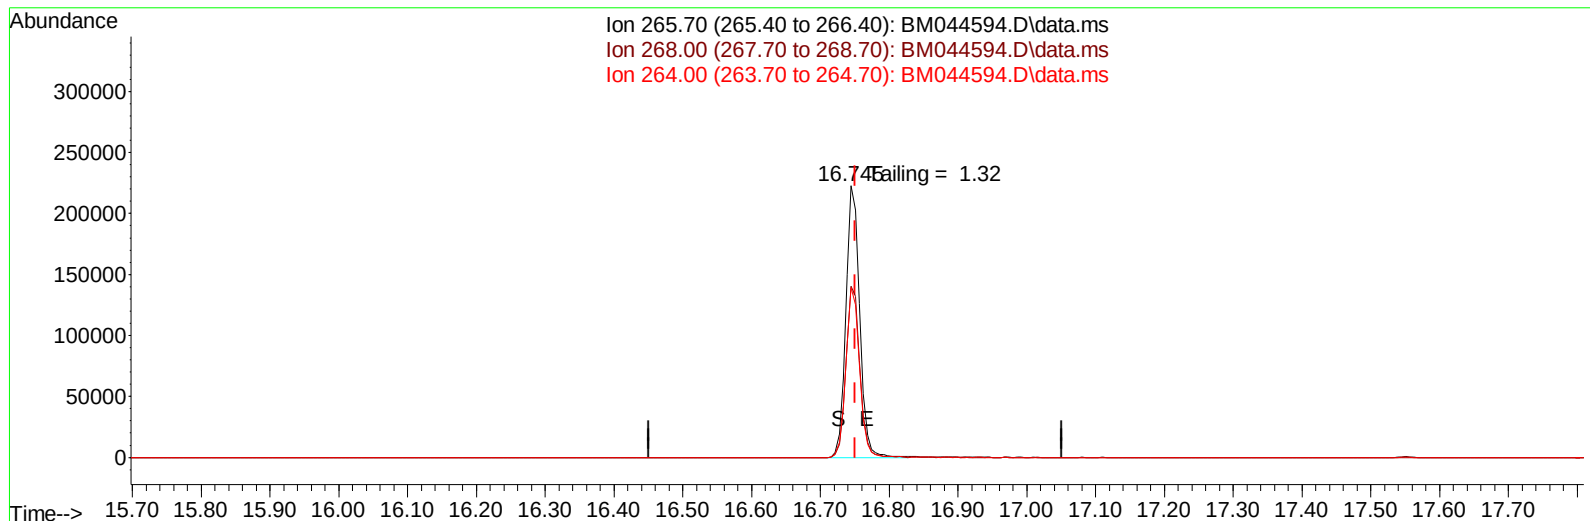

TIC: BM044594.D\data.ms

(70) Pentachlorophenol (C)




16.745min (-0.006) 0.00 ng

response 310142

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.50  | 63.14  |
| 264.00 | 62.30  | 62.59  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031324\  
Data File : BM044594.D  
Acq On : 13 Mar 2024 13:07  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 02:09:55 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031324.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 14 02:00:45 2024  
Response via : Initial Calibration

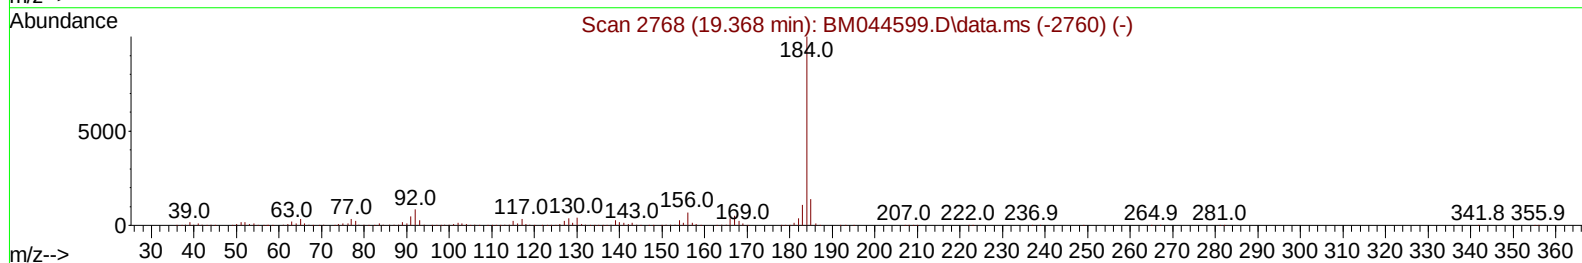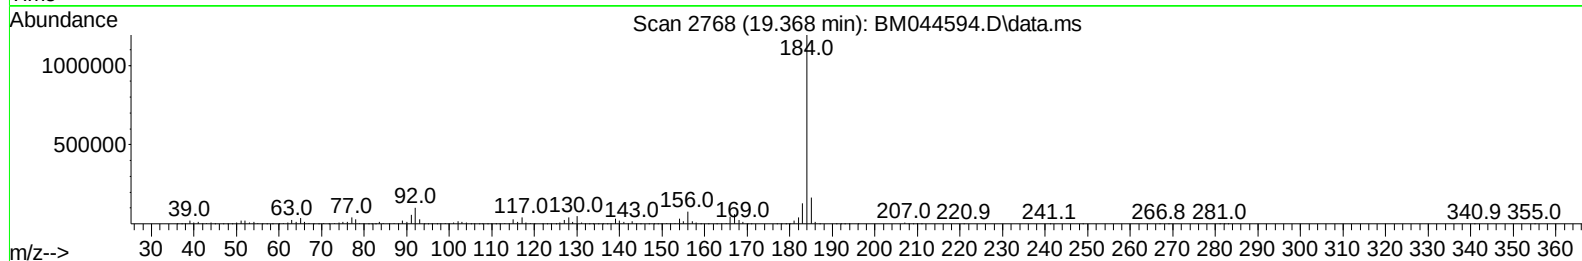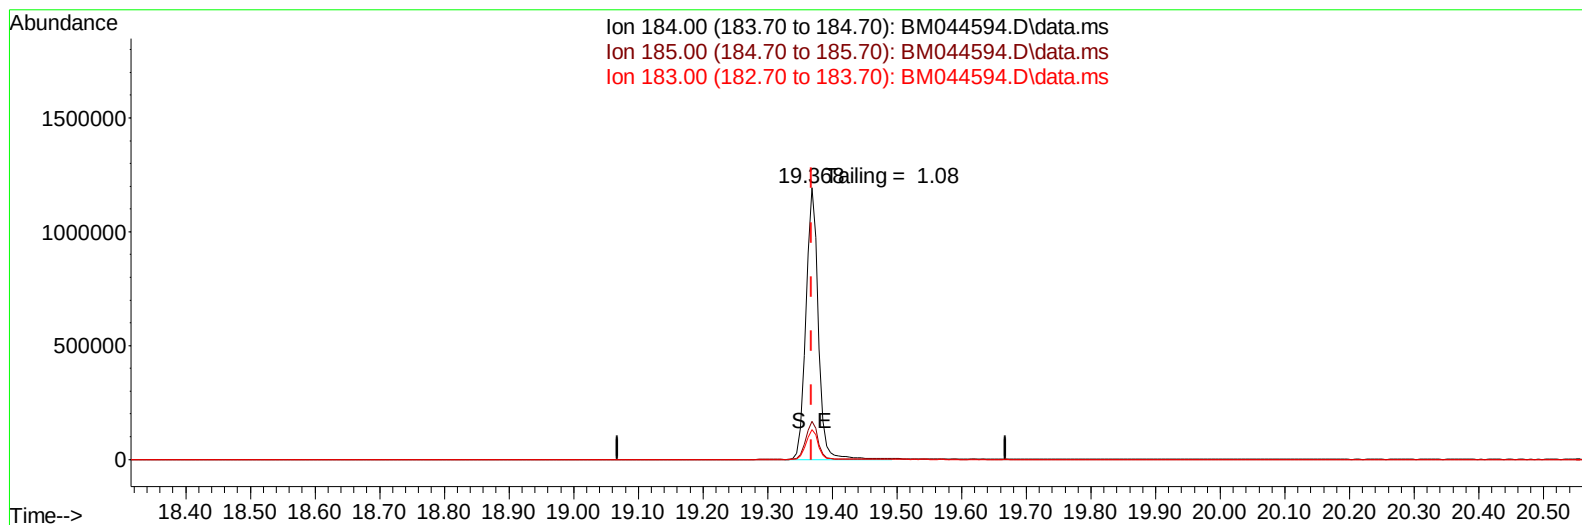

TIC: BM044594.D\data.ms

**(77) Benzidine****19.368min (+ 0.000) 0.00 ng****response 1626042**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.80  | 14.01  |
| 183.00 | 10.90  | 11.02  |
| 0.00   | 0.00   | 0.00   |