
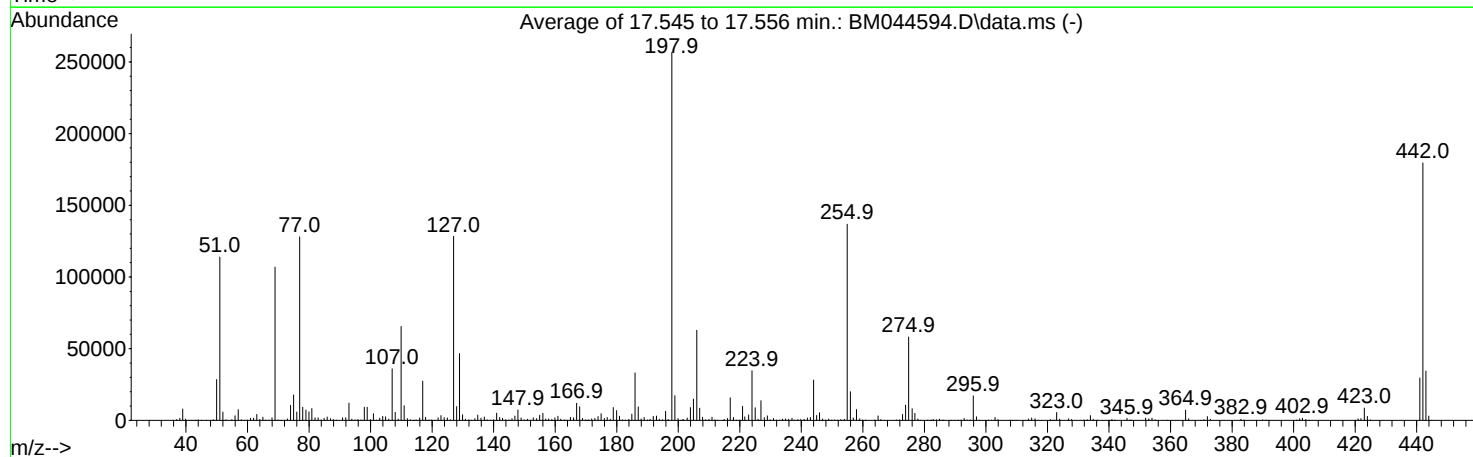


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031324\  
Data File : BM044594.D  
Acq On : 13 Mar 2024 13:07  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031324.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Mar 14 02:28:24 2024

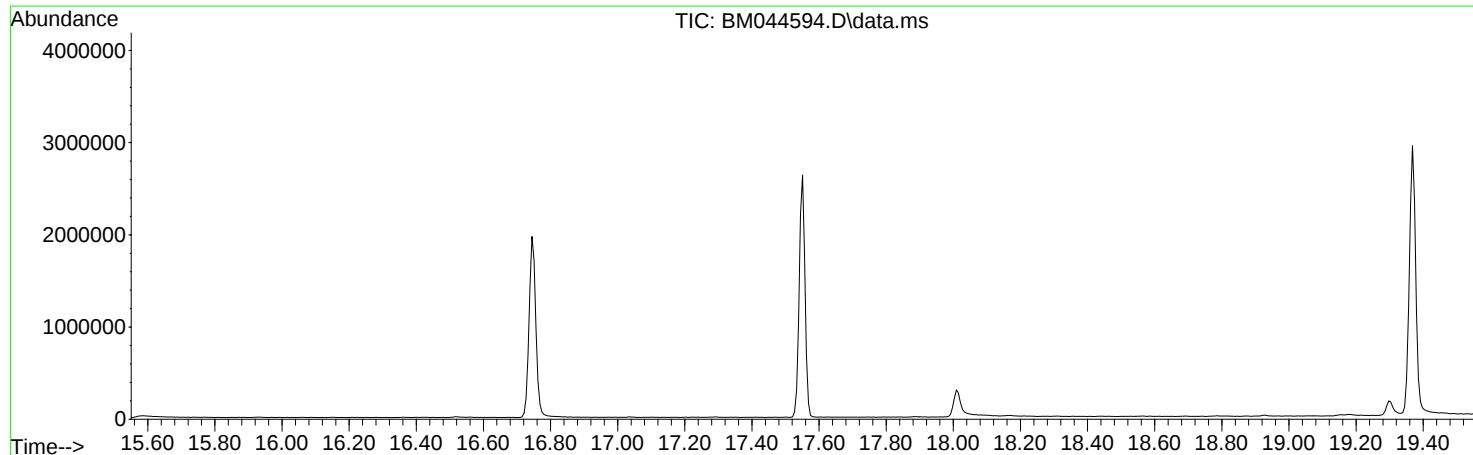




AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 44.4         | 113920     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 1802       | PASS                |
| 69             | 198             | 0.00            | 100             | 41.7         | 106907     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.3          | 336        | PASS                |
| 127            | 198             | 10              | 80              | 50.0         | 128304     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.2          | 515        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 256576     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 17192      | PASS                |
| 275            | 198             | 10              | 60              | 22.6         | 58109      | PASS                |
| 365            | 198             | 1               | 100             | 2.8          | 7112       | PASS                |
| 441            | 198             | 0.01            | 100             | 11.5         | 29544      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 179584     | PASS                |
| 443            | 442             | 15              | 24              | 19.1         | 34328      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031324\  
Data File : BM044594.D  
Acq On : 13 Mar 2024 13:07  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Mar 14 02:09:55 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031324.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 14 02:00:45 2024  
Response via : Initial Calibration

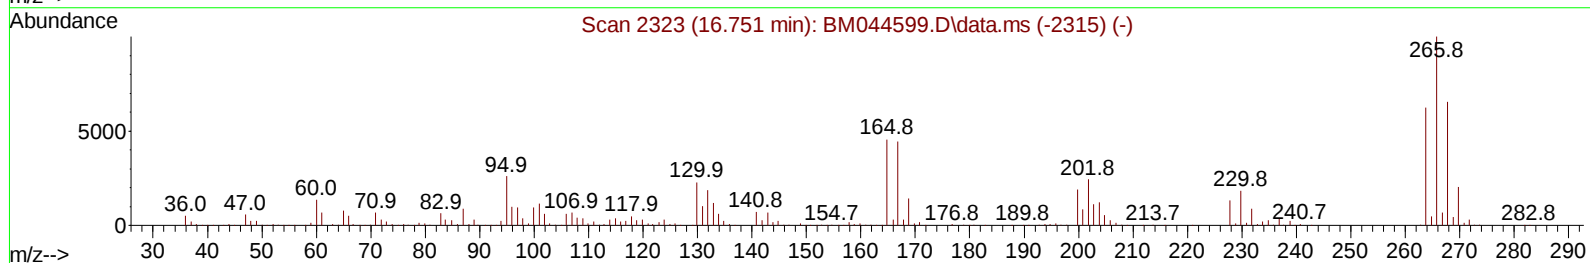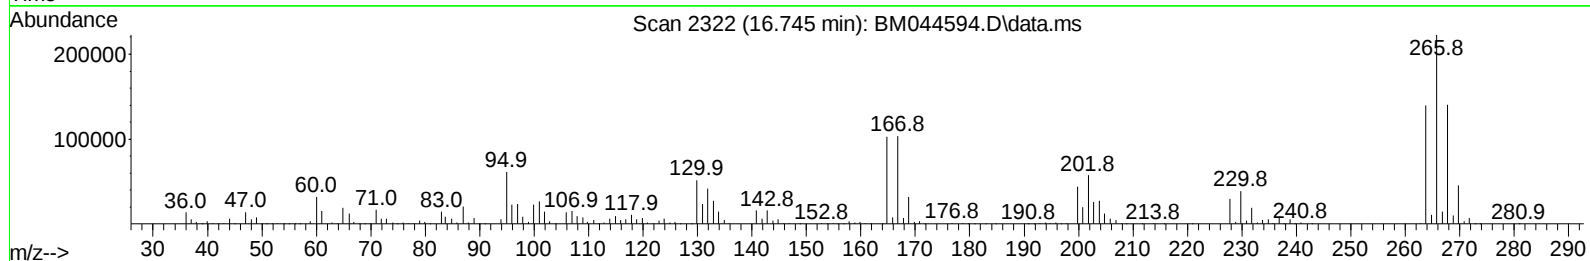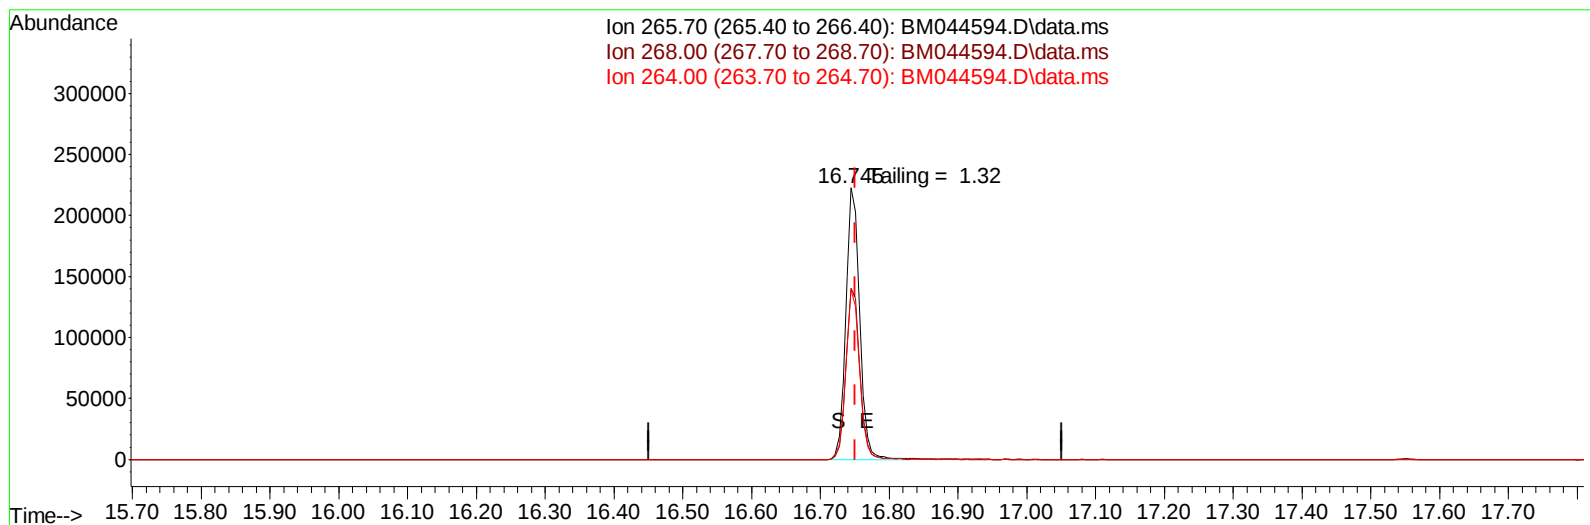

TIC: BM044594.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.006) 0.00 ng




response 310142

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.50  | 63.14  |
| 264.00 | 62.30  | 62.59  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031324\  
Data File : BM044594.D  
Acq On : 13 Mar 2024 13:07  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Mar 14 02:09:55 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031324.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 14 02:00:45 2024  
Response via : Initial Calibration

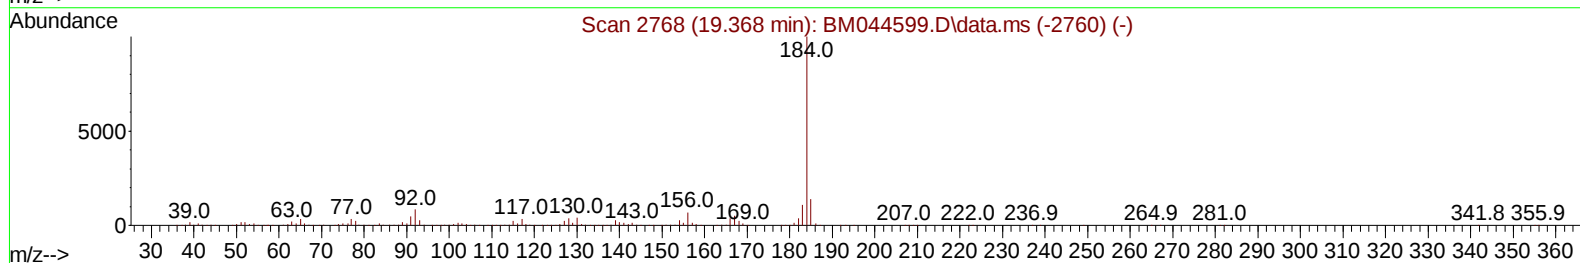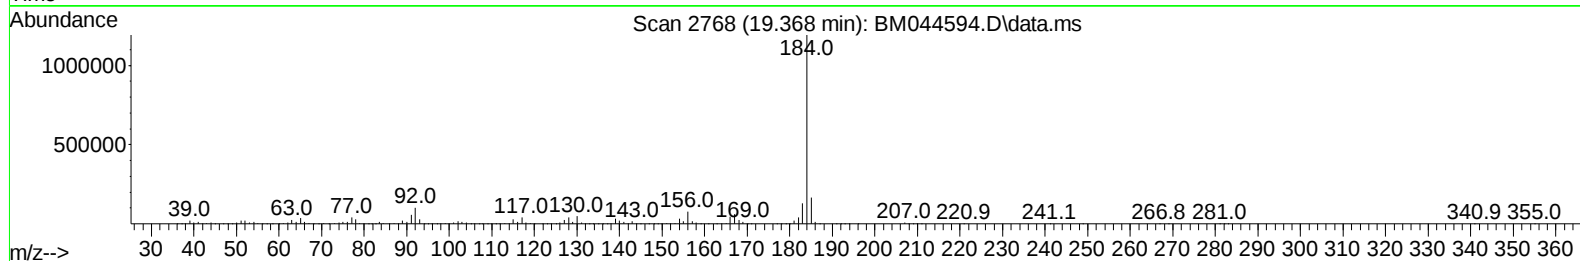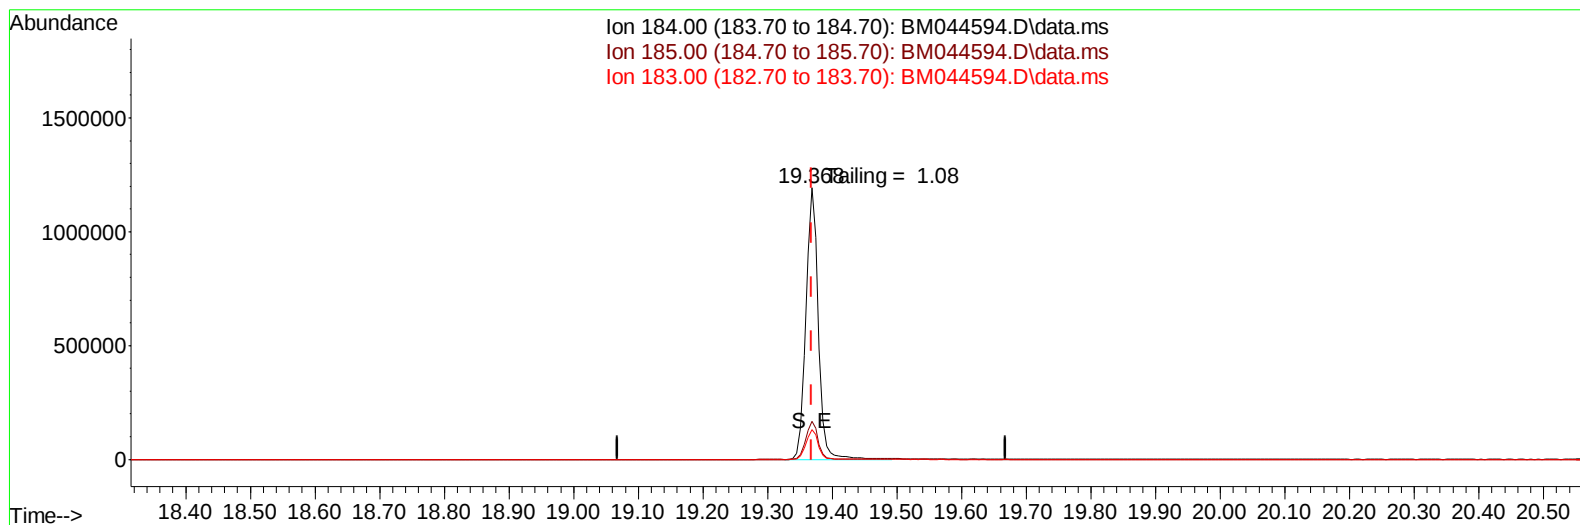

TIC: BM044594.D\data.ms

(77) Benzidine

19.368min (+ 0.000) 0.00 ng

response 1626042

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.80  | 14.01  |
| 183.00 | 10.90  | 11.02  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 3/13/2024     | BNA_M            | <u>BM044594.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 881540           | 20.597             |
| DDD           | 10643            | 20.209             |
| DDE           | 0                | 19.851             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 10643         | 892183           | 1.19               |
|               |                  |                    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP