

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031325\
 Data File : BM049706.D
 Acq On : 13 Mar 2025 09:02
 Operator : RC/JU
 Sample : SSTDICC2.5
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC2.5

Quant Time: Mar 13 14:38:22 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 13 14:27:21 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.804	152	343337	20.000	ng	0.00
21) Naphthalene-d8	10.598	136	1223591	20.000	ng	0.00
39) Acenaphthene-d10	14.445	164	853260	20.000	ng	0.00
64) Phenanthrene-d10	17.186	188	1680850	20.000	ng	0.00
76) Chrysene-d12	21.427	240	1392908	20.000	ng	0.00
86) Perylene-d12	24.438	264	1220001	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	0.000	112	0d	0.000	ng	
7) Phenol-d6	0.000	99	0d	0.000	ng	
23) Nitrobenzene-d5	0.000	82	0d	0.000	ng	
42) 2,4,6-Tribromophenol	0.000	330	0d	0.000	ng	
45) 2-Fluorobiphenyl	0.000	172	0d	0.000	ng	
79) Terphenyl-d14	0.000	244	0d	0.000	ng	
Target Compounds						
19) n-Nitroso-di-n-propyla...	8.610	70	32886	2.221	ng	Qvalue # 90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031325\
Data File : BM049706.D
Acq On : 13 Mar 2025 09:02
Operator : RC/JU
Sample : SSTDICC2.5
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDICC2.5

Quant Time: Mar 13 14:38:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:27:21 2025
Response via : Initial Calibration

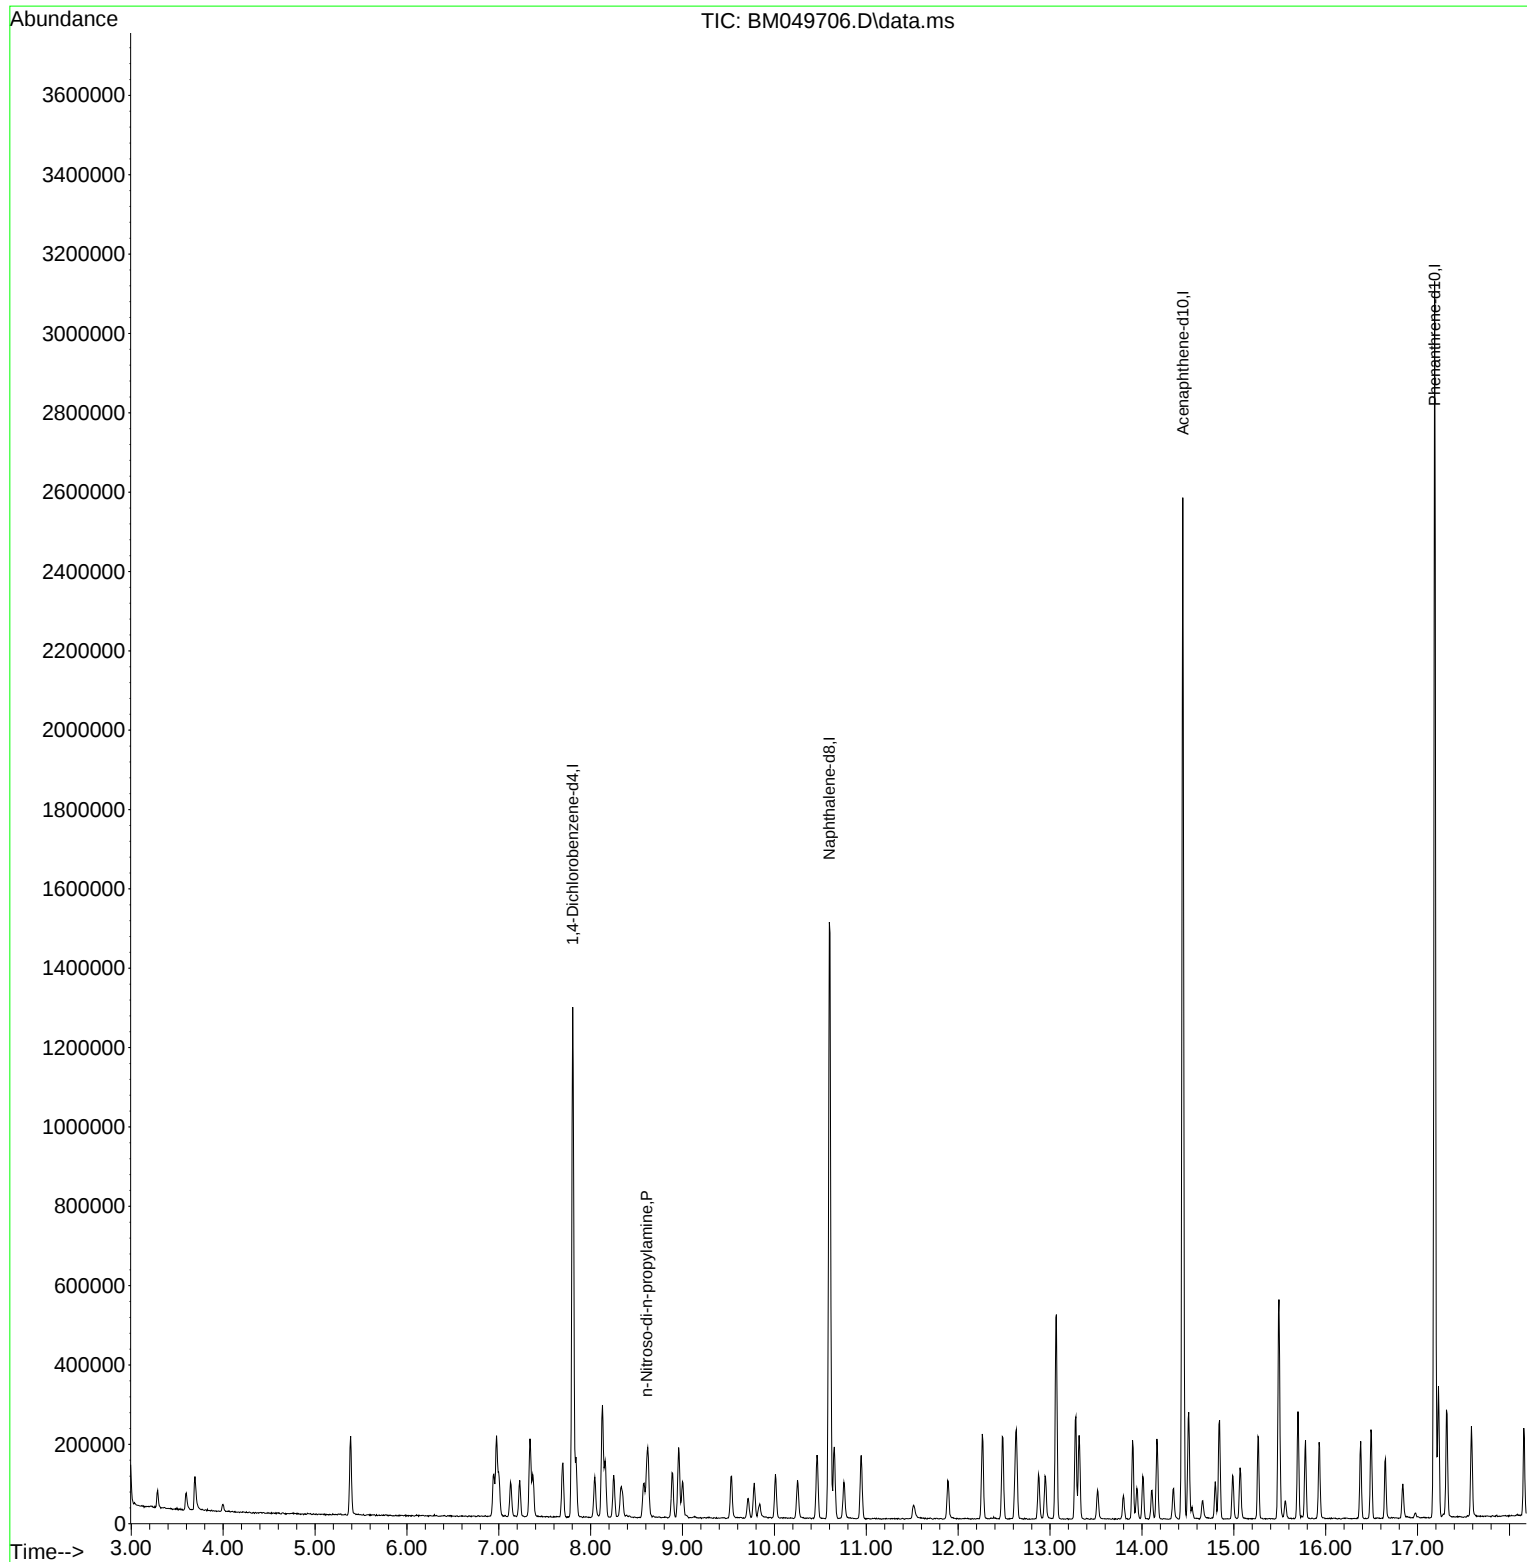

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031325\
Data File : BM049706.D
Acq On : 13 Mar 2025 09:02
Operator : RC/JU
Sample : SSTDICC2.5
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDICC2.5

Quant Time: Mar 13 14:38:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:27:21 2025
Response via : Initial Calibration

