
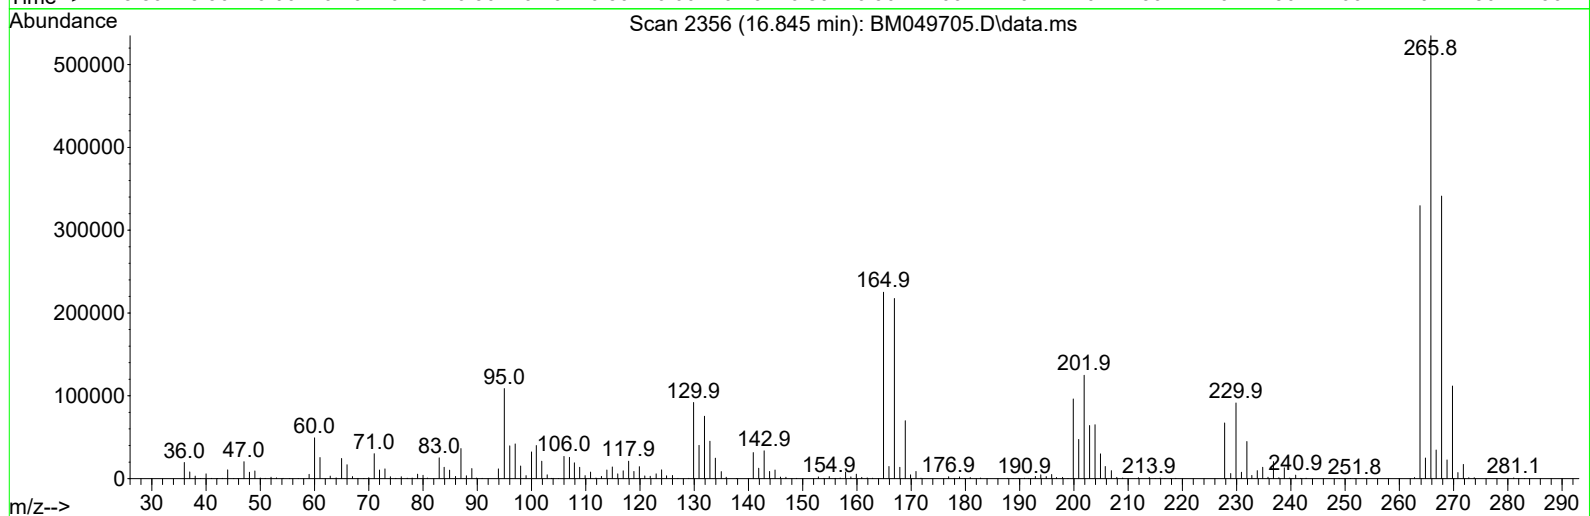


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031325\
Data File : BM049705.D
Acq On : 13 Mar 2025 08:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 14:58:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

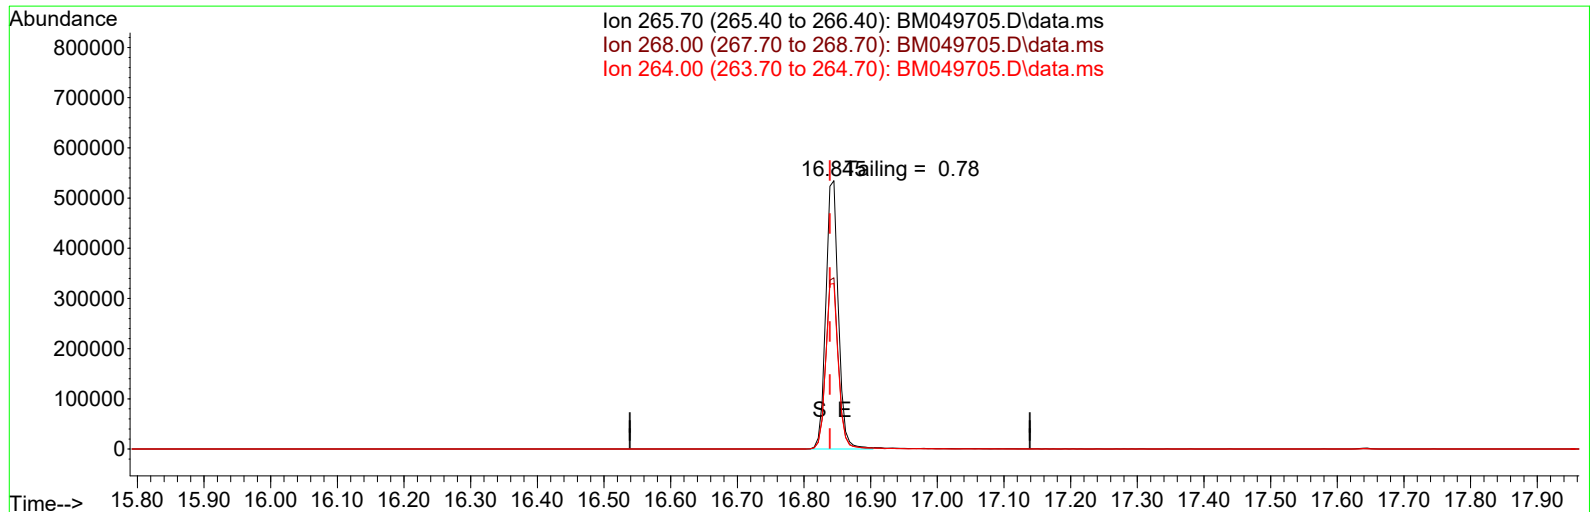

TIC: BM049705.D\data.ms

(70) Pentachlorophenol (C)



16.845min (+ 0.006) 240791.00 ng

response 705303

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	63.81
264.00	64.10	61.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031325\
Data File : BM049705.D
Acq On : 13 Mar 2025 08:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 14:58:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

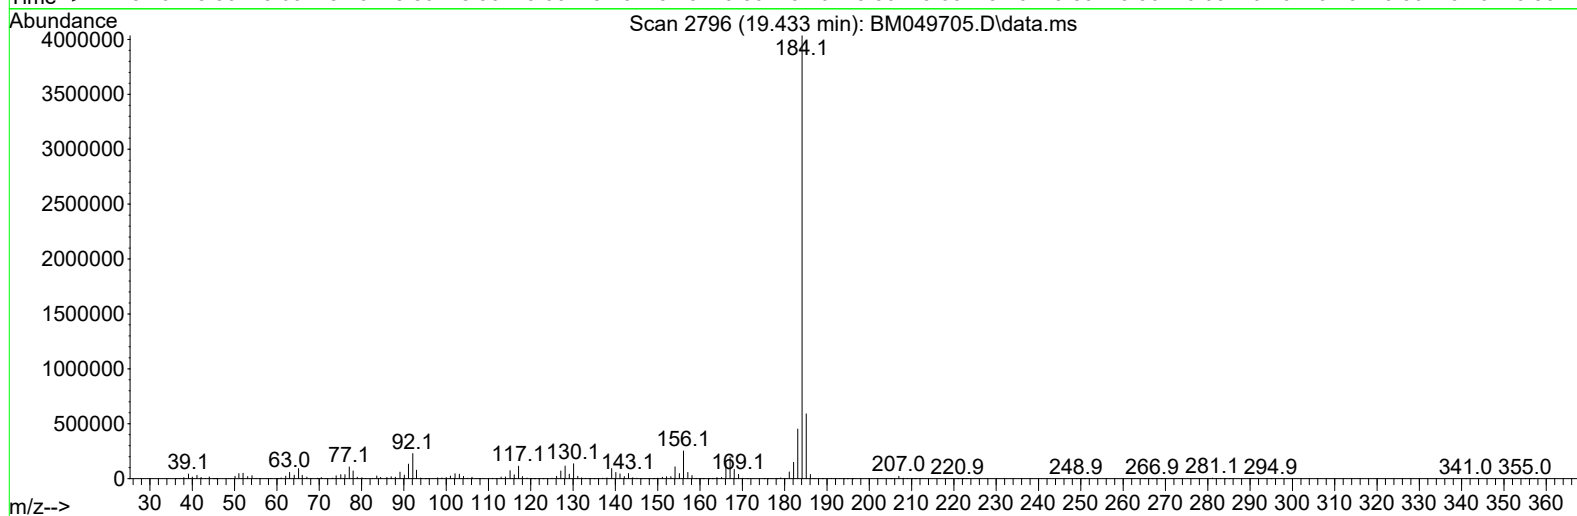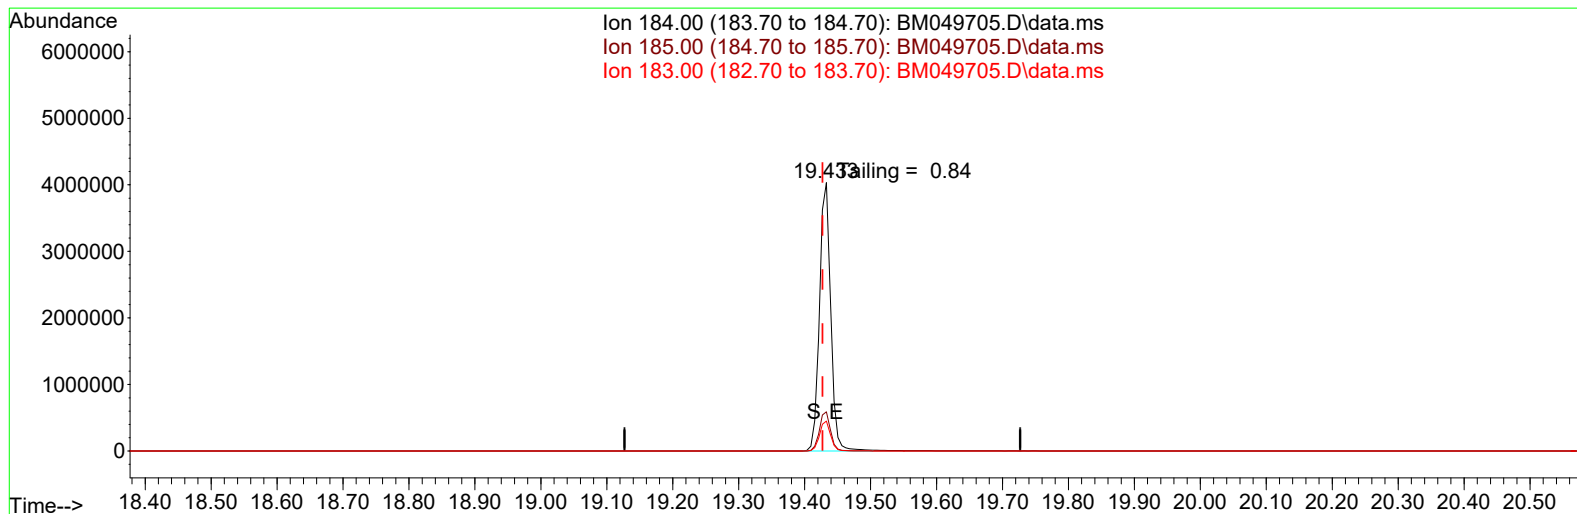

TIC: BM049705.D\data.ms

(77) Benzidine**19.433min (+ 0.006) 192481.98 ng****response 4789142**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.64
183.00	11.00	11.19
0.00	0.00	0.00