


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031325\
Data File : BM049705.D
Acq On : 13 Mar 2025 08:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 13 14:55:34 2025

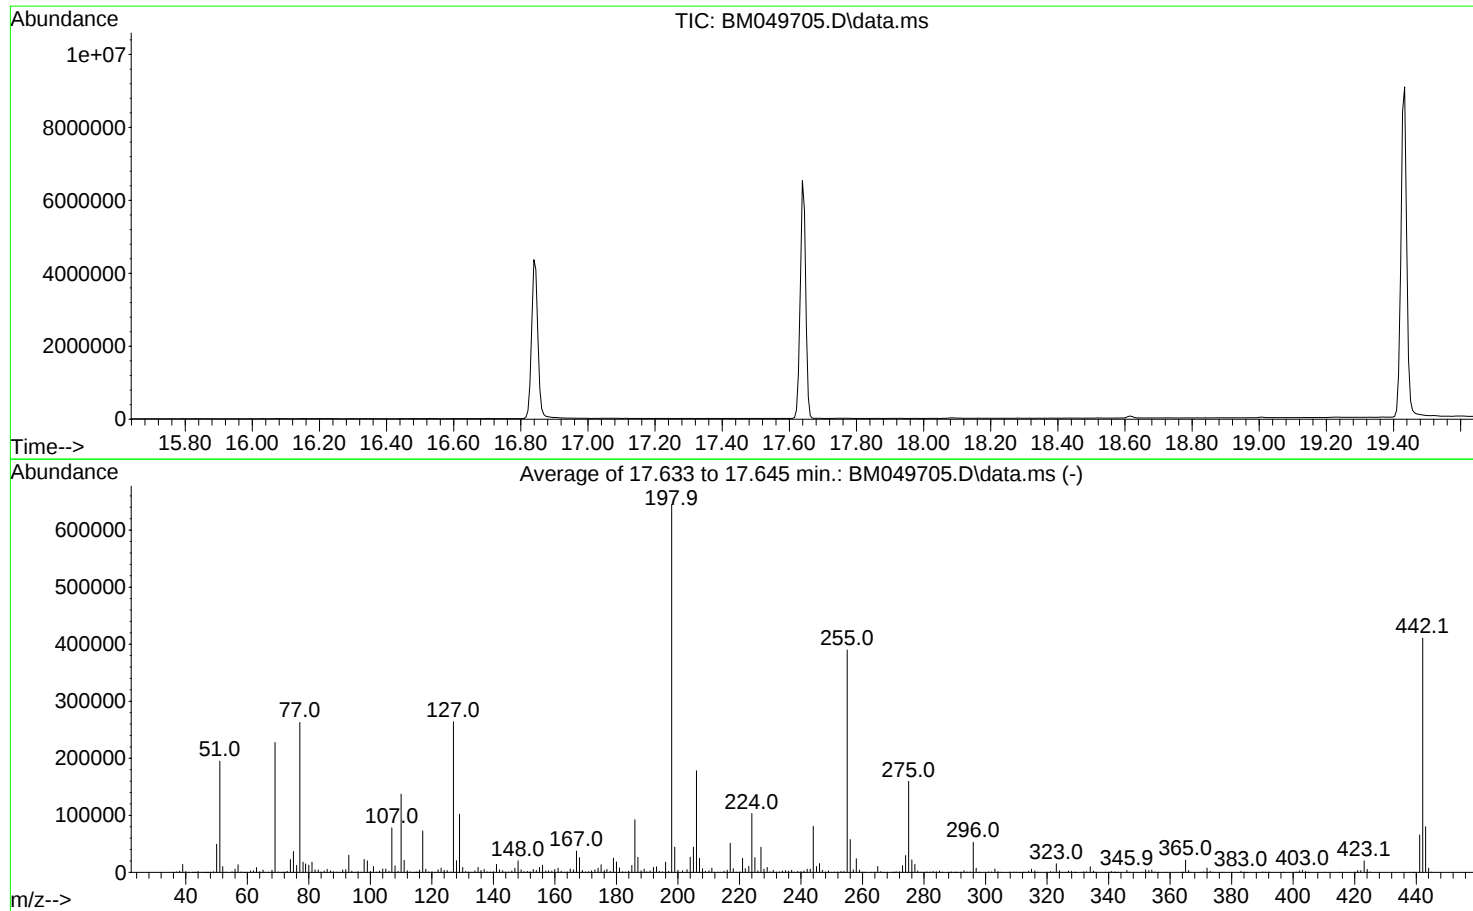



AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	195050	PASS
68	69	0.00	2	1.7	3856	PASS
69	198	0.00	100	35.3	227755	PASS
70	69	0.00	2	0.4	953	PASS
127	198	10	80	40.9	264085	PASS
197	198	0.00	2	0.2	1585	PASS
198	198	100	100	100.0	644928	PASS
199	198	5	9	6.9	44307	PASS
275	198	10	60	24.7	159525	PASS
365	198	1	100	3.4	21715	PASS
441	198	0.01	100	10.2	65573	PASS
442	442	50	100	100.0	410773	PASS
443	442	15	24	19.4	79851	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031325\
Data File : BM049705.D
Acq On : 13 Mar 2025 08:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 13 14:58:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

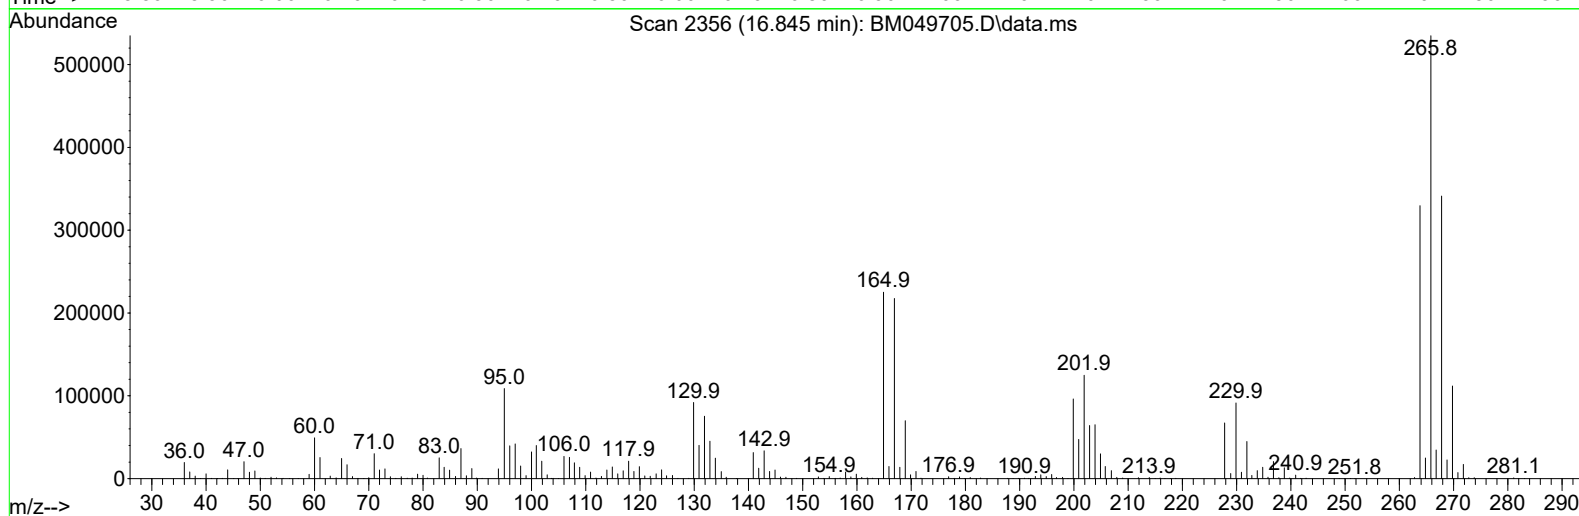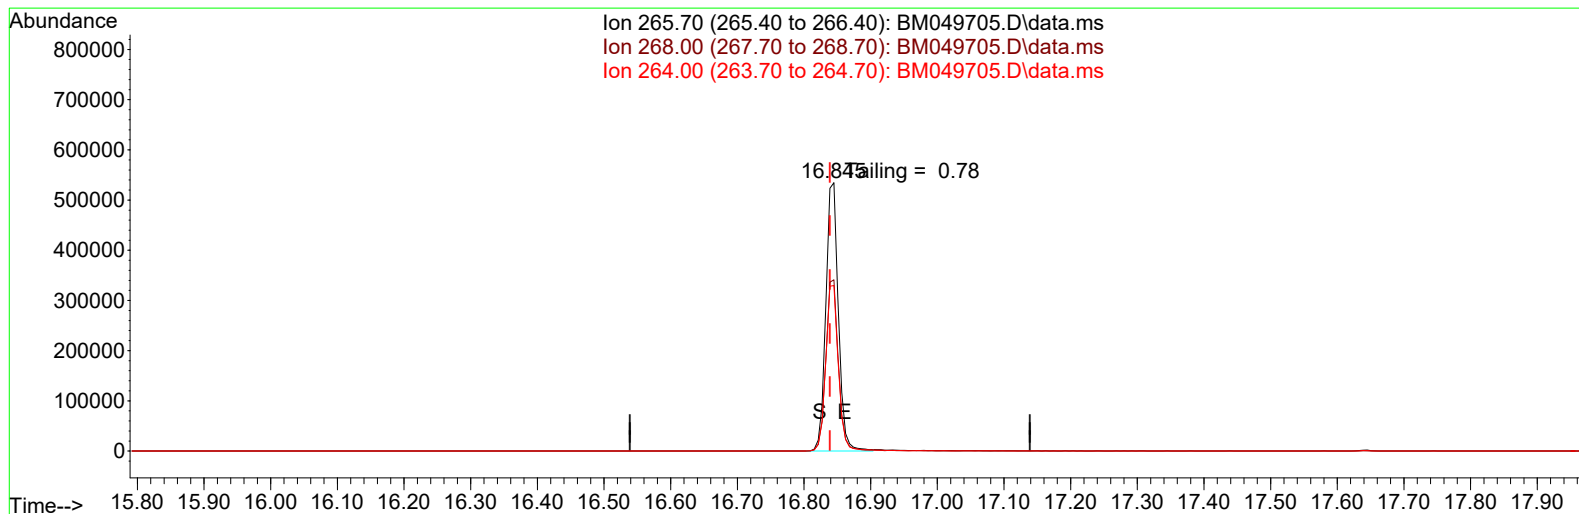

TIC: BM049705.D\data.ms

(70) Pentachlorophenol (C)

16.845min (+ 0.006) 240791.00 ng



response 705303

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	63.81
264.00	64.10	61.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031325\
Data File : BM049705.D
Acq On : 13 Mar 2025 08:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 13 14:58:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 14:55:34 2025
Response via : Initial Calibration

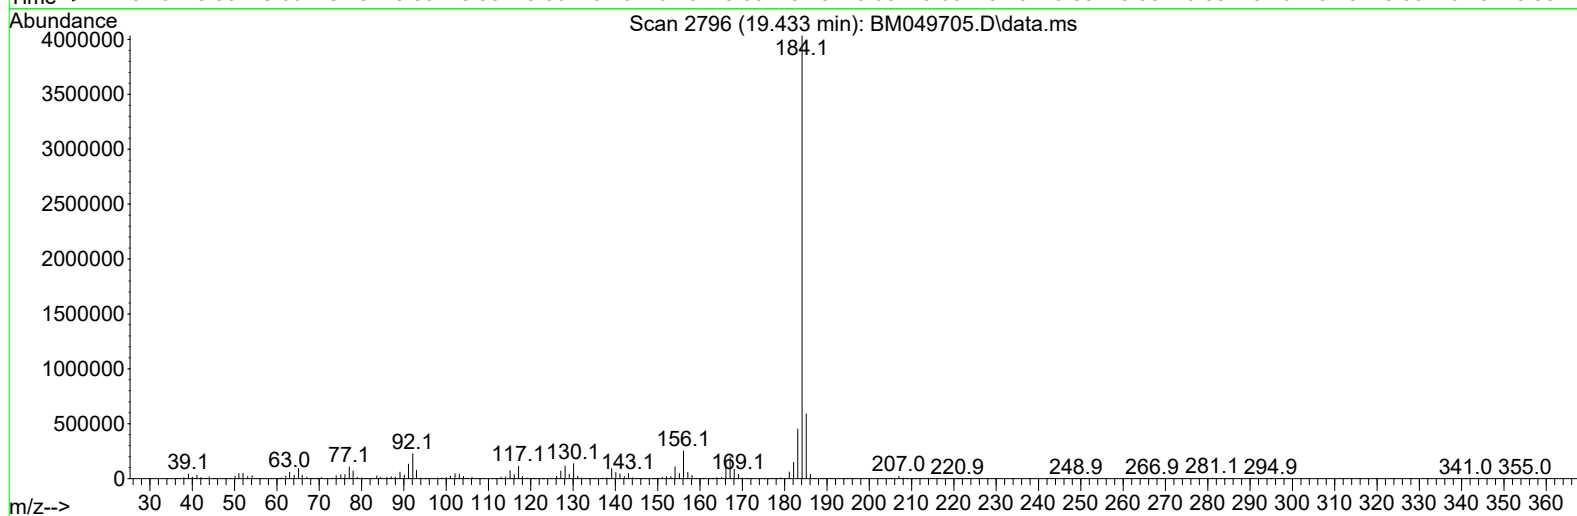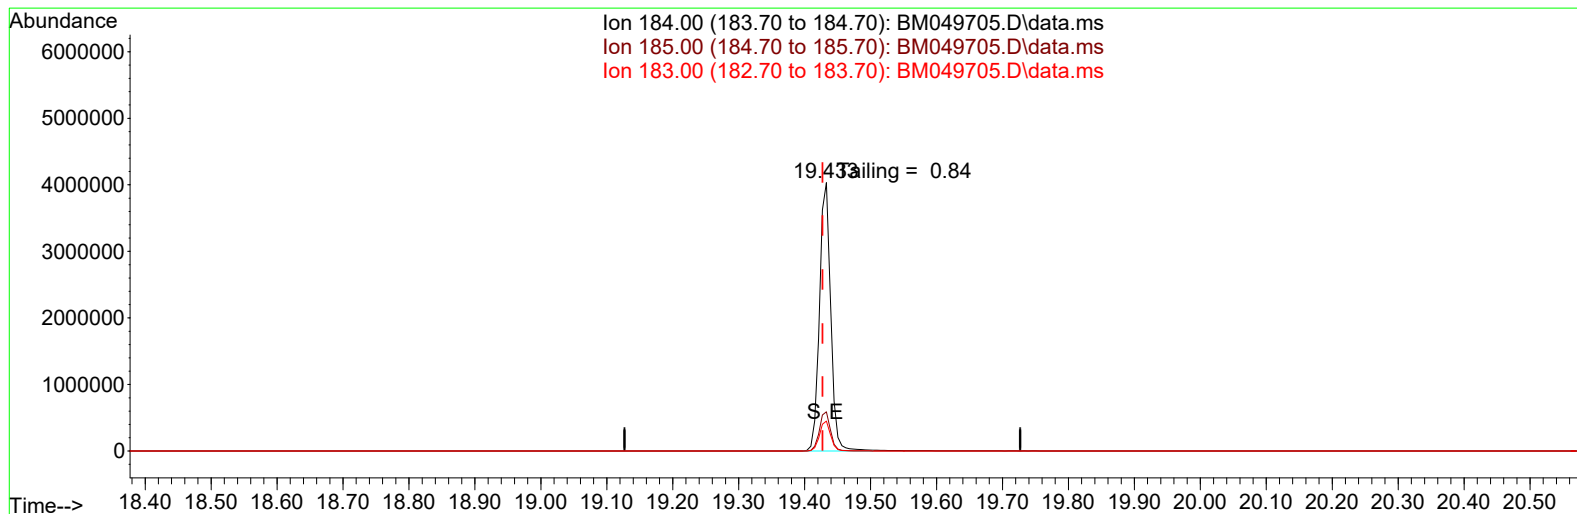

TIC: BM049705.D\data.ms

(77) Benzidine**19.433min (+ 0.006) 192481.98 ng****response 4789142**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.64
183.00	11.00	11.19
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/13/2025	BNA_M	<u>BM049705.D</u>
Compound Name	Response	Retention Time
DDT	2260553	20.674
DDD	15649	20.286
DDE	487	19.721
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16136	2276689	0.71

Instrument :
BNA_M
ClientSampleId :
DFTPP