


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031420\
 Data File : BM025566.D
 Acq On : 14 Mar 2020 11:41
 Operator : CG/JU
 Sample : DFTPP87
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP87

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION
 Last Update : Mon Mar 16 04:27:51 2020

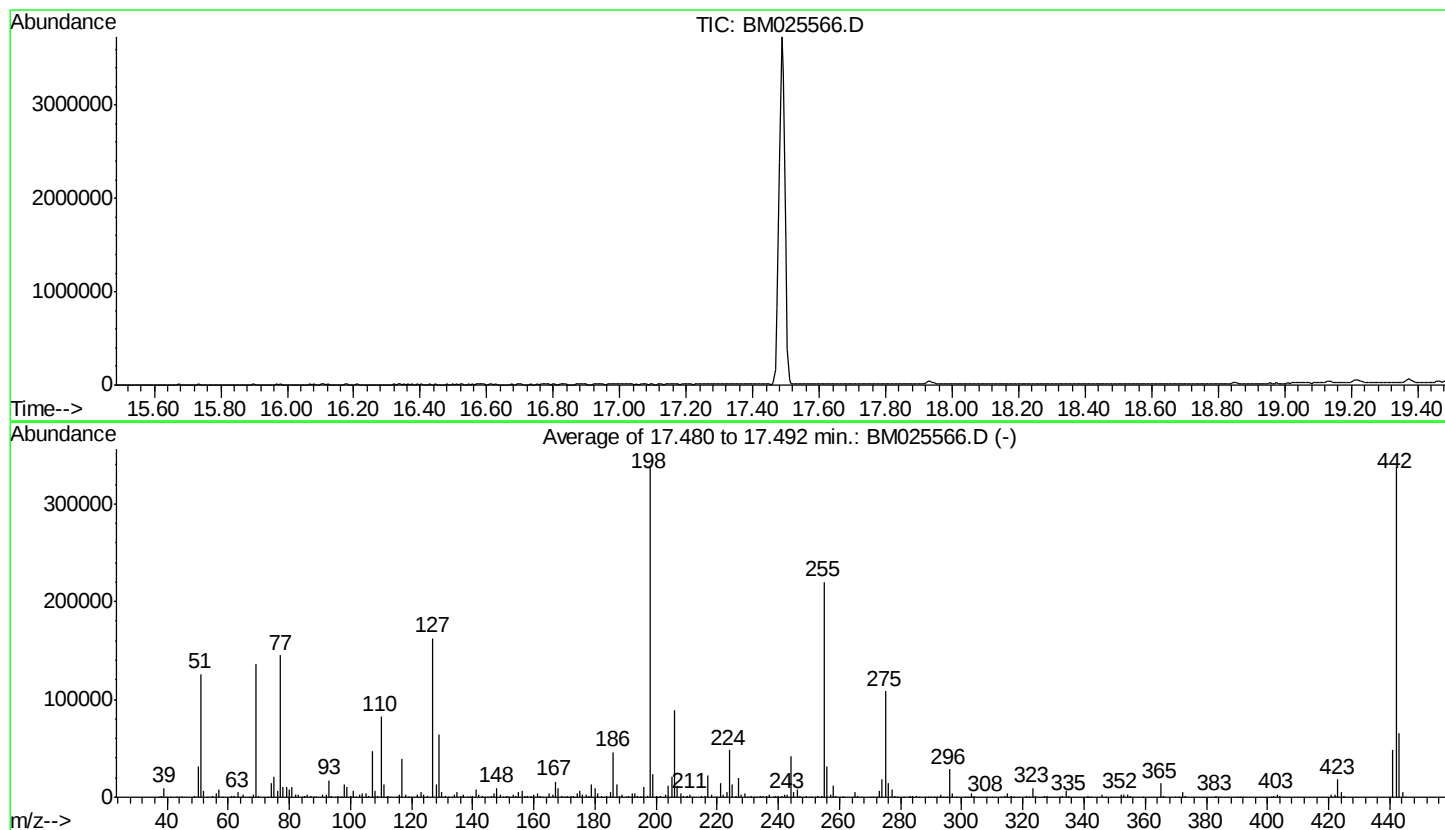

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	125775	PASS
68	69	0.00	2	1.9	2519	PASS
69	198	0.00	100	40.1	136029	PASS
70	69	0.00	2	0.5	705	PASS
127	198	10	80	48.0	162730	PASS
197	198	0.00	2	0.5	1673	PASS
198	198	100	100	100.0	339029	PASS
199	198	5	9	6.9	23416	PASS
275	198	10	60	31.9	108040	PASS
365	198	1	100	4.1	13793	PASS
441	198	0.01	100	14.2	48120	PASS
442	198	50	100	99.7	337941	PASS
443	442	15	24	19.5	66018	PASS

Scan 2476 (17.451 min): BM025566.D
DFTPP87

m/z	Abundance
39.20	311.0
39.90	1035.0
43.00	434.0
44.00	1016.0
49.00	591.0
51.00	337.0
73.00	954.0
84.00	593.0
147.10	343.0
193.10	314.0
207.00	2221.0
221.20	338.0
281.00	576.0
281.90	328.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87

m/z	Abundance
37.10	491.0
38.10	2035.0
39.00	8848.0
40.00	1256.0
41.00	598.0
43.00	476.0
44.00	1047.0
45.00	569.0
49.10	1616.0
50.00	29624.0
51.10	112808.0
52.10	6041.0
53.00	409.0
54.90	593.0
55.90	3535.0
57.00	7735.0
58.00	418.0
61.00	1635.0
62.00	1832.0
63.00	4782.0
64.00	703.0
65.10	2598.0
67.00	315.0
68.10	2154.0
69.00	120392.0
70.00	515.0
73.00	1634.0
74.00	12645.0
75.00	19408.0
76.00	6792.0
77.10	127096.0
78.00	8970.0
79.00	9251.0
80.00	6501.0
81.00	9455.0
82.00	2065.0
83.00	2414.0
84.00	993.0
85.10	1409.0
85.90	3028.0
87.00	1167.0
88.00	629.0
91.00	2000.0
92.00	2271.0
93.00	14952.0
94.00	910.0
96.10	835.0
97.20	576.0
98.00	11210.0
99.00	9767.0
99.90	542.0
101.00	5368.0
103.00	1884.0
104.00	3286.0
105.00	2985.0
106.10	1295.0
107.00	38672.0
108.00	6419.0
108.90	1222.0
110.00	68664.0
111.00	11129.0
112.00	1508.0
113.00	499.0
116.10	1989.0
117.00	33512.0
118.00	2478.0
119.00	312.0
119.90	440.0
122.00	2144.0
123.00	4177.0
124.00	2246.0
125.00	1839.0
127.00	132736.0
128.00	10454.0
129.00	54528.0
130.00	4366.0
131.00	824.0
132.10	432.0
133.00	541.0
134.00	1769.0
135.00	4227.0
136.00	1411.0
136.90	2190.0
138.00	454.0
138.80	383.0
140.20	841.0
141.00	7292.0
142.00	2484.0
143.00	1673.0
144.10	336.0
145.10	500.0
146.00	1316.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87

147.00	3512.0
148.00	7676.0
149.00	1434.0
150.00	499.0
150.90	991.0
152.00	518.0
153.10	1810.0
154.00	1247.0
155.00	4519.0
156.00	4771.0
157.00	1042.0
158.00	1562.0
159.00	978.0
159.90	2376.0
161.00	3491.0
162.00	1121.0
163.00	563.0
165.00	2931.0
166.00	2374.0
167.00	13070.0
168.00	8962.0
169.00	1398.0
170.20	400.0
171.00	942.0
172.00	1040.0
173.00	1602.0
174.00	3306.0
175.10	4604.0
176.00	1655.0
176.90	2573.0
178.00	623.0
178.90	9910.0
180.00	7515.0
181.00	2999.0
182.00	555.0
184.00	1078.0
185.00	4319.0
186.00	35648.0
187.00	11830.0
188.00	1045.0
189.00	2286.0
191.00	1346.0
192.00	2788.0
193.00	3370.0
194.10	744.0
194.90	428.0
196.00	8801.0
197.10	1973.0
198.00	260096.0
199.00	17712.0
200.00	1427.0
201.50	1348.0
203.00	2126.0
204.00	9472.0
205.00	16307.0
206.10	68200.0
207.10	11663.0
208.00	2613.0
209.00	1237.0
210.30	1277.0
211.10	2709.0
211.90	576.0
215.00	635.0
216.00	1250.0
217.00	16880.0
218.00	1647.0
220.10	324.0
221.00	10191.0
221.80	2277.0
223.00	4506.0
224.00	34520.0
225.00	9714.0
226.10	1323.0
227.00	13842.0
227.90	1933.0
229.00	3036.0
230.10	510.0
231.00	1474.0
233.00	311.0
234.00	1058.0
235.10	1441.0
236.00	599.0
237.10	1819.0
238.00	322.0
239.00	740.0
240.00	513.0
241.10	791.0
242.00	1941.0
243.00	2151.0
244.00	29960.0
245.10	4246.0
246.00	5236.0
247.00	1497.0
249.00	1221.0
253.00	629.0
254.20	1727.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87

255.00	156224.0
256.00	23368.0
257.00	2332.0
258.00	8741.0
259.00	1324.0
265.00	4024.0
265.90	679.0
270.90	494.0
272.10	333.0
273.00	4166.0
274.00	12332.0
275.00	72200.0
276.00	9822.0
277.00	5599.0
278.00	1387.0
281.00	636.0
283.00	714.0
284.00	626.0
285.10	1188.0
290.90	318.0
293.00	1332.0
294.00	436.0
295.10	576.0
296.00	20544.0
297.00	2888.0
303.00	2466.0
304.00	849.0
308.00	301.0
313.00	300.0
314.00	1024.0
315.00	2608.0
315.90	1508.0
317.00	336.0
320.90	638.0
323.00	6547.0
324.10	847.0
327.00	1274.0
327.90	564.0
332.00	390.0
333.00	882.0
334.00	4078.0
335.10	1148.0
341.10	638.0
346.00	1189.0
352.00	2080.0
353.00	1493.0
354.10	1884.0
355.10	530.0
365.00	8107.0
366.10	1621.0
371.00	385.0
372.10	2917.0
373.10	1016.0
383.00	865.0
402.10	1128.0
403.00	1657.0
404.00	829.0
421.00	1406.0
422.10	1826.0
423.10	10462.0
424.10	3561.0
425.10	599.0
441.10	24624.0
442.10	185984.0
443.10	37440.0
444.10	2956.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87

m/z	Abundance
37.00	780.0
38.00	2097.0
39.10	12731.0
40.00	1253.0
41.10	405.0
43.10	437.0
44.00	1449.0
45.00	668.0
49.10	1909.0
50.10	35824.0
51.10	153408.0
52.00	7567.0
53.10	451.0
55.00	1412.0
56.00	5429.0
57.00	9360.0
58.00	391.0
61.00	1791.0
62.00	2298.0
63.10	6162.0
64.00	785.0
65.10	2778.0
68.00	2763.0
69.00	164096.0
70.00	858.0
73.10	1957.0
74.00	15820.0
75.00	25296.0
76.10	8249.0
77.10	175040.0
78.10	12879.0
79.00	12760.0
80.00	9075.0
81.00	13741.0
82.00	3681.0
83.00	2878.0
84.00	598.0
85.10	1876.0
86.00	3683.0
87.10	1593.0
88.10	1053.0
91.00	2615.0
92.00	3691.0
93.00	20720.0
93.90	1308.0
95.10	511.0
96.00	1034.0
96.90	325.0
98.00	15475.0
99.00	13702.0
100.00	988.0
101.00	6638.0
101.90	567.0
103.00	2329.0
104.00	4028.0
105.00	4417.0
106.00	1092.0
107.00	56016.0
108.00	8365.0
109.10	1614.0
110.00	100376.0
111.00	15401.0
112.00	1858.0
113.00	507.0
115.00	531.0
116.00	3763.0
117.00	45048.0
118.00	3112.0
119.00	344.0
120.00	576.0
122.00	3757.0
123.00	6010.0
124.00	2915.0
125.00	2383.0
127.00	197056.0
128.00	14950.0
129.00	77856.0
130.00	6588.0
131.00	1334.0
132.00	793.0
133.10	553.0
134.00	2436.0
135.00	6173.0
136.00	2015.0
137.10	3389.0
138.00	734.0
139.00	456.0
140.00	1181.0
141.00	10037.0
141.90	2846.0
143.00	2220.0
144.10	740.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87

145.00	502.0
146.00	2028.0
147.00	4917.0
148.00	11427.0
149.00	2621.0
150.00	561.0
151.10	1611.0
151.80	875.0
153.00	3025.0
154.00	2582.0
155.10	5325.0
156.10	8257.0
157.00	1685.0
157.90	1884.0
159.00	1198.0
160.00	2599.0
161.00	4434.0
161.90	1408.0
162.90	583.0
164.00	479.0
165.00	3946.0
166.10	3155.0
167.00	18624.0
168.00	10183.0
169.10	2111.0
170.00	658.0
171.00	1003.0
172.00	1864.0
172.90	2556.0
174.10	4279.0
175.10	7397.0
176.00	2496.0
177.00	3607.0
178.00	1095.0
179.00	15398.0
180.00	11363.0
181.00	5018.0
182.00	810.0
183.00	487.0
183.90	1256.0
185.00	7507.0
186.00	56496.0
187.00	15967.0
188.10	1667.0
189.00	3507.0
189.90	563.0
191.00	1768.0
192.00	4692.0
193.00	5337.0
193.90	1255.0
195.10	702.0
196.00	12366.0
197.20	3047.0
198.00	406016.0
199.00	28600.0
200.00	2417.0
201.50	2037.0
203.00	2864.0
204.00	13813.0
205.00	24600.0
206.00	107960.0
207.00	15345.0
208.00	4019.0
209.00	1490.0
210.20	1693.0
211.00	3722.0
215.00	1256.0
216.00	2003.0
217.00	27696.0
218.00	3633.0
219.20	486.0
221.00	18000.0
221.90	3867.0
223.00	5547.0
224.00	57352.0
225.00	14743.0
226.20	1956.0
227.00	23768.0
228.00	3623.0
229.00	5330.0
230.00	762.0
231.00	1905.0
232.00	490.0
233.00	572.0
234.00	1626.0
235.10	1915.0
236.10	1119.0
237.00	2549.0
238.10	402.0
238.90	1106.0
240.00	1192.0
241.00	1521.0
242.00	2856.0
243.10	3323.0
244.00	47792.0
245.10	6618.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87

246.00	9640.0
246.90	1609.0
248.00	476.0
249.00	1682.0
249.90	367.0
250.80	394.0
252.00	401.0
253.00	1174.0
254.20	1748.0
255.00	261632.0
256.00	37672.0
257.00	3118.0
258.00	13833.0
258.90	2432.0
260.90	365.0
265.00	5856.0
266.00	999.0
271.00	536.0
271.90	907.0
273.00	8686.0
274.00	20816.0
275.00	126648.0
276.00	17656.0
277.00	9111.0
278.00	1707.0
279.00	375.0
281.00	1042.0
282.10	342.0
283.00	1214.0
284.00	801.0
285.00	1906.0
286.10	437.0
289.00	378.0
289.90	319.0
292.10	427.0
293.00	2567.0
294.00	694.0
295.10	754.0
296.00	32848.0
297.00	4612.0
298.10	335.0
301.00	465.0
301.90	540.0
303.10	4493.0
304.00	1179.0
308.00	537.0
310.00	621.0
312.90	304.0
314.00	1556.0
315.00	4121.0
316.00	2075.0
316.90	335.0
321.00	1448.0
322.10	740.0
323.10	11376.0
324.00	2366.0
327.00	2327.0
328.00	763.0
332.00	674.0
333.00	966.0
334.10	7051.0
335.00	1881.0
341.10	1469.0
341.90	399.0
346.00	2567.0
347.00	483.0
352.00	3718.0
353.00	2336.0
354.10	3853.0
355.00	781.0
365.00	15872.0
366.00	2147.0
371.10	996.0
372.10	5970.0
373.00	1466.0
383.00	1537.0
384.00	371.0
390.00	650.0
390.90	478.0
392.10	398.0
401.10	357.0
402.10	2362.0
403.10	3155.0
404.10	1336.0
421.00	2904.0
422.10	3037.0
423.10	20096.0
424.10	6671.0
425.00	926.0
440.20	390.0
441.10	56512.0
442.10	380032.0
443.10	74032.0
444.10	7182.0
445.00	448.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87

m/z	Abundance
37.00	427.0
38.00	1884.0
39.10	8505.0
40.00	1978.0
41.10	410.0
43.10	620.0
44.00	1200.0
45.00	651.0
49.00	1421.0
50.10	28888.0
51.10	112120.0
52.00	4641.0
53.10	398.0
55.00	908.0
56.00	3324.0
57.00	8463.0
58.00	465.0
60.90	1708.0
62.00	1611.0
63.00	4181.0
63.90	499.0
65.00	2428.0
68.00	2642.0
69.00	123600.0
70.00	742.0
73.00	1348.0
74.00	13552.0
75.00	19736.0
76.10	6542.0
77.10	133120.0
78.10	8897.0
79.00	9829.0
80.00	7187.0
81.00	9865.0
82.00	2775.0
83.00	2160.0
83.90	673.0
85.00	1525.0
86.00	2827.0
87.00	1234.0
87.80	330.0
88.90	343.0
91.00	2027.0
92.00	2933.0
93.00	15968.0
94.00	875.0
95.10	467.0
96.10	890.0
97.10	479.0
98.00	11808.0
99.00	9440.0
100.00	871.0
101.00	5907.0
102.00	2040.0
102.90	3224.0
104.00	3283.0
106.10	1494.0
107.00	45728.0
108.00	5929.0
109.00	1179.0
110.00	77520.0
111.00	11480.0
112.10	1183.0
113.00	687.0
116.10	1963.0
117.00	37440.0
118.10	2663.0
118.90	357.0
119.90	669.0
122.00	3054.0
123.00	4621.0
124.00	1811.0
125.00	1681.0
127.00	158400.0
128.00	13084.0
129.00	60352.0
130.00	4809.0
131.00	893.0
131.90	534.0
133.00	510.0
134.00	2244.0
135.00	5044.0
136.00	2131.0
137.00	2834.0
138.00	417.0
140.00	789.0
141.00	8222.0
141.90	2737.0
143.00	1650.0
143.90	691.0
144.90	613.0
145.90	1412.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87

147.00	4609.0
148.00	9861.0
149.00	1999.0
149.90	615.0
151.00	1220.0
151.60	623.0
153.00	2723.0
154.00	2001.0
155.00	5111.0
156.00	7361.0
157.10	1702.0
158.10	1456.0
158.90	1337.0
160.10	2756.0
161.00	3807.0
162.10	1087.0
163.00	339.0
164.10	332.0
165.00	3165.0
166.10	2679.0
167.00	16072.0
168.00	9089.0
169.00	1204.0
170.20	473.0
171.00	873.0
171.90	1637.0
173.00	1574.0
173.90	3788.0
175.00	6017.0
176.00	2030.0
177.00	3547.0
178.00	981.0
179.00	12329.0
180.00	9115.0
181.00	4572.0
182.00	836.0
183.00	338.0
184.10	949.0
185.10	5719.0
186.00	46456.0
187.00	12904.0
188.00	1305.0
189.00	2833.0
190.00	695.0
191.10	1661.0
192.00	4930.0
193.00	5150.0
194.10	974.0
195.10	761.0
196.00	10422.0
198.00	350976.0
199.00	23936.0
200.00	2054.0
201.40	2081.0
203.00	2385.0
204.00	12982.0
205.00	22064.0
206.10	91120.0
207.00	14245.0
208.00	3573.0
209.00	1127.0
209.90	1293.0
211.00	3500.0
211.90	725.0
214.90	910.0
216.00	2027.0
217.00	23920.0
218.00	3430.0
219.90	698.0
221.00	14735.0
221.80	3439.0
223.00	5543.0
224.00	52400.0
225.00	14197.0
226.10	1471.0
227.00	20184.0
228.00	3679.0
229.00	4399.0
230.10	437.0
231.00	1319.0
232.00	389.0
232.90	365.0
234.00	1357.0
235.00	1751.0
235.90	1032.0
237.10	1893.0
238.00	343.0
239.00	715.0
239.90	723.0
240.90	1396.0
242.00	2583.0
243.00	3065.0
244.10	46296.0
245.10	5759.0
246.00	8113.0
247.00	1680.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87

248.00	618.0
249.00	1821.0
250.90	470.0
252.00	401.0
253.00	855.0
255.00	243520.0
256.00	33928.0
257.00	2923.0
258.00	13300.0
259.00	2178.0
259.90	494.0
261.10	493.0
264.00	482.0
265.00	5582.0
266.00	905.0
267.10	340.0
269.90	384.0
271.00	713.0
272.00	535.0
273.00	7124.0
274.00	21088.0
275.00	125272.0
276.00	15302.0
277.00	9655.0
278.00	1568.0
278.90	461.0
281.10	575.0
281.90	585.0
283.00	1054.0
284.00	1242.0
285.00	1455.0
286.00	394.0
288.00	370.0
289.00	742.0
289.90	416.0
291.90	403.0
293.00	2292.0
293.90	811.0
295.20	754.0
296.00	31680.0
297.00	4161.0
297.90	421.0
301.10	392.0
302.00	602.0
303.10	3721.0
304.00	890.0
308.00	578.0
310.10	325.0
312.90	402.0
314.00	1758.0
315.00	4566.0
316.10	2193.0
317.00	478.0
321.10	918.0
322.00	628.0
323.10	10937.0
324.10	1885.0
327.00	2342.0
328.10	1028.0
332.00	845.0
333.00	1183.0
334.10	6957.0
335.10	1709.0
341.10	1630.0
342.00	442.0
346.00	3302.0
347.00	629.0
352.00	3300.0
353.00	3018.0
354.10	4148.0
355.00	848.0
359.10	303.0
365.00	17400.0
365.90	1915.0
369.90	503.0
371.10	653.0
372.00	5989.0
373.10	1615.0
383.00	1756.0
384.00	431.0
390.10	730.0
391.00	323.0
392.10	405.0
401.10	470.0
402.00	2070.0
403.10	3195.0
404.00	1210.0
421.00	3012.0
422.00	3589.0
423.10	22768.0
424.10	6101.0
425.10	991.0
440.10	423.0
441.10	63224.0
442.10	447808.0
443.10	86584.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87

444.107415.0

444.90445.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87