

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031424\
 Data File : BM044611.D
 Acq On : 14 Mar 2024 13:33
 Operator : MA/JU
 Sample : PB159579BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK579

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044611.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	34	rBV	57919	70382	1.53%	0.152%
2	3.652	93	96	119	rBV	659113	1061480	23.05%	2.288%
3	3.963	145	149	153	rVB	11882	14875	0.32%	0.032%
4	6.875	636	644	657	rBV	791087	1261138	27.39%	2.718%
5	7.052	667	674	687	rBV	673406	1066530	23.16%	2.298%
6	7.234	697	705	716	rBV	789261	1262379	27.42%	2.720%
7	7.704	778	785	795	rVB	614938	993464	21.58%	2.141%
8	8.404	897	904	919	rBV	915809	1509994	32.80%	3.254%
9	8.863	974	982	992	rBV	720450	1213309	26.35%	2.615%
10	9.575	1094	1103	1110	rBV	595546	997353	21.66%	2.149%
11	10.104	1187	1193	1209	rBV	823615	1457454	31.66%	3.141%
12	10.481	1249	1257	1265	rBV	836679	1401717	30.44%	3.021%
13	10.628	1275	1282	1299	rBV	840667	1590211	34.54%	3.427%
14	12.086	1523	1530	1539	rBV3	11913	30575	0.66%	0.066%
15	13.245	1723	1727	1733	rVB6	5619	8207	0.18%	0.018%
16	13.769	1809	1816	1827	rBV	1617319	2250937	48.89%	4.851%
17	14.039	1855	1862	1874	rBV	1808564	2643455	57.41%	5.697%
18	14.345	1908	1914	1922	rBV	1238782	1789577	38.87%	3.857%
19	14.563	1943	1951	1970	rBV	594236	1144613	24.86%	2.467%
20	14.780	1984	1988	1995	rVB8	6803	12682	0.28%	0.027%
21	15.345	2077	2084	2095	rBV	2263682	3272681	71.08%	7.053%
22	15.474	2099	2106	2121	rBV	811288	1190705	25.86%	2.566%
23	15.586	2121	2125	2130	rVB5	9749	14375	0.31%	0.031%
24	16.133	2211	2218	2222	rBV5	9675	16040	0.35%	0.035%
25	16.521	2281	2284	2288	rBV5	3174	5193	0.11%	0.011%
26	16.786	2325	2329	2332	rBV4	3983	5535	0.12%	0.012%
27	17.098	2376	2382	2393	rBV	1449829	2158448	46.88%	4.651%
28	17.198	2393	2399	2411	rBV2	2446325	3628353	78.81%	7.819%
29	17.792	2497	2500	2503	rBV5	3269	4705	0.10%	0.010%
30	18.010	2532	2537	2548	rBV	114309	214910	4.67%	0.463%
31	19.068	2713	2717	2721	rVB3	30125	42641	0.93%	0.092%
32	19.139	2725	2729	2733	rVV	24364	35889	0.78%	0.077%
33	19.298	2752	2756	2766	rBV2	77433	131456	2.86%	0.283%
34	19.498	2784	2790	2799	rBV	2944612	4241200	92.12%	9.140%
35	21.298	3091	3096	3104	rBV	1863486	2406699	52.27%	5.186%
36	23.403	3447	3454	3461	rBV2	2412016	4604136	100.00%	9.922%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031424\
Data File : BM044611.D
Acq On : 14 Mar 2024 13:33
Operator : MA/JU
Sample : PB159579BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK579

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

37	23.545	3471	3478	3489	rVB	1366252	2650025	57.56%	5.711%
----	--------	------	------	------	-----	---------	---------	--------	--------


Sum of corrected areas: 46403323

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031424\
Data File : BM044611.D
Acq On : 14 Mar 2024 13:33
Operator : MA/JU
Sample : PB159579BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK579

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

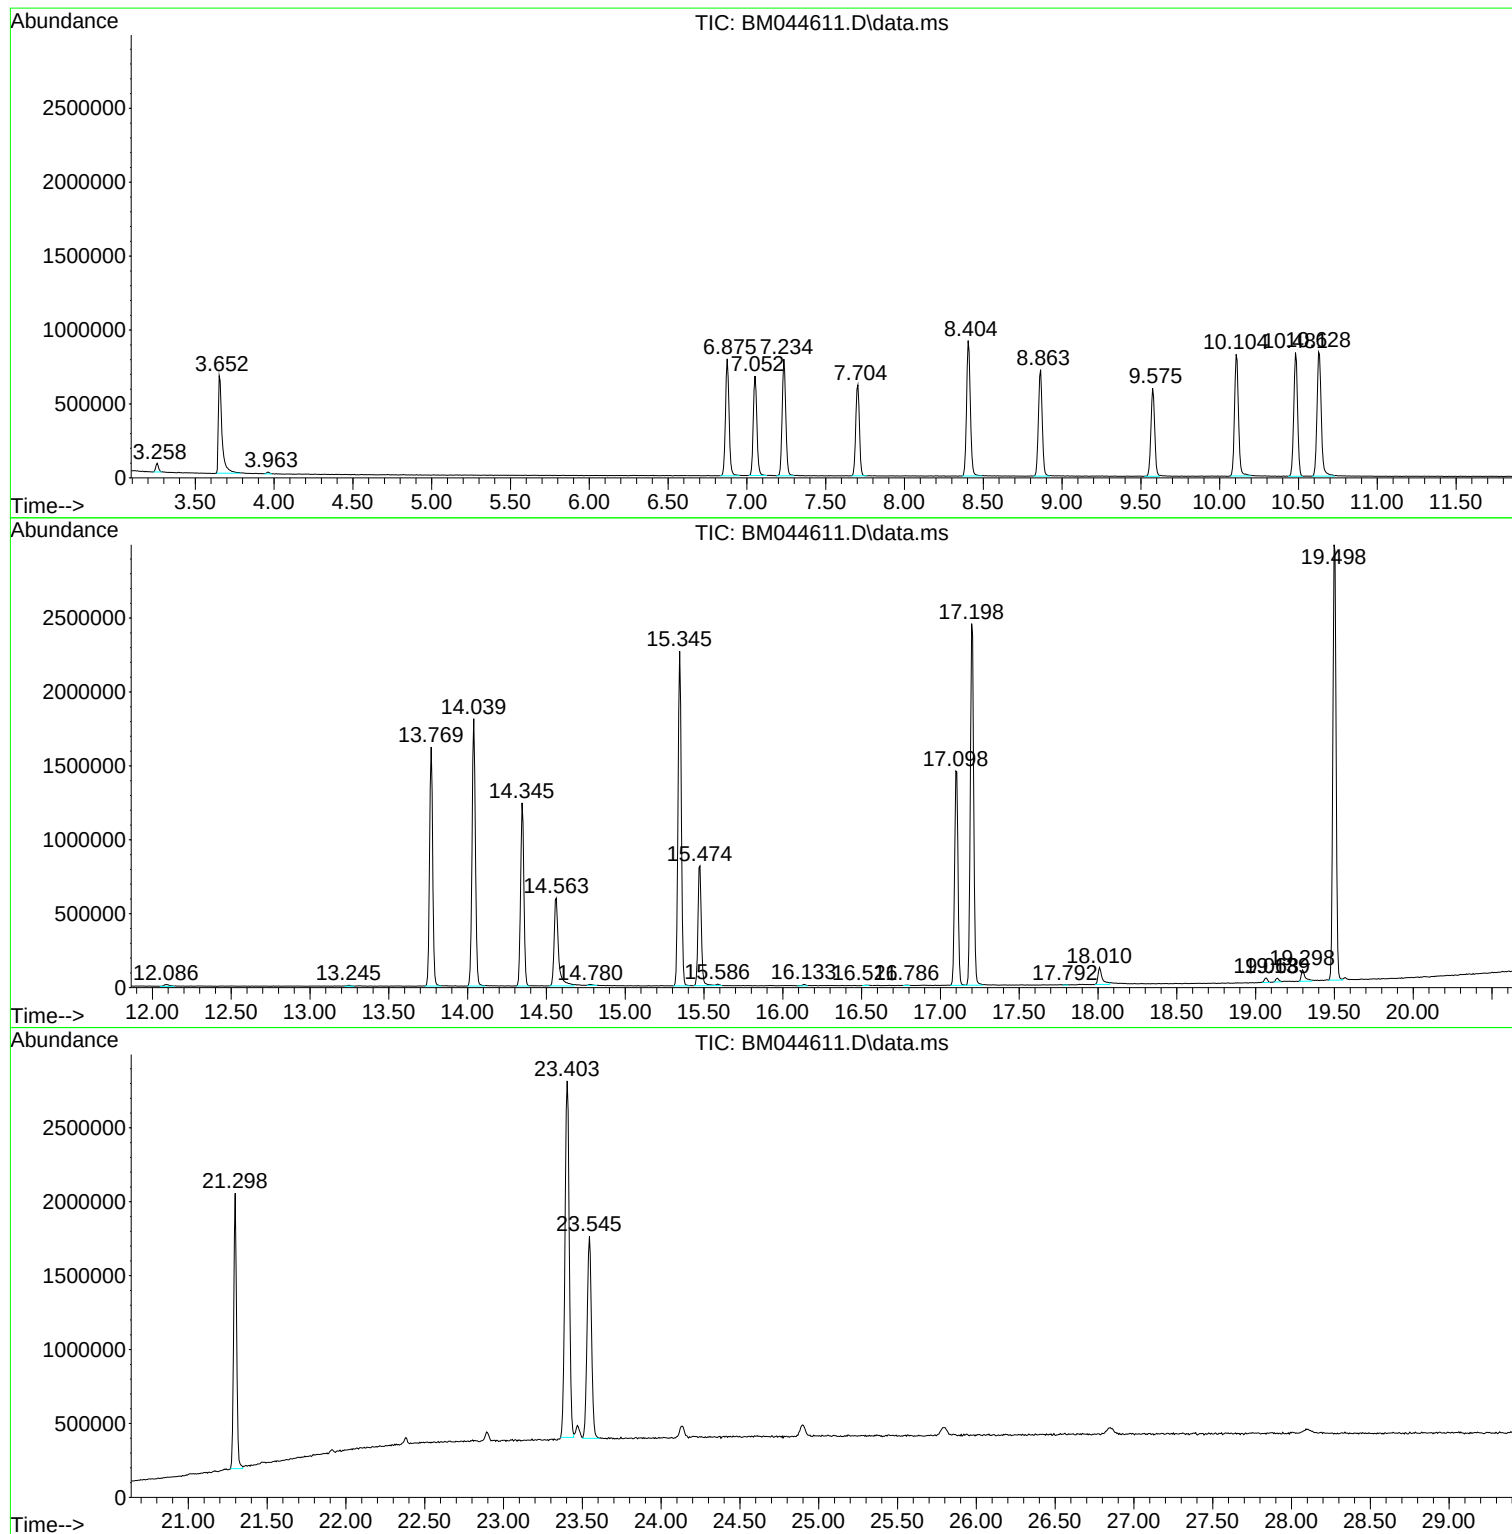

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031424\
Data File : BM044611.D
Acq On : 14 Mar 2024 13:33
Operator : MA/JU
Sample : PB159579BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK579

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031424\
Data File : BM044611.D
Acq On : 14 Mar 2024 13:33
Operator : MA/JU
Sample : PB159579BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK579

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------