

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031516\
 Data File : BM004606.D
 Acq On : 15 Mar 2016 20:10
 Operator : UM/SJ
 Sample : H1710-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MS-DS-E70

Quant Time: Mar 16 05:57:20 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM031516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 16 05:57:50 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	65230	20.00	ng/ul	0.00
18) Naphthalene-d8	10.64	136	279376	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.48	164	157871	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.22	188	362250	20.00	ng/ul	0.00
78) Chrysene-d12	21.40	240	435417	20.00	ng/ul	0.00
86) Perylene-d12	23.70	264	439835	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.33	96	8704	4.60	ng/uL	0.00
5) Phenol-d5	7.00	99	171440	31.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.18	67	104132	34.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	140095	32.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.54	113	136864	31.68	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	64580	33.24	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	70663	33.67	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	129989	31.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	181518	36.85	ng/ul	0.00
44) Dimethylphthalate-d6	13.89	166	438757	35.55	ng/ul	0.00
47) Acenaphthylene-d8	14.17	160	524964	34.69	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	74193	31.10	ng/ul	0.00
58) Fluorene-d10	15.47	176	384768	35.77	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.58	200	53675	28.19	ng/ul	0.00
71) Anthracene-d10	17.32	188	615512	36.91	ng/ul	0.00
79) Pyrene-d10	19.62	212	723110	36.38	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.56	264	822306	41.86	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.93	163	154758	12.35	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031516\
Data File : BM004606.D
Acq On : 15 Mar 2016 20:10
Operator : UM/SJ
Sample : H1710-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MS-DS-E70

Quant Time: Mar 16 05:57:20 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 16 05:57:50 2016
Response via : Initial Calibration

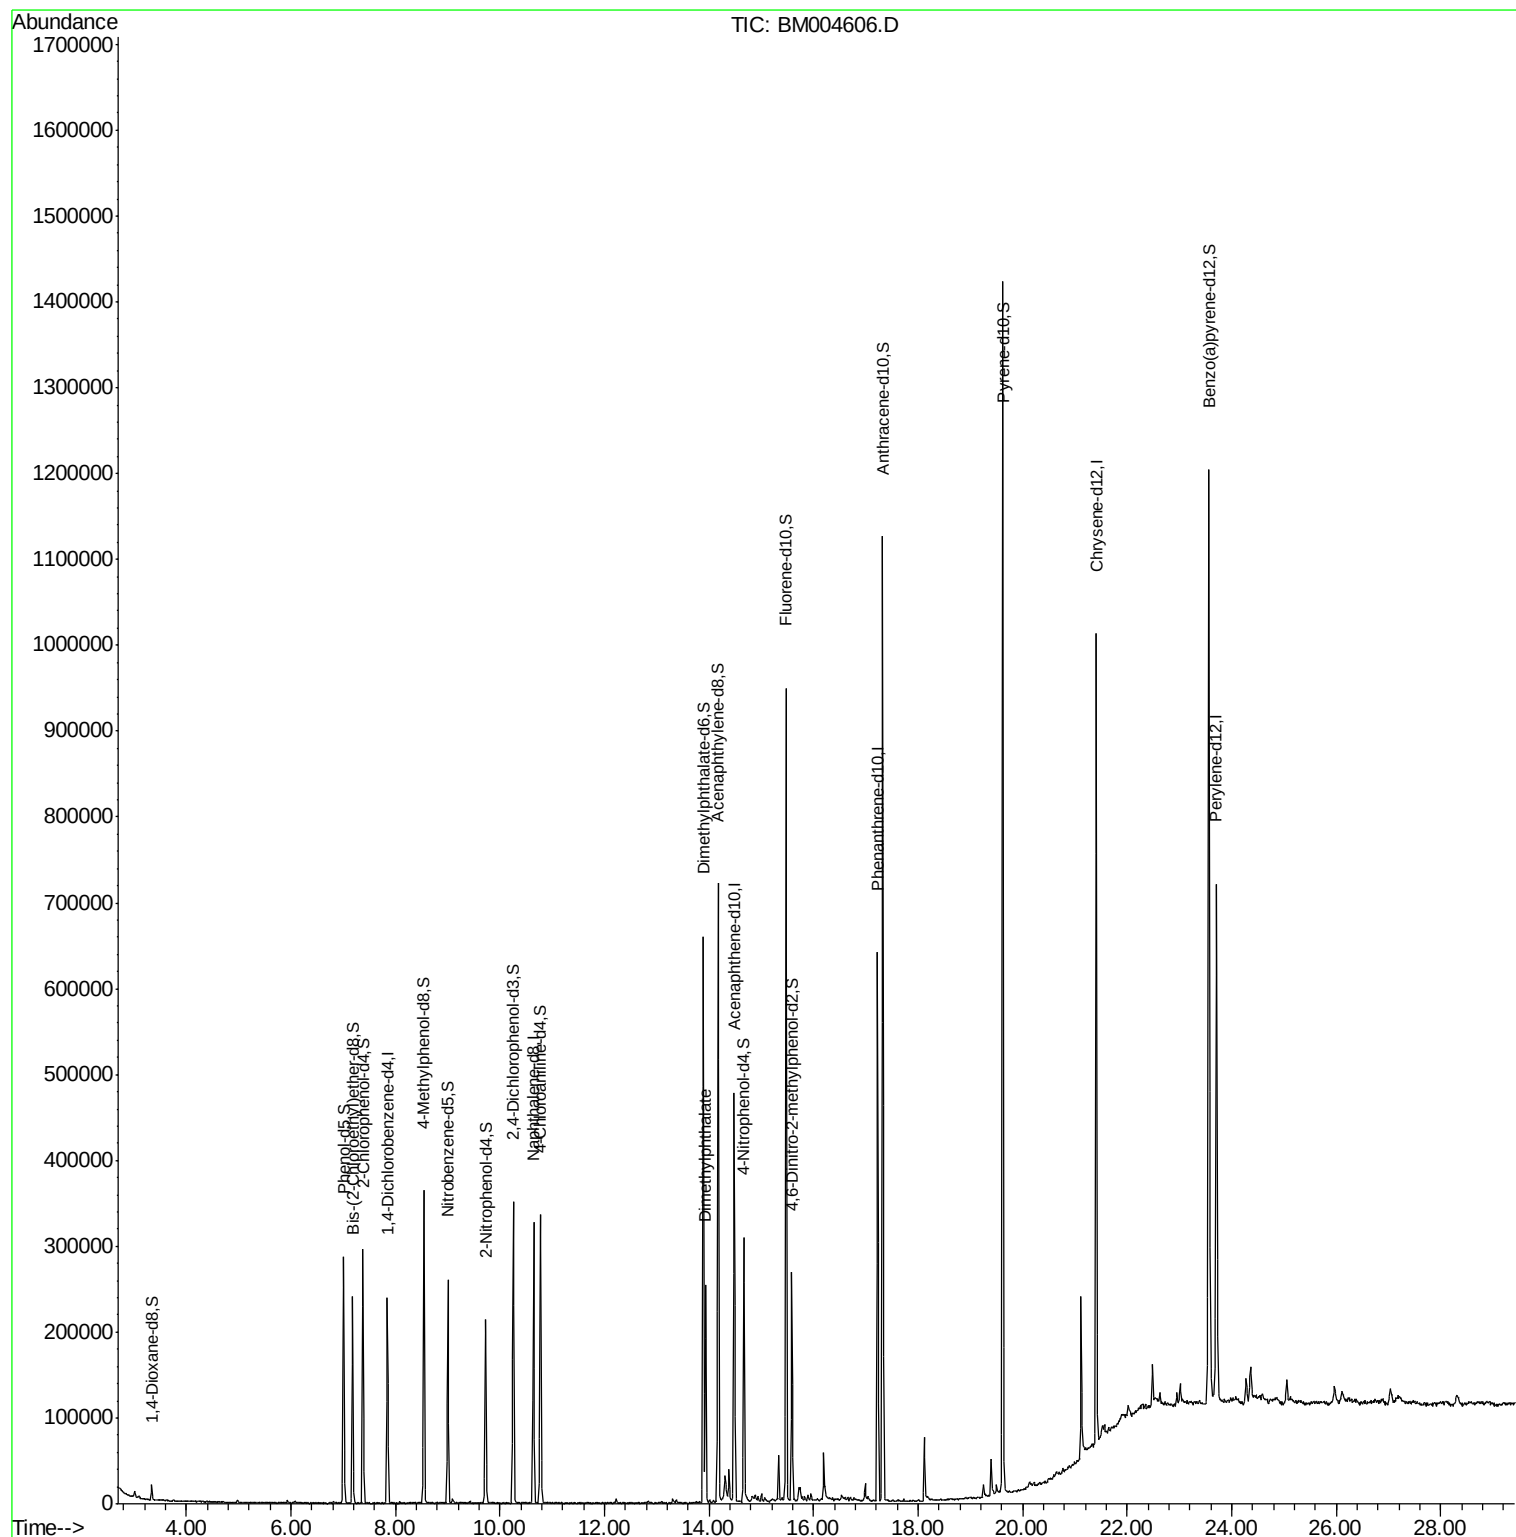

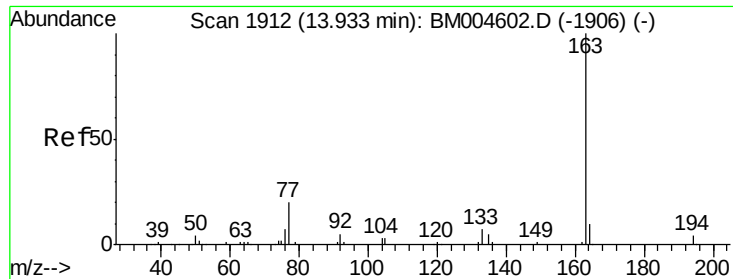

#45

Dimethylphthalate

Concen: 12.35 ng/ul

RT: 13.93 min Scan# 1912

Delta R.T. 0.00 min

Lab File: BM004606.D

Acq: 15 Mar 2016 20:10

Instrument :

BNA_M

ClientSampleId :

MS-DS-E70


Tot Ion:163 Resp: 154758

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 10.4 7.8 11.8

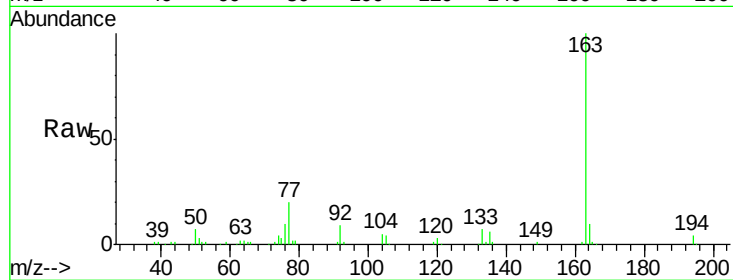

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

