

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031516\
 Data File : BM004609.D
 Acq On : 15 Mar 2016 21:58
 Operator : UM/SJ
 Sample : H1710-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MS-SS-E210

Quant Time: Mar 16 05:57:44 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM031516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 16 05:57:50 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	65991	20.00	ng/ul	0.00
18) Naphthalene-d8	10.64	136	286439	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.48	164	165452	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.22	188	392081	20.00	ng/ul	0.00
78) Chrysene-d12	21.40	240	470368	20.00	ng/ul	0.00
86) Perylene-d12	23.70	264	470604	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.34	96	5789	3.03	ng/uL	0.00
5) Phenol-d5	7.00	99	105220	19.41	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.18	67	64150	20.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.38	132	85972	19.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.54	113	82116	18.79	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	38357	19.25	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	40725	18.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	79023	18.72	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	108430	21.47	ng/ul	0.00
44) Dimethylphthalate-d6	13.89	166	267149	20.65	ng/ul	0.00
47) Acenaphthylene-d8	14.17	160	320259	20.20	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	38923	15.57	ng/ul	0.00
58) Fluorene-d10	15.47	176	241197	21.40	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.58	200	28035	13.61	ng/ul	0.00
71) Anthracene-d10	17.32	188	382170	21.17	ng/ul	0.00
79) Pyrene-d10	19.61	212	406085	18.91	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.55	264	351793	16.74	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.93	163	95314	7.26	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031516\
Data File : BM004609.D
Acq On : 15 Mar 2016 21:58
Operator : UM/SJ
Sample : H1710-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MS-SS-E210

Quant Time: Mar 16 05:57:44 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 16 05:57:50 2016
Response via : Initial Calibration

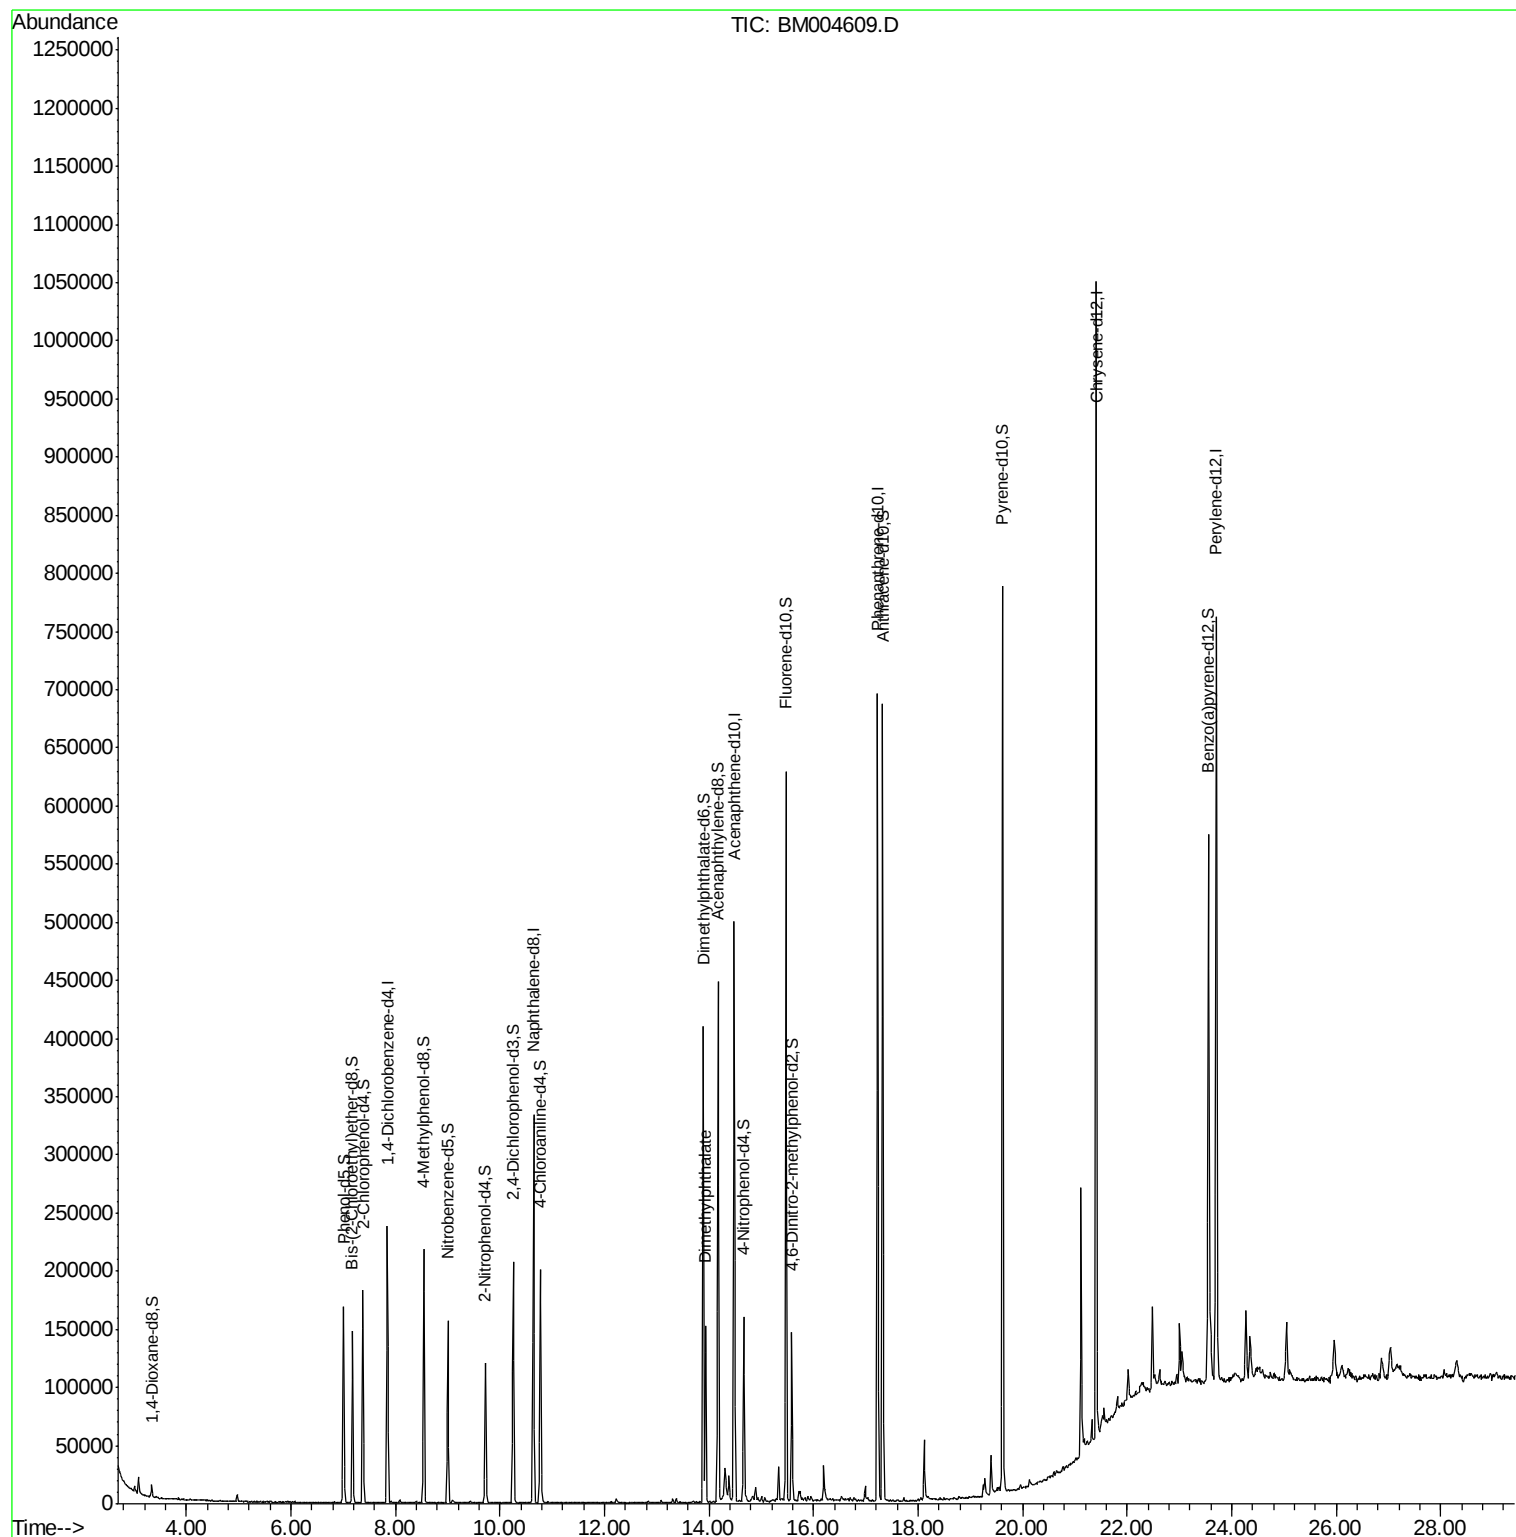

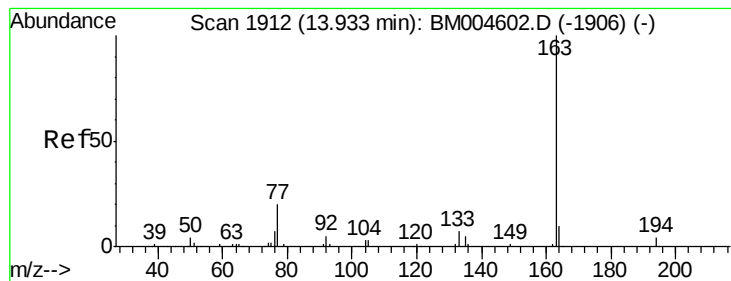

#45
 Dimethylphthalate
 Concen: 7.26 ng/ul
 RT: 13.93 min Scan# 1912
 Delta R.T. 0.00 min
 Lab File: BM004609.D
 Acq: 15 Mar 2016 21:58

Instrument :
 BNA_M
 ClientSampleId :
 MS-SS-E210

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.2	4.8
164	10.1	7.8	11.8

