

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
 Data File : BM004607.D
 Acq On : 15 Mar 2016 20:46
 Operator : UM/SJ
 Sample : H1710-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MS-SS-E140

Quant Time: Mar 16 05:57:28 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 16 05:57:50 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	61533	20.00	ng/ul	0.00
18) Naphthalene-d8	10.64	136	265108	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.48	164	150992	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.22	188	349080	20.00	ng/ul	0.00
78) Chrysene-d12	21.40	240	416585	20.00	ng/ul	0.00
86) Perylene-d12	23.70	264	418352	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.33	96	5016	2.81	ng/uL	0.00
5) Phenol-d5	7.00	99	94419	18.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	57073	19.91	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	78127	19.19	ng/ul	0.00
13) 4-Methylphenol-d8	8.54	113	75628	18.56	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	33791	18.33	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	35977	18.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	70849	18.14	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	98926	21.16	ng/ul	0.00
44) Dimethylphthalate-d6	13.89	166	234733	19.89	ng/ul	0.00
47) Acenaphthylene-d8	14.17	160	283651	19.60	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	35080	15.37	ng/ul	0.00
58) Fluorene-d10	15.47	176	213193	20.72	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.58	200	24693	13.46	ng/ul	0.00
71) Anthracene-d10	17.32	188	334963	20.84	ng/ul	0.00
79) Pyrene-d10	19.61	212	377413	19.85	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.56	264	356140	19.06	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.93	163	76132	6.35	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
Data File : BM004607.D
Acq On : 15 Mar 2016 20:46
Operator : UM/SJ
Sample : H1710-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MS-SS-E140

Quant Time: Mar 16 05:57:28 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 16 05:57:50 2016
Response via : Initial Calibration

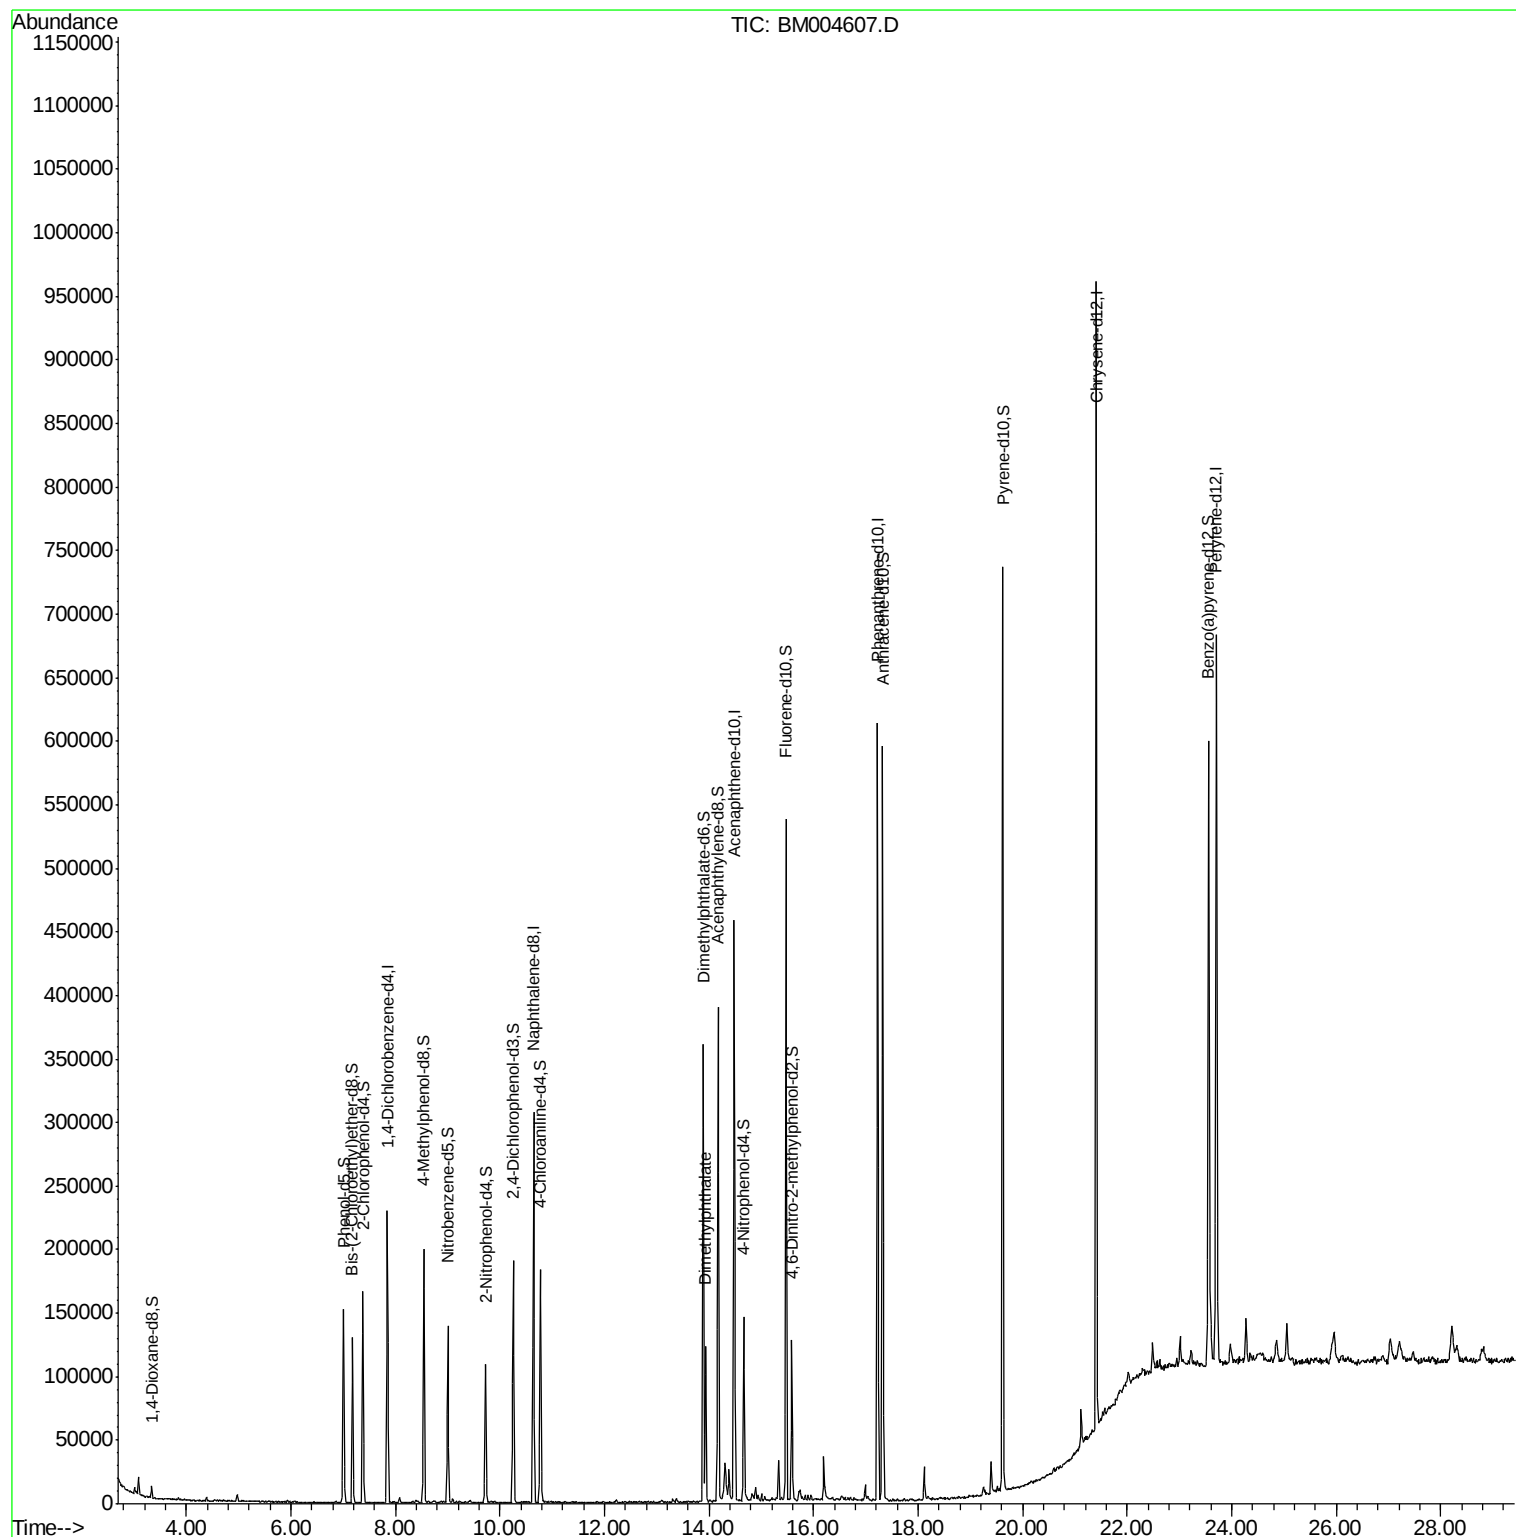


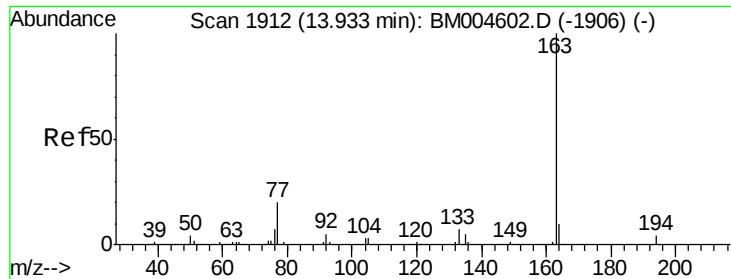

#45
 Dimethylphthalate
 Concen: 6.35 ng/ul
 RT: 13.93 min Scan# 1912
 Delta R.T. -0.00 min
 Lab File: BM004607.D
 Acq: 15 Mar 2016 20:46

Instrument :
 BNA_M
 ClientSampleId :
 MS-SS-E140

Tgt Ion:	163	Resp:	76132
Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.2	4.8
164	9.8	7.8	11.8

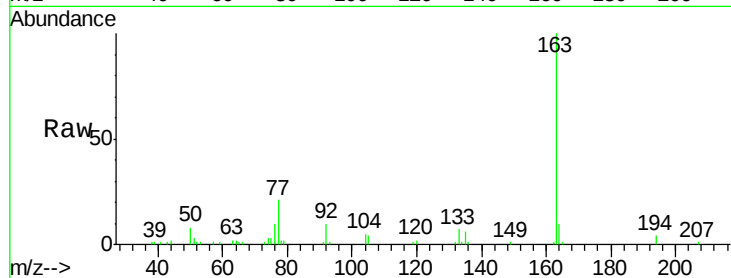

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

