

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
 Data File : BM004613.D
 Acq On : 16 Mar 2016 00:23
 Operator : UM/SJ
 Sample : H1710-13
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MS-DS-D210

Quant Time: Mar 16 05:58:18 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 16 05:57:50 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	54921	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	244115	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.48	164	146379	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.22	188	347079	20.00	ng/ul	0.00
78) Chrysene-d12	21.40	240	406797	20.00	ng/ul	0.00
86) Perylene-d12	23.70	264	398956	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.33	96	6328	3.98	ng/uL	0.00
5) Phenol-d5	7.00	99	122456	27.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	72992	28.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	98114	27.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.54	113	99822	27.44	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	44440	26.18	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	47568	25.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	93986	26.13	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	129716	30.13	ng/ul	0.00
44) Dimethylphthalate-d6	13.89	166	354508	30.98	ng/ul	0.00
47) Acenaphthylene-d8	14.17	160	407949	29.08	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	62218	28.13	ng/ul	0.00
58) Fluorene-d10	15.47	176	312992	31.38	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.58	200	40052	21.96	ng/ul	0.00
71) Anthracene-d10	17.32	188	525984	32.92	ng/ul	0.00
79) Pyrene-d10	19.61	212	630487	33.95	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.55	264	687404	38.58	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.93	163	135255	11.64	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
Data File : BM004613.D
Acq On : 16 Mar 2016 00:23
Operator : UM/SJ
Sample : H1710-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MS-DS-D210

Quant Time: Mar 16 05:58:18 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 16 05:57:50 2016
Response via : Initial Calibration

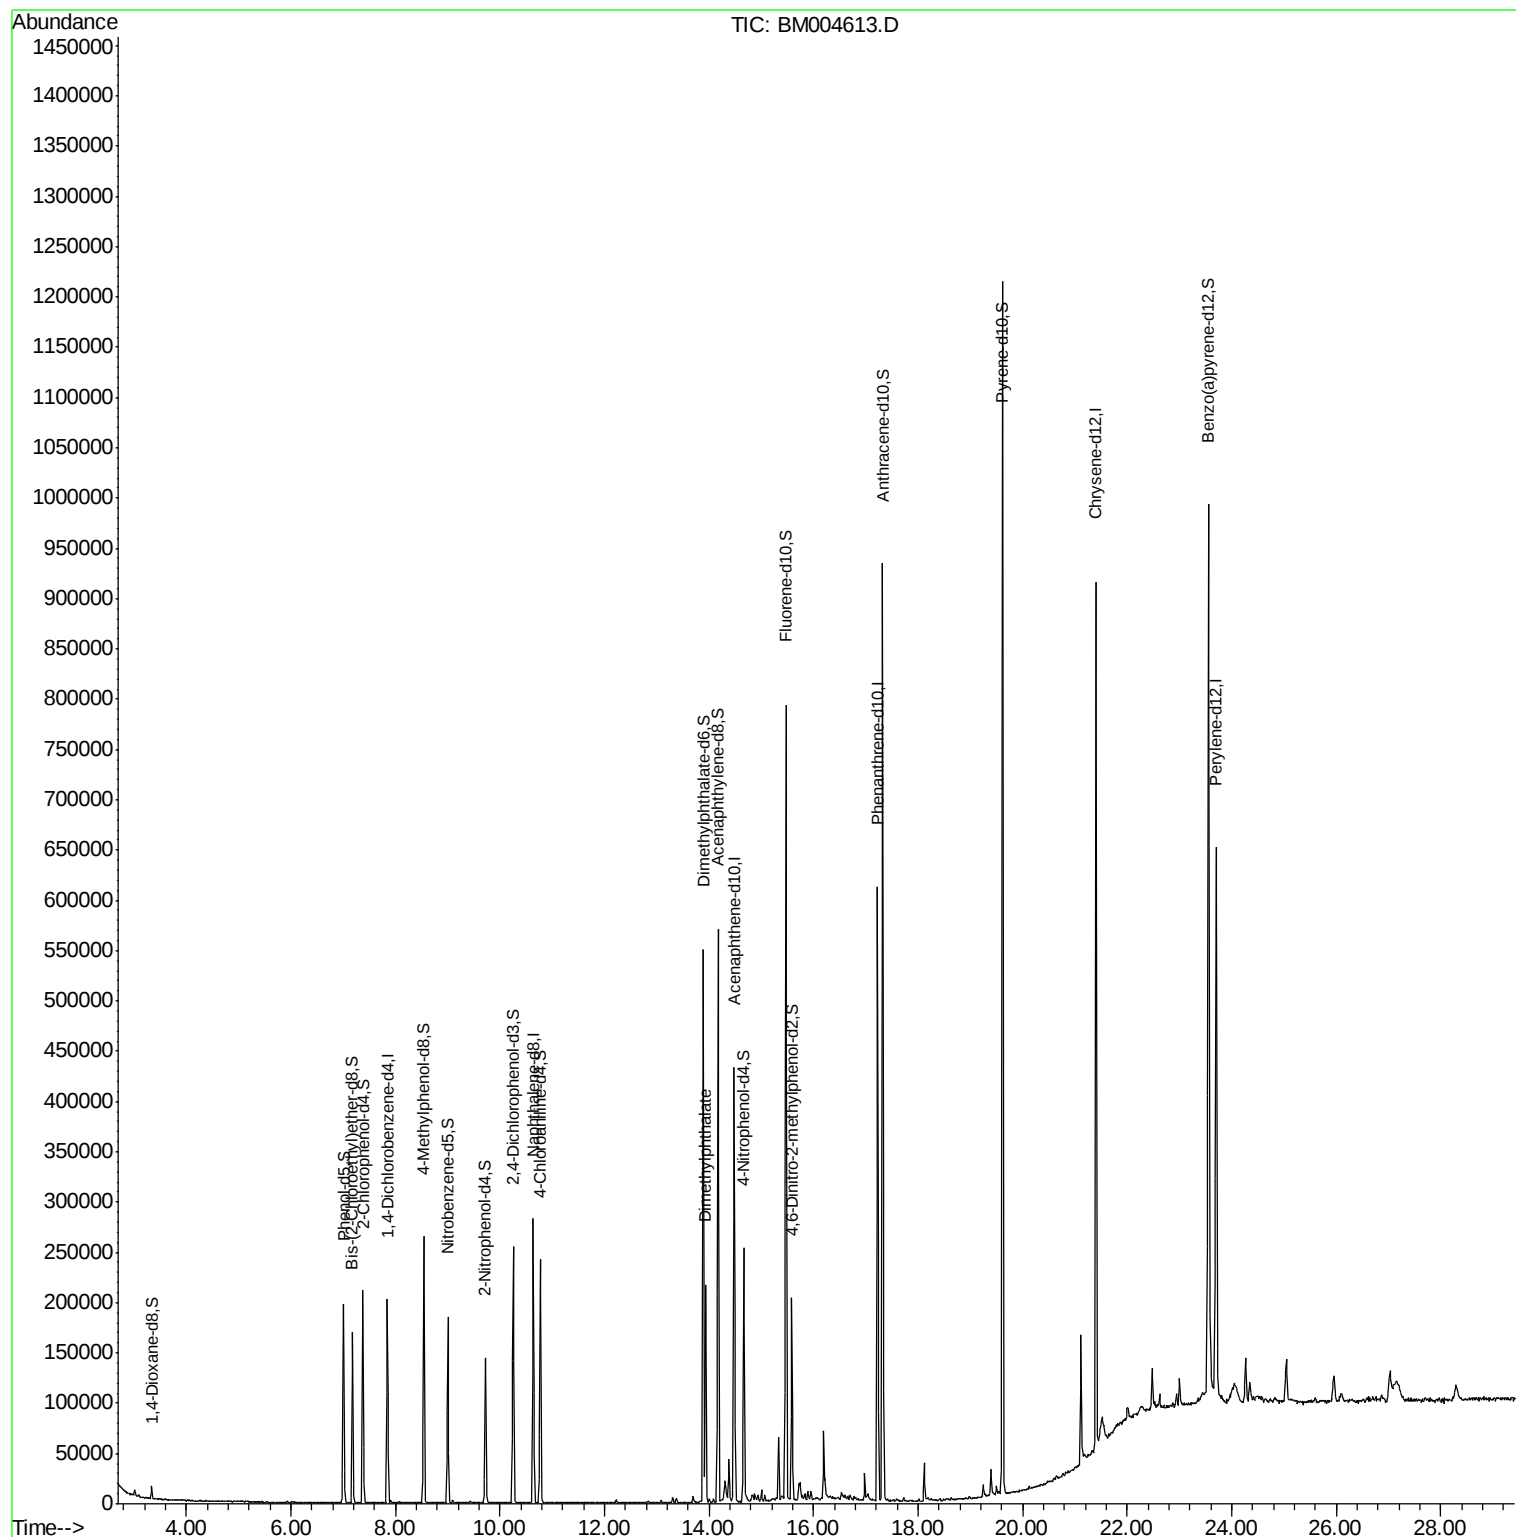


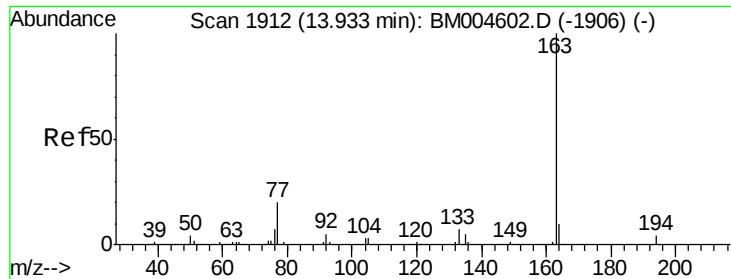

#45
 Dimethylphthalate
 Concen: 11.64 ng/ul
 RT: 13.93 min Scan# 1912
 Delta R.T. -0.00 min
 Lab File: BM004613.D
 Acq: 16 Mar 2016 00:23

Instrument :
 BNA_M
 ClientSampleId :
 MS-DS-D210

Tgt Ion:	163	Resp:	135255
Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.2	4.8
164	10.0	7.8	11.8

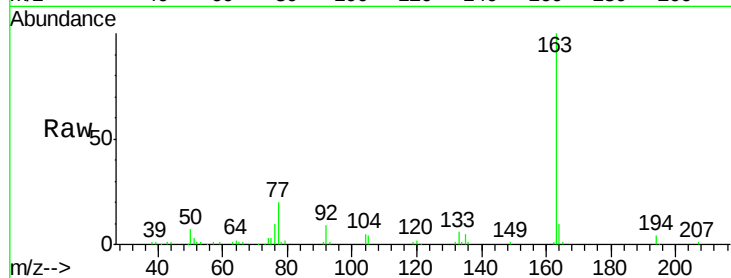

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

