

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
 Data File : BM004619.D
 Acq On : 16 Mar 2016 04:36
 Operator : UM/SJ
 Sample : H1778-20
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC9Z8

Quant Time: Mar 16 07:29:43 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 16 07:32:20 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	82940	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	363106	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.47	164	206594	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.22	188	479200	20.00	ng/ul	0.00
78) Chrysene-d12	21.40	240	575294	20.00	ng/ul	0.00
86) Perylene-d12	23.70	264	576220	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.34	96	10640	4.43	ng/uL	0.00
5) Phenol-d5	7.00	99	205458	30.15	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	121306	31.40	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	163320	29.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.54	113	165059	30.04	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	75005	29.70	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	80180	29.40	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	153359	28.66	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	225397	35.20	ng/ul	0.00
44) Dimethylphthalate-d6	13.89	166	493198	30.54	ng/ul	0.00
47) Acenaphthylene-d8	14.17	160	614170	31.02	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	81152	25.99	ng/ul	0.00
58) Fluorene-d10	15.47	176	446873	31.75	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.58	200	49866	19.80	ng/ul	0.00
71) Anthracene-d10	17.32	188	713463	32.34	ng/ul	0.00
79) Pyrene-d10	19.61	212	826328	31.47	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.56	264	924229	35.91	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.93	163	154703	9.44	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
Data File : BM004619.D
Acq On : 16 Mar 2016 04:36
Operator : UM/SJ
Sample : H1778-20
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC9Z8

Quant Time: Mar 16 07:29:43 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 16 07:32:20 2016
Response via : Initial Calibration

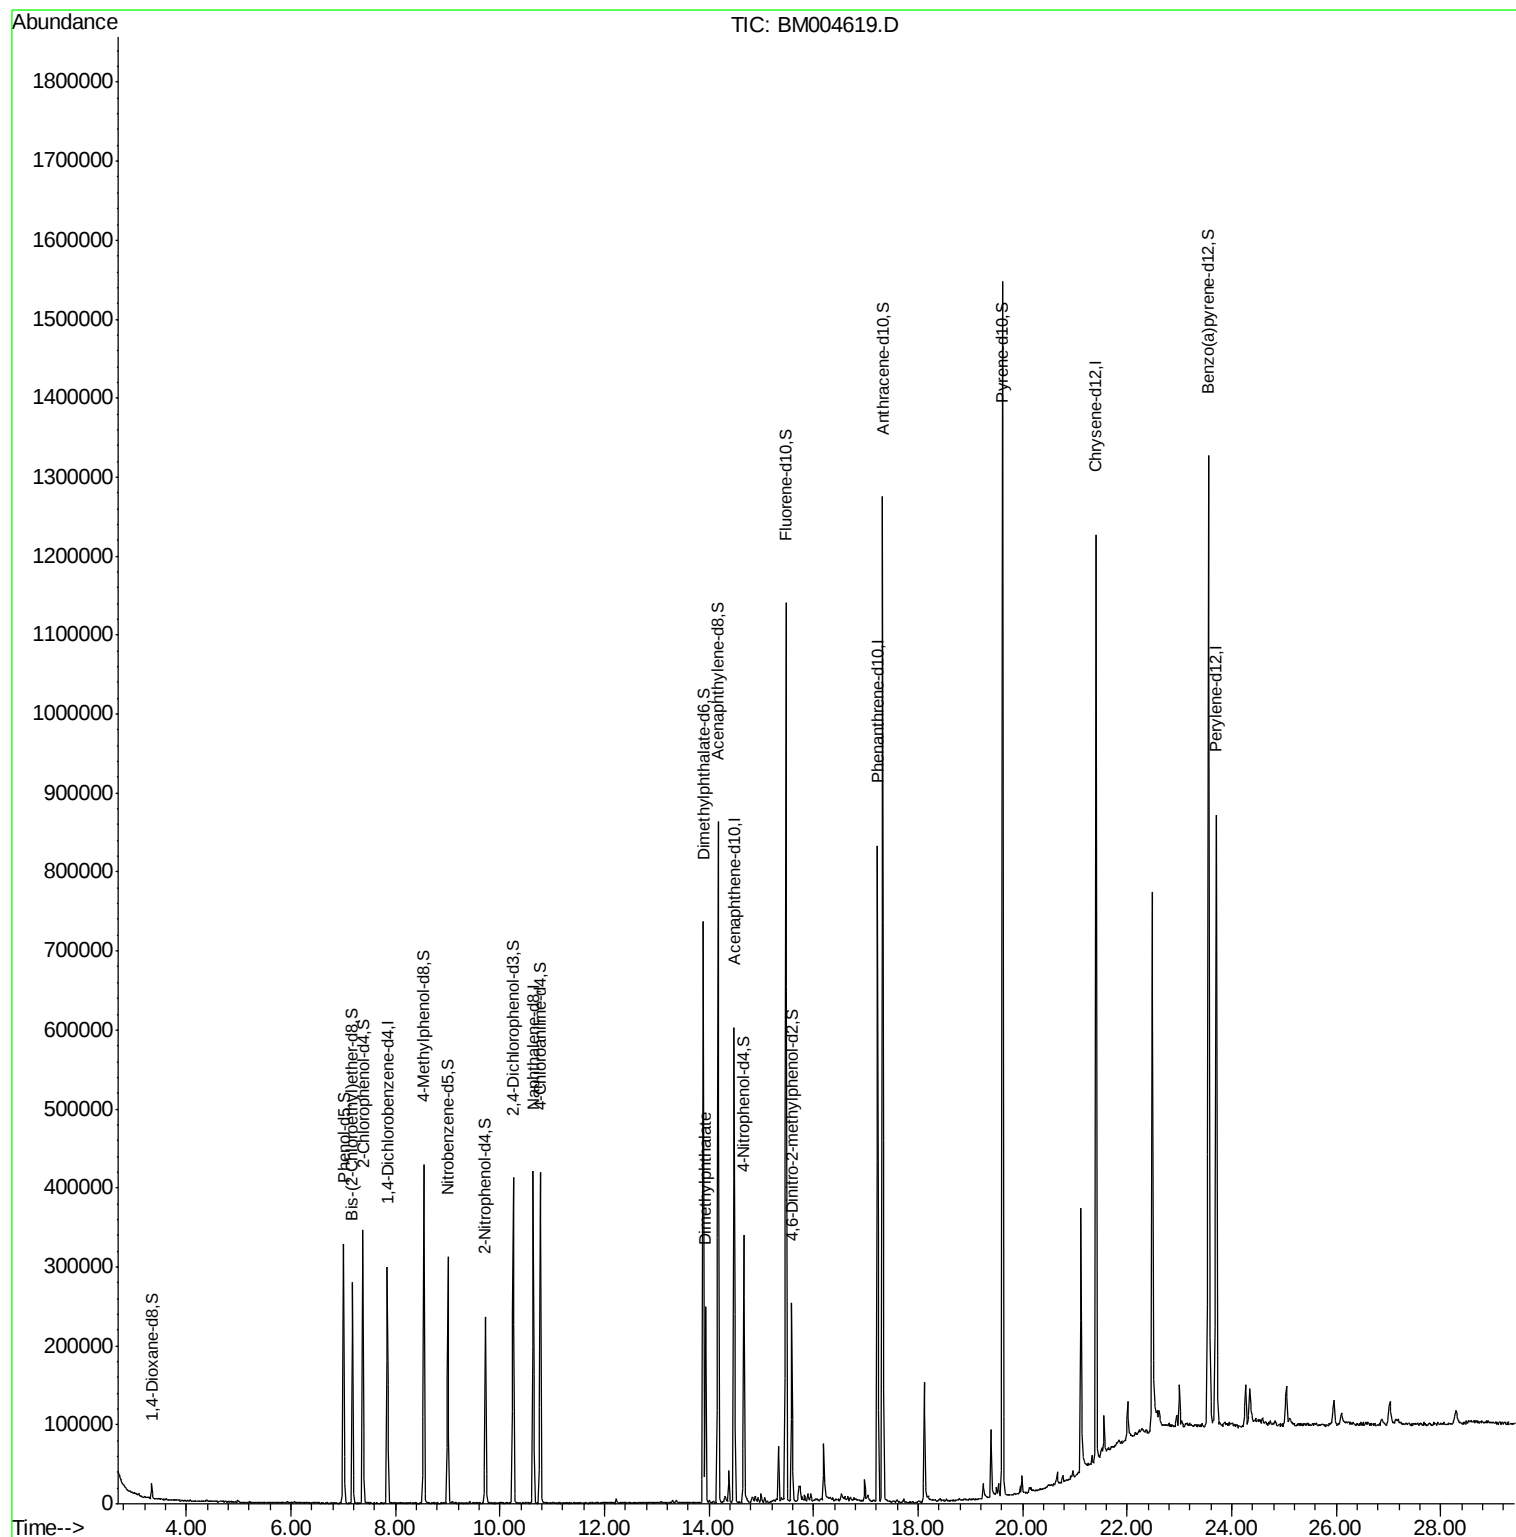

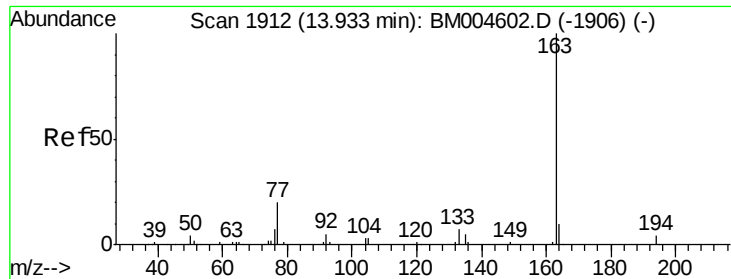

#45

Dimethylphthalate

Concen: 9.44 ng/ul

RT: 13.93 min Scan# 1912

Delta R.T. -0.00 min

Lab File: BM004619.D

Acq: 16 Mar 2016 04:36

Instrument :

BNA_M

ClientSampleId :

BC9Z8


Tgt Ion:163 Resp: 154703

Ion Ratio Lower Upper

163 100

194 4.3 3.2 4.8

164 9.4 7.8 11.8

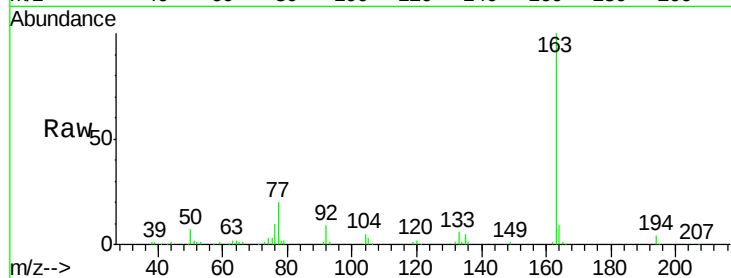

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

