

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
 Data File : BM004620.D
 Acq On : 16 Mar 2016 05:12
 Operator : UM/SJ
 Sample : H1779-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BCA09

Quant Time: Mar 16 07:29:50 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 16 07:32:20 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	68293	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	294514	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.47	164	165586	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.22	188	368683	20.00	ng/ul	0.00
78) Chrysene-d12	21.40	240	413782	20.00	ng/ul	0.00
86) Perylene-d12	23.70	264	412413	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.33	96	6089	3.08	ng/uL	0.00
5) Phenol-d5	7.00	99	117744	20.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	71788	22.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	95254	21.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.54	113	92388	20.42	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	42013	20.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	44329	20.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	87716	20.21	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	126985	24.45	ng/ul	0.00
44) Dimethylphthalate-d6	13.89	166	277842	21.46	ng/ul	0.00
47) Acenaphthylene-d8	14.17	160	345301	21.76	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	37875	15.14	ng/ul	0.00
58) Fluorene-d10	15.47	176	254073	22.52	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.58	200	24023	12.40	ng/ul	0.00
71) Anthracene-d10	17.32	188	391790	23.08	ng/ul	0.00
79) Pyrene-d10	19.61	212	443657	23.49	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.55	264	470575	25.55	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.93	163	118500	9.02	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
Data File : BM004620.D
Acq On : 16 Mar 2016 05:12
Operator : UM/SJ
Sample : H1779-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BCA09

Quant Time: Mar 16 07:29:50 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 16 07:32:20 2016
Response via : Initial Calibration

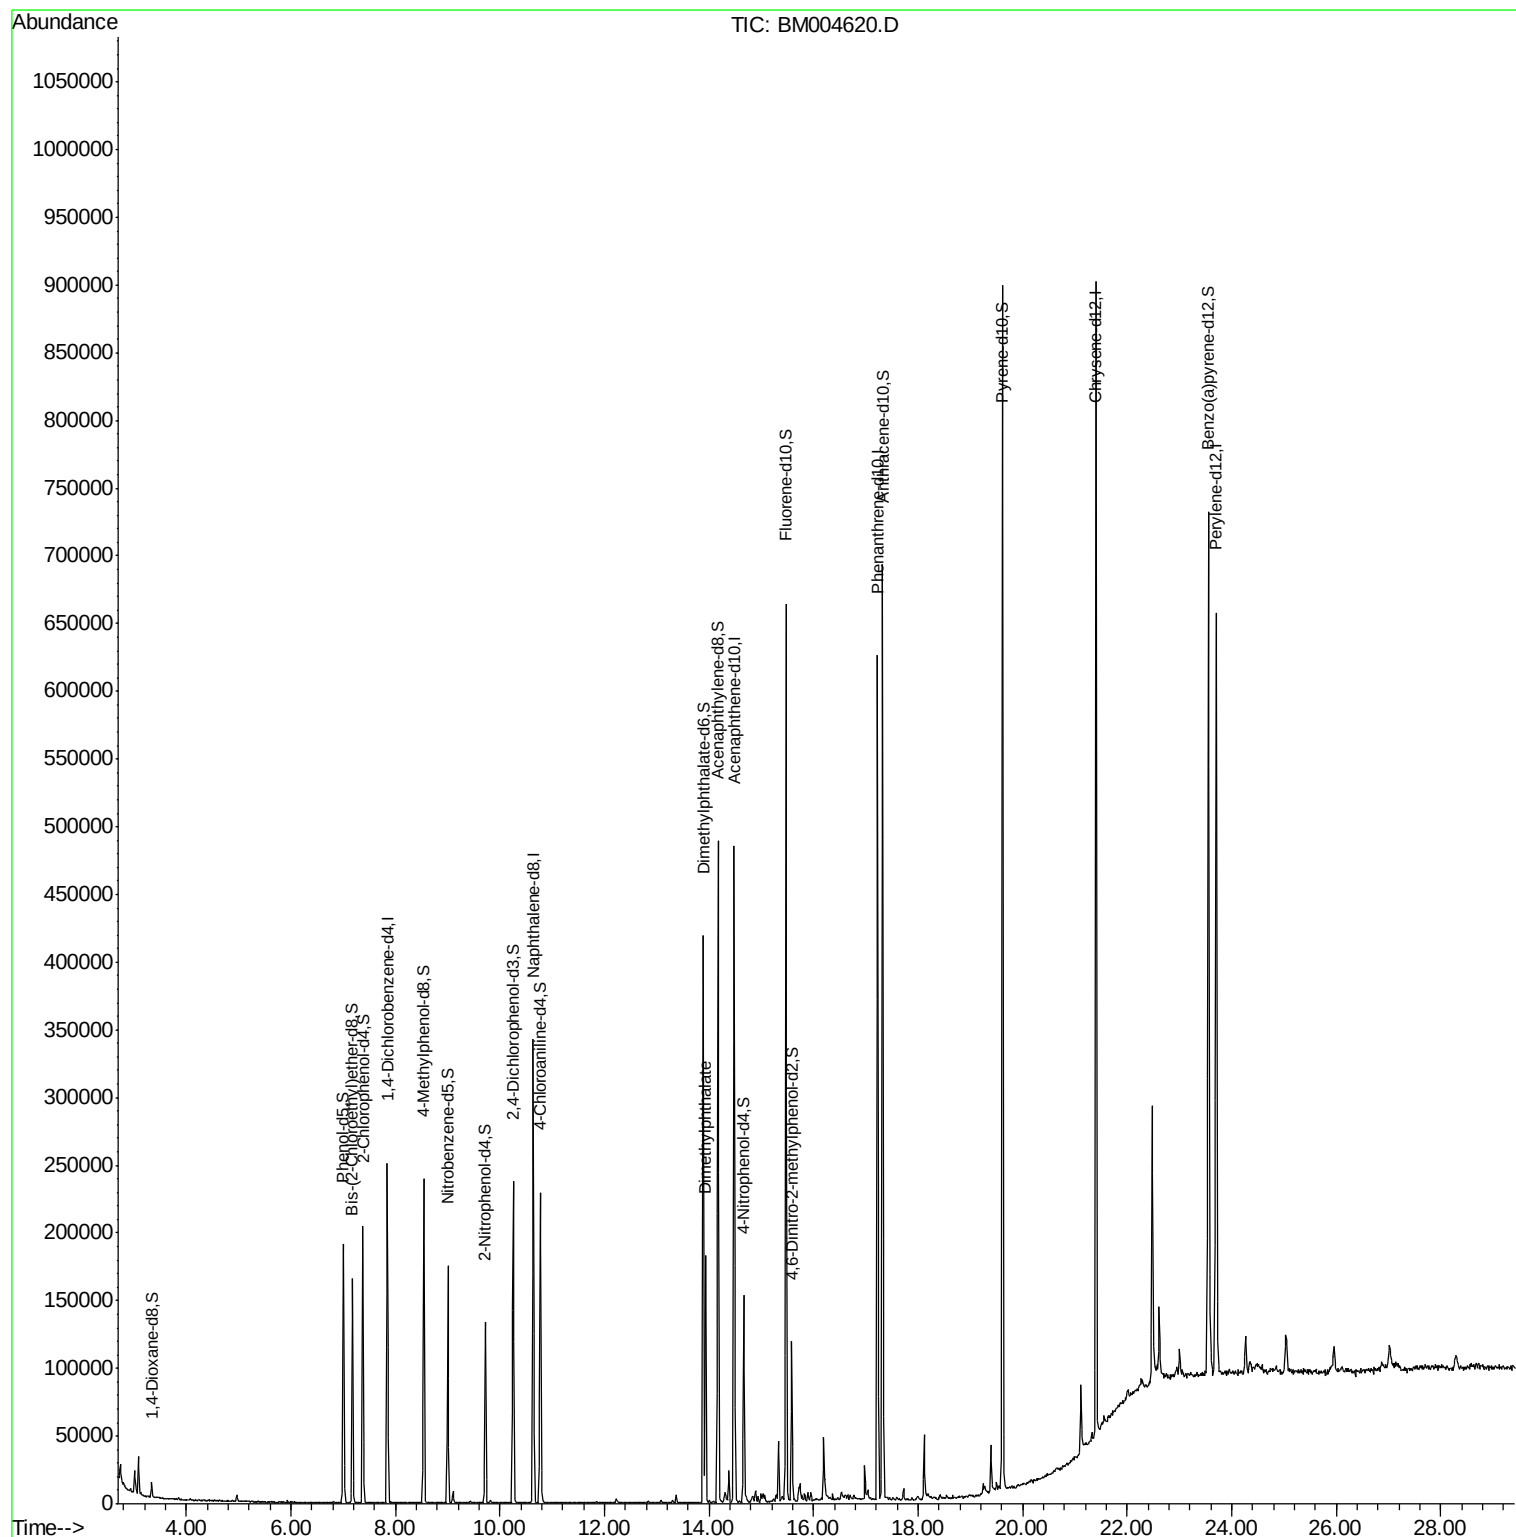

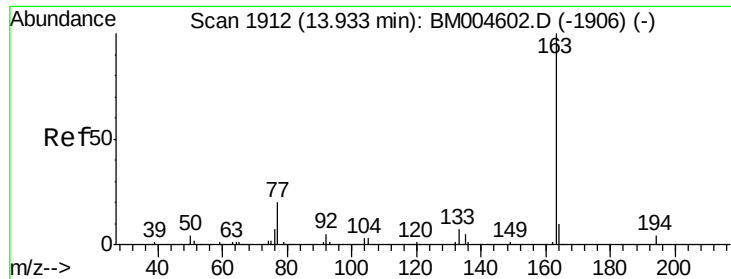

#45

Dimethylphthalate

Concen: 9.02 ng/ul

RT: 13.93 min Scan# 1912

Delta R.T. -0.00 min

Lab File: BM004620.D

Acq: 16 Mar 2016 05:12

Instrument :

BNA_M

ClientSampleId :

BCA09


Tgt Ion:163 Resp: 118500

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 10.2 7.8 11.8

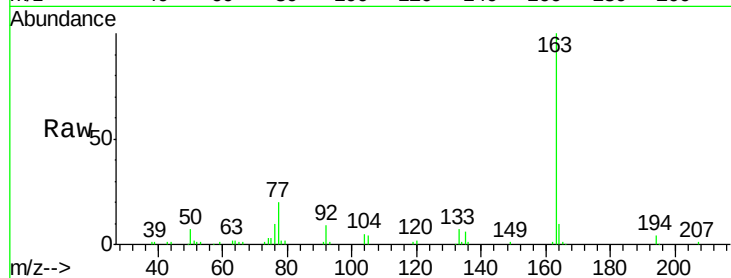

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

