

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
 Data File : BM004624.D
 Acq On : 16 Mar 2016 07:36
 Operator : UM/SJ
 Sample : H1779-22 5X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BCA21

Quant Time: Mar 16 10:16:00 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 16 07:32:20 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	58766	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	255903	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.47	164	149483	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.22	188	350804	20.00	ng/ul	0.00
78) Chrysene-d12	21.40	240	412104	20.00	ng/ul	0.00
86) Perylene-d12	23.70	264	402829	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.34	96	790	0.46	ng/uL	0.00
5) Phenol-d5	7.00	99	14710	3.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	9668	3.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	12165	3.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.54	113	10563	2.71	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	4282	2.41	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	4210	2.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	10159	2.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	13237	2.93	ng/ul	0.00
44) Dimethylphthalate-d6	13.88	166	35958	3.08	ng/ul	0.00
47) Acenaphthylene-d8	14.17	160	43079	3.01	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	627	0.28	ng/ul	0.00
58) Fluorene-d10	15.47	176	38017	3.73	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.58	200	590	0.32	ng/ul	0.00
71) Anthracene-d10	17.32	188	56717	3.51	ng/ul	0.00
79) Pyrene-d10	19.61	212	70133	3.73	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.55	264	74904	4.16	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.93	163	12819	1.08	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
Data File : BM004624.D
Acq On : 16 Mar 2016 07:36
Operator : UM/SJ
Sample : H1779-22 5X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BCA21

Quant Time: Mar 16 10:16:00 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 16 07:32:20 2016
Response via : Initial Calibration

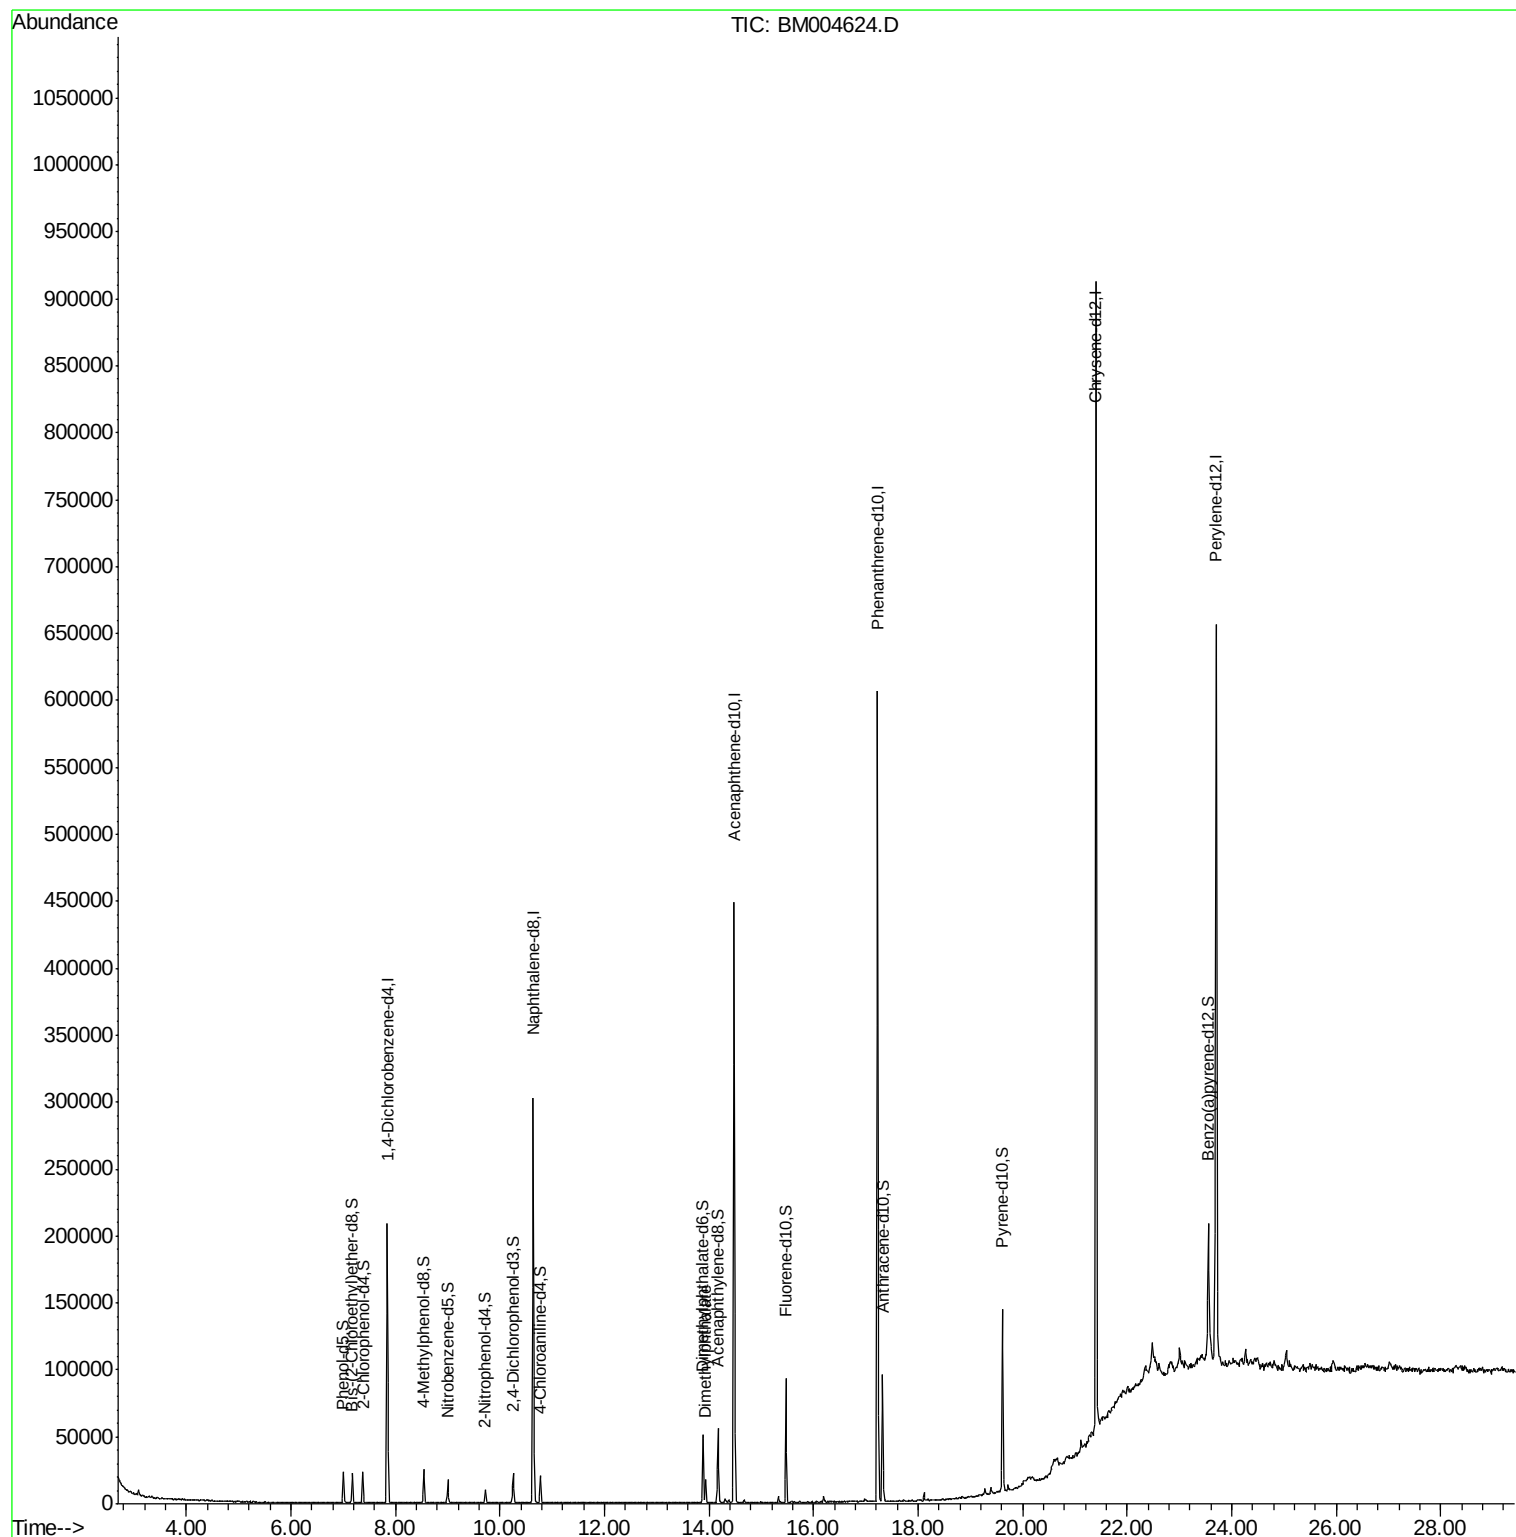

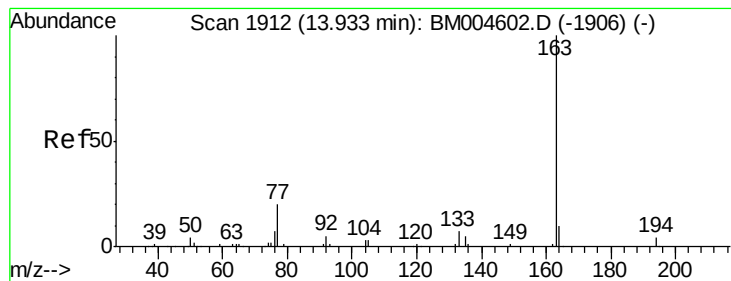

#45
 Dimethylphthalate
 Concen: 1.08 ng/ul
 RT: 13.93 min Scan# 1911
 Delta R.T. -0.01 min
 Lab File: BM004624.D
 Acq: 16 Mar 2016 07:36

Instrument :
 BNA_M
 ClientSampleId :
 BCA21

Tgt Ion:	163	Resp:	12819
Ion	Ratio	Lower	Upper
163	100		
194	3.5	3.2	4.8
164	11.2	7.8	11.8

