

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
 Data File : BM004607.D
 Acq On : 15 Mar 2016 20:46
 Operator : UM/SJ
 Sample : H1710-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MS-SS-E140

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	63	67	77	rVB	14895	18918	1.65%	0.153%
2	3.334	106	110	115	rVB	10068	12716	1.11%	0.103%
3	7.004	728	734	742	rBV	152149	246084	21.42%	1.985%
4	7.175	757	763	771	rBV	129895	203200	17.68%	1.639%
5	7.375	791	797	807	rVB	166141	258468	22.49%	2.085%
6	7.845	869	877	884	rBV	230042	360393	31.36%	2.907%
7	8.539	986	995	1005	rBV	199773	316332	27.53%	2.552%
8	8.998	1066	1073	1080	rBV	138795	228176	19.86%	1.840%
9	9.722	1187	1196	1202	rBV	108316	179503	15.62%	1.448%
10	10.251	1280	1286	1296	rBV	189961	308127	26.81%	2.485%
11	10.639	1345	1352	1360	rVB	307150	525680	45.75%	4.240%
12	10.769	1368	1374	1383	rBV	183052	304710	26.52%	2.458%
13	13.886	1898	1904	1908	rBV	359598	486485	42.34%	3.924%
14	13.933	1908	1912	1921	rVB	122208	164033	14.27%	1.323%
15	14.169	1946	1952	1960	rBV	389046	587147	51.10%	4.736%
16	14.304	1964	1975	1983	rVV2	28743	76016	6.62%	0.613%
17	14.380	1983	1988	1993	rVB	22199	31123	2.71%	0.251%
18	14.480	1998	2005	2013	rVB2	457070	700890	61.00%	5.653%
19	14.663	2029	2036	2049	rBV	144639	220691	19.21%	1.780%
20	14.892	2069	2075	2079	rVB5	9231	15078	1.31%	0.122%
21	15.333	2145	2150	2155	rVB	31215	39653	3.45%	0.320%
22	15.468	2167	2173	2180	rVB	535457	777422	67.66%	6.271%
23	15.580	2186	2192	2198	rBV	124896	165467	14.40%	1.335%
24	15.721	2209	2216	2217	rBV3	8176	14053	1.22%	0.113%
25	16.192	2292	2296	2299	rBV	33745	42959	3.74%	0.347%
26	16.986	2427	2431	2436	rBV2	11910	16568	1.44%	0.134%
27	17.221	2465	2471	2477	rBV	611497	856880	74.57%	6.912%
28	17.321	2482	2488	2497	rBV	592850	850513	74.02%	6.860%
29	18.109	2617	2622	2630	rBV	25615	37591	3.27%	0.303%
30	19.392	2837	2840	2849	rBV2	25417	37456	3.26%	0.302%
31	19.615	2872	2878	2890	rBV	726294	1019280	88.70%	8.222%
32	21.115	3130	3133	3138	rBV3	29478	41191	3.58%	0.332%
33	21.403	3177	3182	3189	rBV	903697	1149094	100.00%	9.269%
34	23.556	3541	3548	3560	rBV	488071	976998	85.02%	7.880%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
Data File : BM004607.D
Acq On : 15 Mar 2016 20:46
Operator : UM/SJ
Sample : H1710-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MS-SS-E140

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Title : SVOA CALIBRATION

35	23.703	3566	3573	3582	rVB2	570154	1128795	98.23%	9.105%
----	--------	------	------	------	------	--------	---------	--------	--------


Sum of corrected areas: 12397690

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
Data File : BM004607.D
Acq On : 15 Mar 2016 20:46
Operator : UM/SJ
Sample : H1710-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MS-SS-E140

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

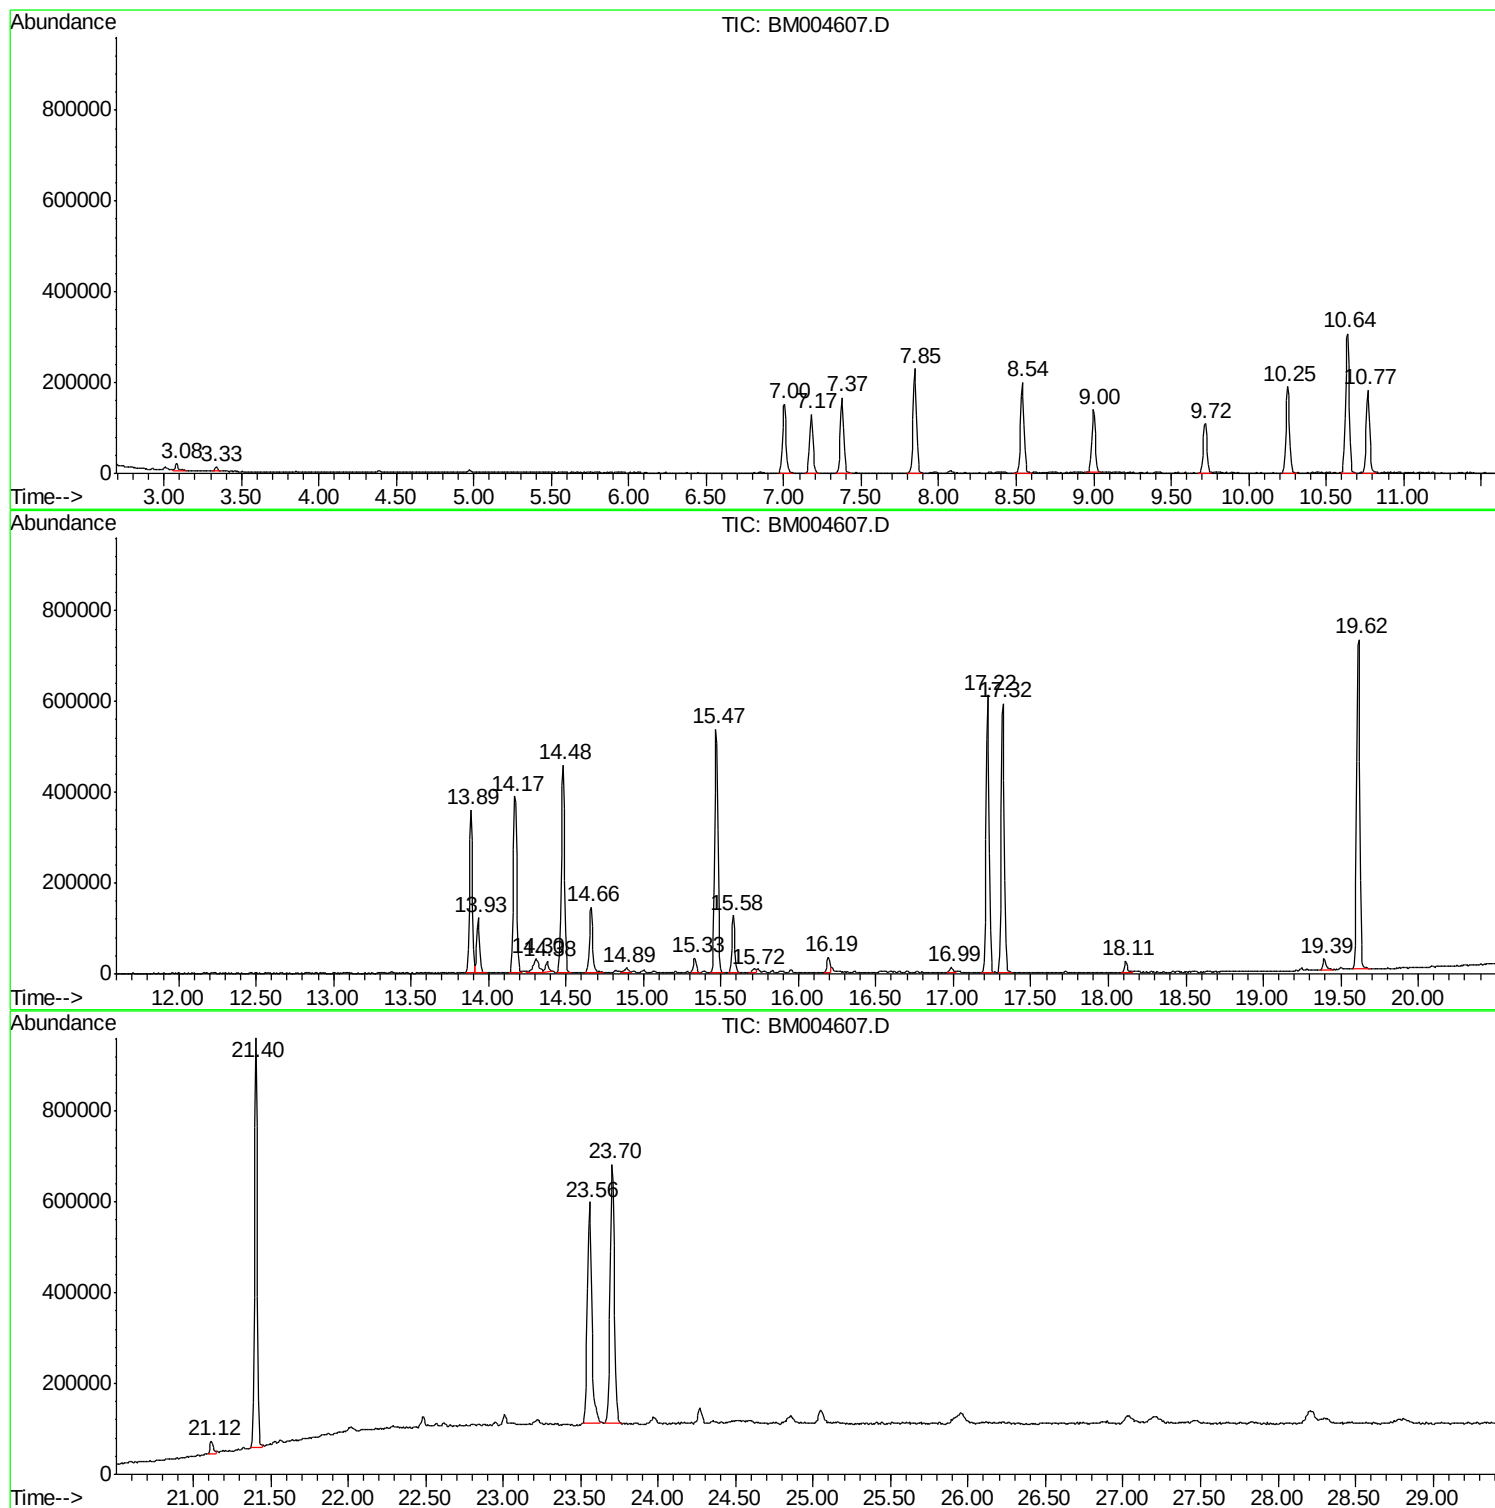

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
Data File : BM004607.D
Acq On : 15 Mar 2016 20:46
Operator : UM/SJ
Sample : H1710-05
Misc :
ALS Vial : 16 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
MS-SS-E140

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1,6-Anhydro-.beta.-D-glucop... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
14.30	2.17 ng/ul	76016	Acenaphthene-d10	14.48	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	1,6-Anhydro-.beta.-D-glucopyrano...	162	C6H10O5	000498-07-7	64
2	3,4-Altrosan	162	C6H10O5	1000129-76-4	38
3	Hexanoic acid, 6-bromo-	194	C6H11BrO2	004224-70-8	38
4	.beta.-Methyl xyloside	164	C6H12O5	1000130-04-0	36
5	Butanoic acid	88	C4H8O2	000107-92-6	33

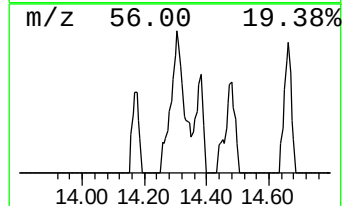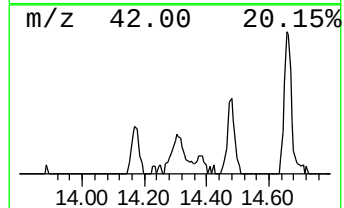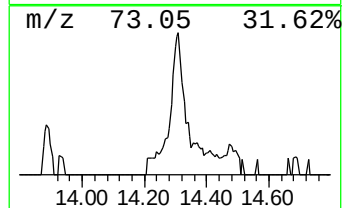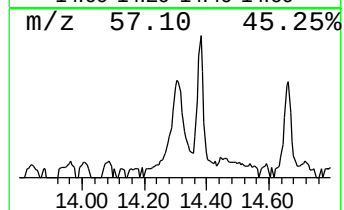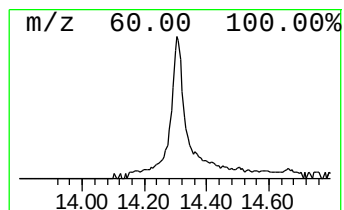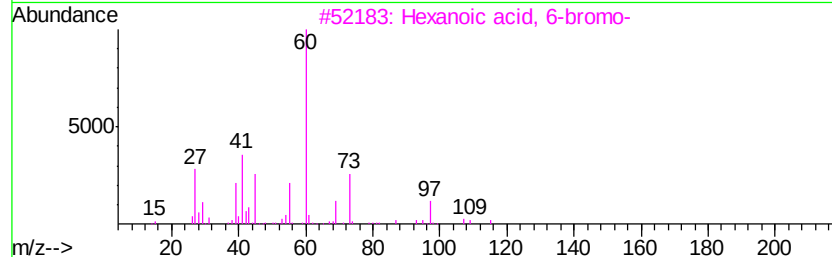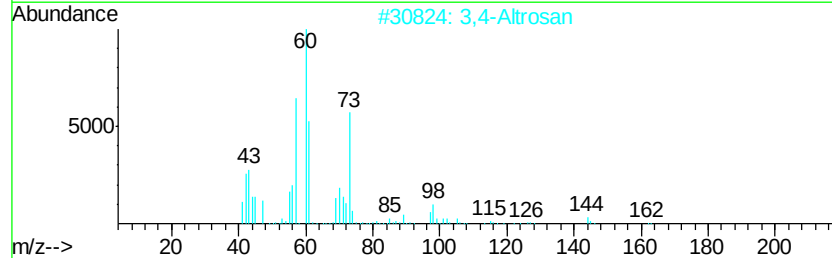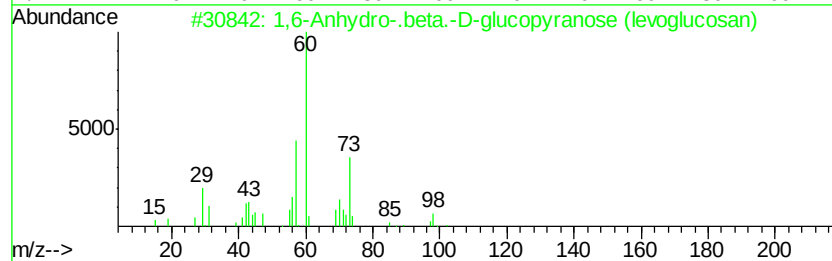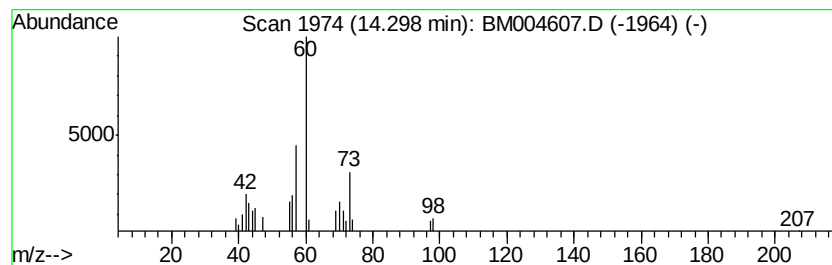

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
Data File : BM004607.D
Acq On : 15 Mar 2016 20:46
Operator : UM/SJ
Sample : H1710-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MS-SS-E140

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
1,6-Anhydro-.beta...	14.30	2.2	ng/ul	76016	3	14.48	700890	20.0