

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
 Data File : BM004615.D
 Acq On : 16 Mar 2016 01:35
 Operator : UM/SJ
 Sample : H1710-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MS-SS-I210

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	63	67	72	rVB	16343	19754	1.55%	0.135%
2	3.334	107	110	116	rVB	12407	15586	1.22%	0.106%
3	4.969	384	388	394	rBV2	8855	13415	1.05%	0.092%
4	7.004	726	734	742	rBV	183363	295599	23.16%	2.017%
5	7.175	757	763	771	rVB	165857	250866	19.66%	1.712%
6	7.375	790	797	805	rVB	205069	313501	24.57%	2.139%
7	7.845	870	877	884	rBV	253752	402773	31.56%	2.748%
8	8.539	988	995	1004	rVB	227022	356766	27.96%	2.434%
9	8.998	1067	1073	1083	rBV	168637	272786	21.38%	1.861%
10	9.716	1188	1195	1204	rBV	125766	211016	16.54%	1.440%
11	10.251	1280	1286	1296	rBV	226950	371146	29.08%	2.532%
12	10.633	1344	1351	1359	rBV	337917	577977	45.29%	3.944%
13	10.769	1367	1374	1381	rBV	210099	357931	28.05%	2.442%
14	13.886	1898	1904	1908	rBV	423405	573515	44.94%	3.913%
15	13.933	1908	1912	1920	rVB	171951	232458	18.22%	1.586%
16	14.169	1946	1952	1960	rBV	466810	691751	54.21%	4.720%
17	14.304	1963	1975	1983	rVV2	16231	43461	3.41%	0.297%
18	14.380	1983	1988	1992	rVV	20348	29415	2.31%	0.201%
19	14.480	1996	2005	2012	rVB2	481973	747919	58.61%	5.103%
20	14.657	2029	2035	2048	rBV	127061	197860	15.51%	1.350%
21	14.892	2069	2075	2079	rBV3	17666	27193	2.13%	0.186%
22	15.327	2145	2149	2155	rVB	31357	40377	3.16%	0.275%
23	15.468	2167	2173	2179	rBV	650432	926439	72.60%	6.321%
24	15.580	2186	2192	2198	rBV	125282	165908	13.00%	1.132%
25	15.715	2208	2215	2217	rBV3	9584	15745	1.23%	0.107%
26	16.192	2291	2296	2299	rBV	32681	44069	3.45%	0.301%
27	16.980	2424	2430	2435	rBV2	15061	22118	1.73%	0.151%
28	17.221	2465	2471	2475	rBV	626424	905550	70.96%	6.179%
29	17.262	2475	2478	2482	rVV	78293	102351	8.02%	0.698%
30	17.321	2482	2488	2500	rVB	690082	1022375	80.12%	6.976%
31	18.109	2616	2622	2626	rBV2	40335	59362	4.65%	0.405%
32	18.292	2647	2653	2657	rBV3	10346	17207	1.35%	0.117%
33	19.274	2811	2820	2829	rBV	110502	158073	12.39%	1.079%
34	19.392	2836	2840	2846	rBV2	18729	24908	1.95%	0.170%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
Data File : BM004615.D
Acq On : 16 Mar 2016 01:35
Operator : UM/SJ
Sample : H1710-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MS-SS-I210

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Title : SVOA CALIBRATION

35	19.609	2871	2877	2888	rBV	855469	1243389	97.44%	8.484%
36	20.133	2962	2966	2972	rVB	12981	16705	1.31%	0.114%
37	21.109	3129	3132	3141	rVB4	69234	86467	6.78%	0.590%
38	21.315	3163	3167	3171	rBV	98114	104952	8.22%	0.716%
39	21.397	3175	3181	3186	rVV	940632	1276103	100.00%	8.707%
40	21.433	3186	3187	3192	rVB	50659	46264	3.63%	0.316%
41	23.003	3449	3454	3459	rBV2	75267	143566	11.25%	0.980%
42	23.550	3540	3547	3562	rVB	501068	1042305	81.68%	7.112%
43	23.697	3565	3572	3588	rVB	592312	1189018	93.18%	8.113%


Sum of corrected areas: 14655939

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
Data File : BM004615.D
Acq On : 16 Mar 2016 01:35
Operator : UM/SJ
Sample : H1710-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MS-SS-I210

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

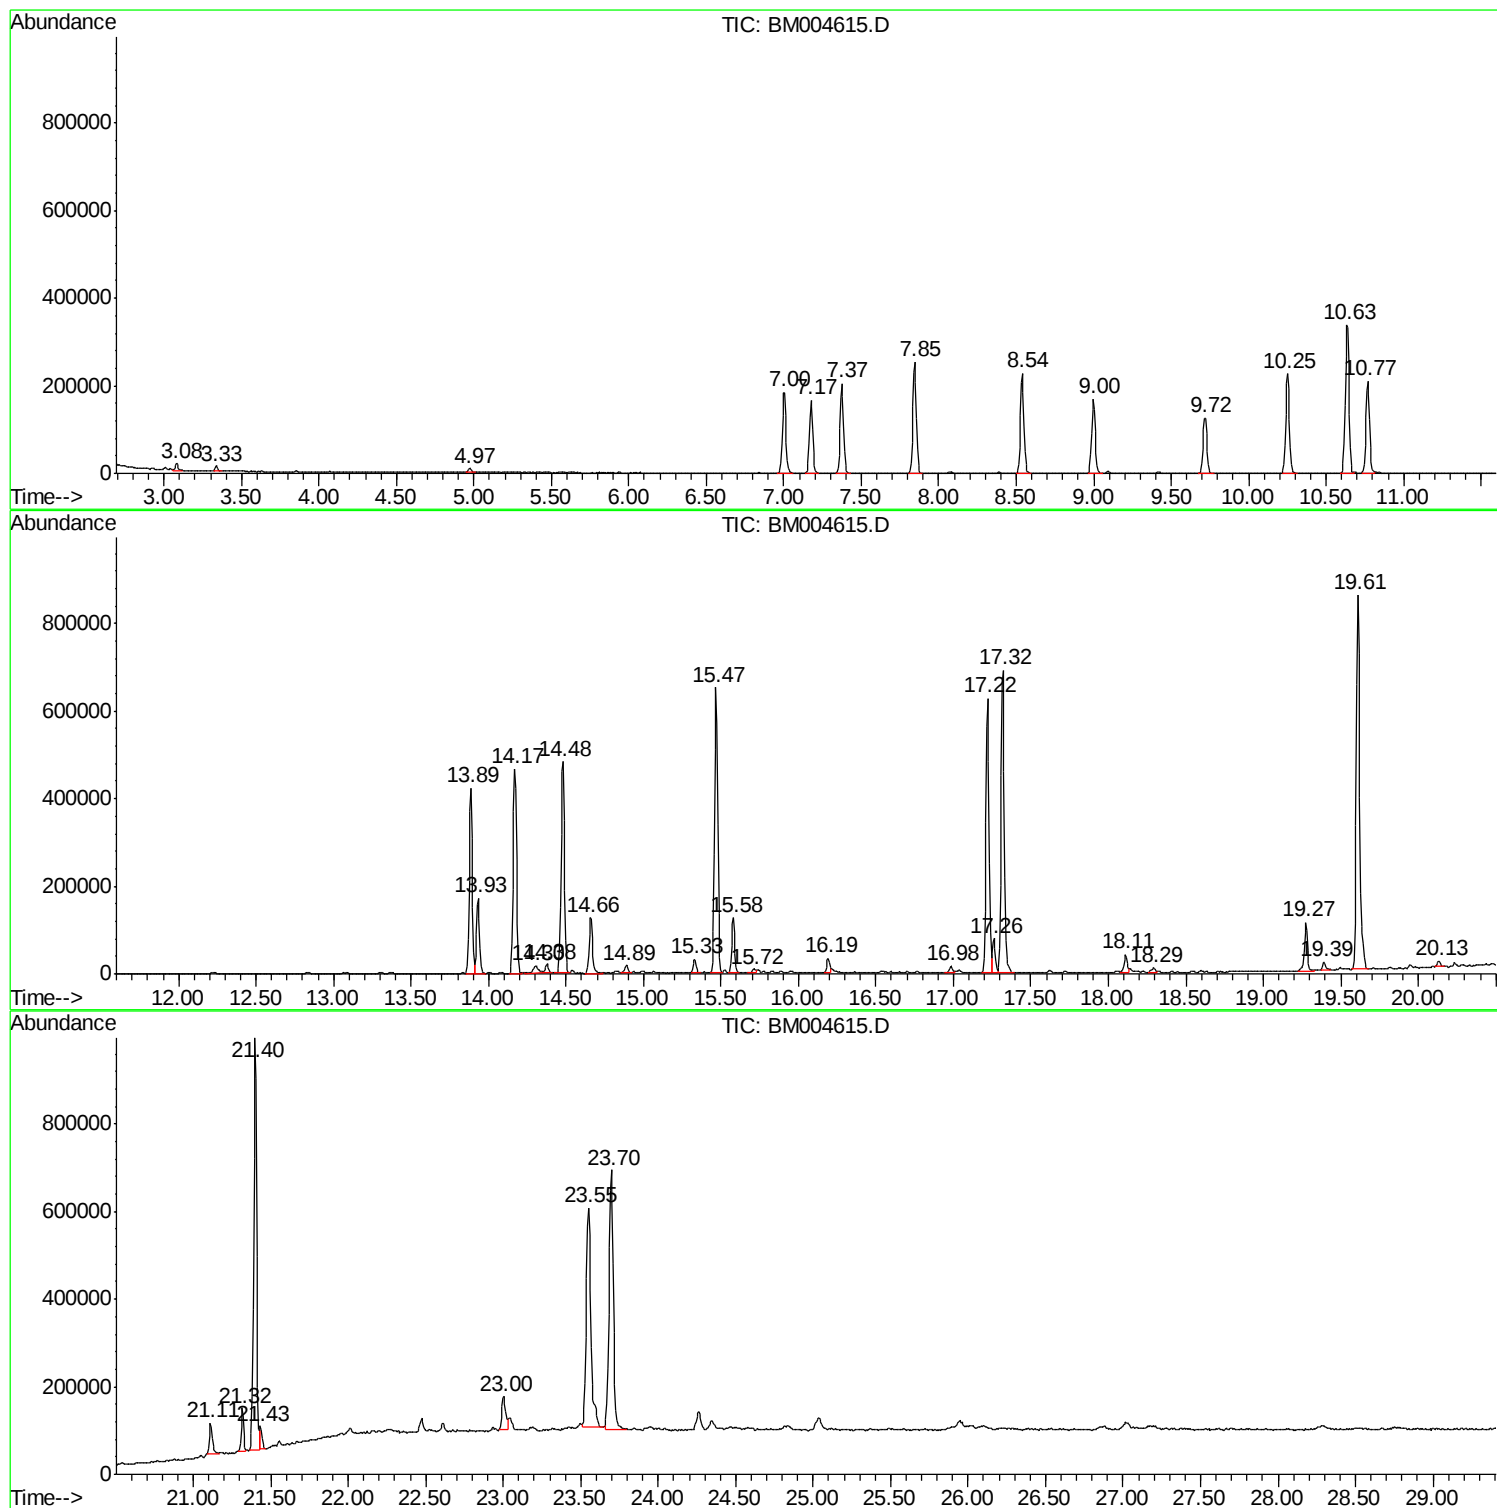

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
Data File : BM004615.D
Acq On : 16 Mar 2016 01:35
Operator : UM/SJ
Sample : H1710-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MS-SS-I210

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031516\
Data File : BM004615.D
Acq On : 16 Mar 2016 01:35
Operator : UM/SJ
Sample : H1710-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MS-SS-I210

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc