

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031517\
 Data File : BM009260.D
 Acq On : 15 Mar 2017 11:32
 Operator : SJ/MA
 Sample : I2235-02RE
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BK7RE

Manual Integrations
 APPROVED

mohammad

3/16/2017 4:40:50 PM

Quant Time: Mar 16 01:25:07 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-2016\SOM-EPA-BM031317M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 16 01:18:23 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.96	152	196520m	20.00	ng/ul	0.08
18) Naphthalene-d8	10.69	136	579448	20.00	ng/ul	0.01
35) Acenaphthene-d10	14.52	164	363392	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.26	188	957083m	20.00	ng/ul	0.00
77) Chrysene-d12	21.44	240	1437371	20.00	ng/ul	0.00
85) Perylene-d12	23.78	264	1464331	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.35	96	15999m	3.59	ng/uL	0.01
5) Phenol-d5	7.04	99	76672	3.61	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.24	67	266939	19.28	ng/ul	0.04
9) 2-Chlorophenol-d4	7.42	132	210818	16.23	ng/ul	0.02
13) 4-Methylphenol-d8	8.59	113	149010	8.79	ng/ul	0.01
19) Nitrobenzene-d5	9.06	128	136629	33.02	ng/ul	0.01
22) 2-Nitrophenol-d4	9.77	143	146642	31.93	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.30	165	279610	28.50	ng/ul	0.00
29) 4-Chloroaniline-d4	10.82	131	16643	1.42	ng/ul	0.00
43) Dimethylphthalate-d6	13.93	166	1044717	37.85	ng/ul	0.00
46) Acenaphthylene-d8	14.22	160	1230082	38.76	ng/ul	0.00
51) 4-Nitrophenol-d4	14.71	143	29792	5.44	ng/ul	0.00
57) Fluorene-d10	15.51	176	919998	37.36	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.63	200	162238	28.33	ng/ul	0.00
70) Anthracene-d10	17.36	188	1582481	34.94	ng/ul	0.00
78) Pyrene-d10	19.66	212	2027602	34.95	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.63	264	2408916	35.96	ng/ul	0.00

Target Compounds

						Ovalue
6) Phenol	7.07	94	28246	1.24	ng/ul#	70
10) 2-Chlorophenol	7.45	128	58823	4.39	ng/ul#	76
20) Nitrobenzene	9.10	77	231956	16.81	ng/ul#	82
23) 2-Nitrophenol	9.80	139	6068	1.21	ng/ul#	81
27) 2,4-Dichlorophenol	10.36	162	83987m	8.65	ng/ul	
36) 1,2,4,5-Tetrachlorobenzene	12.70	216	74845	6.85	ng/ul	99
72) 1,2,3,4-Tetrachlorobenzene	13.31	216	104666	9.31	ng/uL	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031517\
Data File : BM009260.D
Acq On : 15 Mar 2017 11:32
Operator : SJ/MA
Sample : I2235-02RE
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0BK7RE




Manual Integrations
APPROVED

mohammad

3/16/2017 4:40:50 PM

Quant Time: Mar 16 01:25:07 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-2016\SOM-EPA-BM031317
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 16 01:18:23 2017
Response via : Initial Calibration

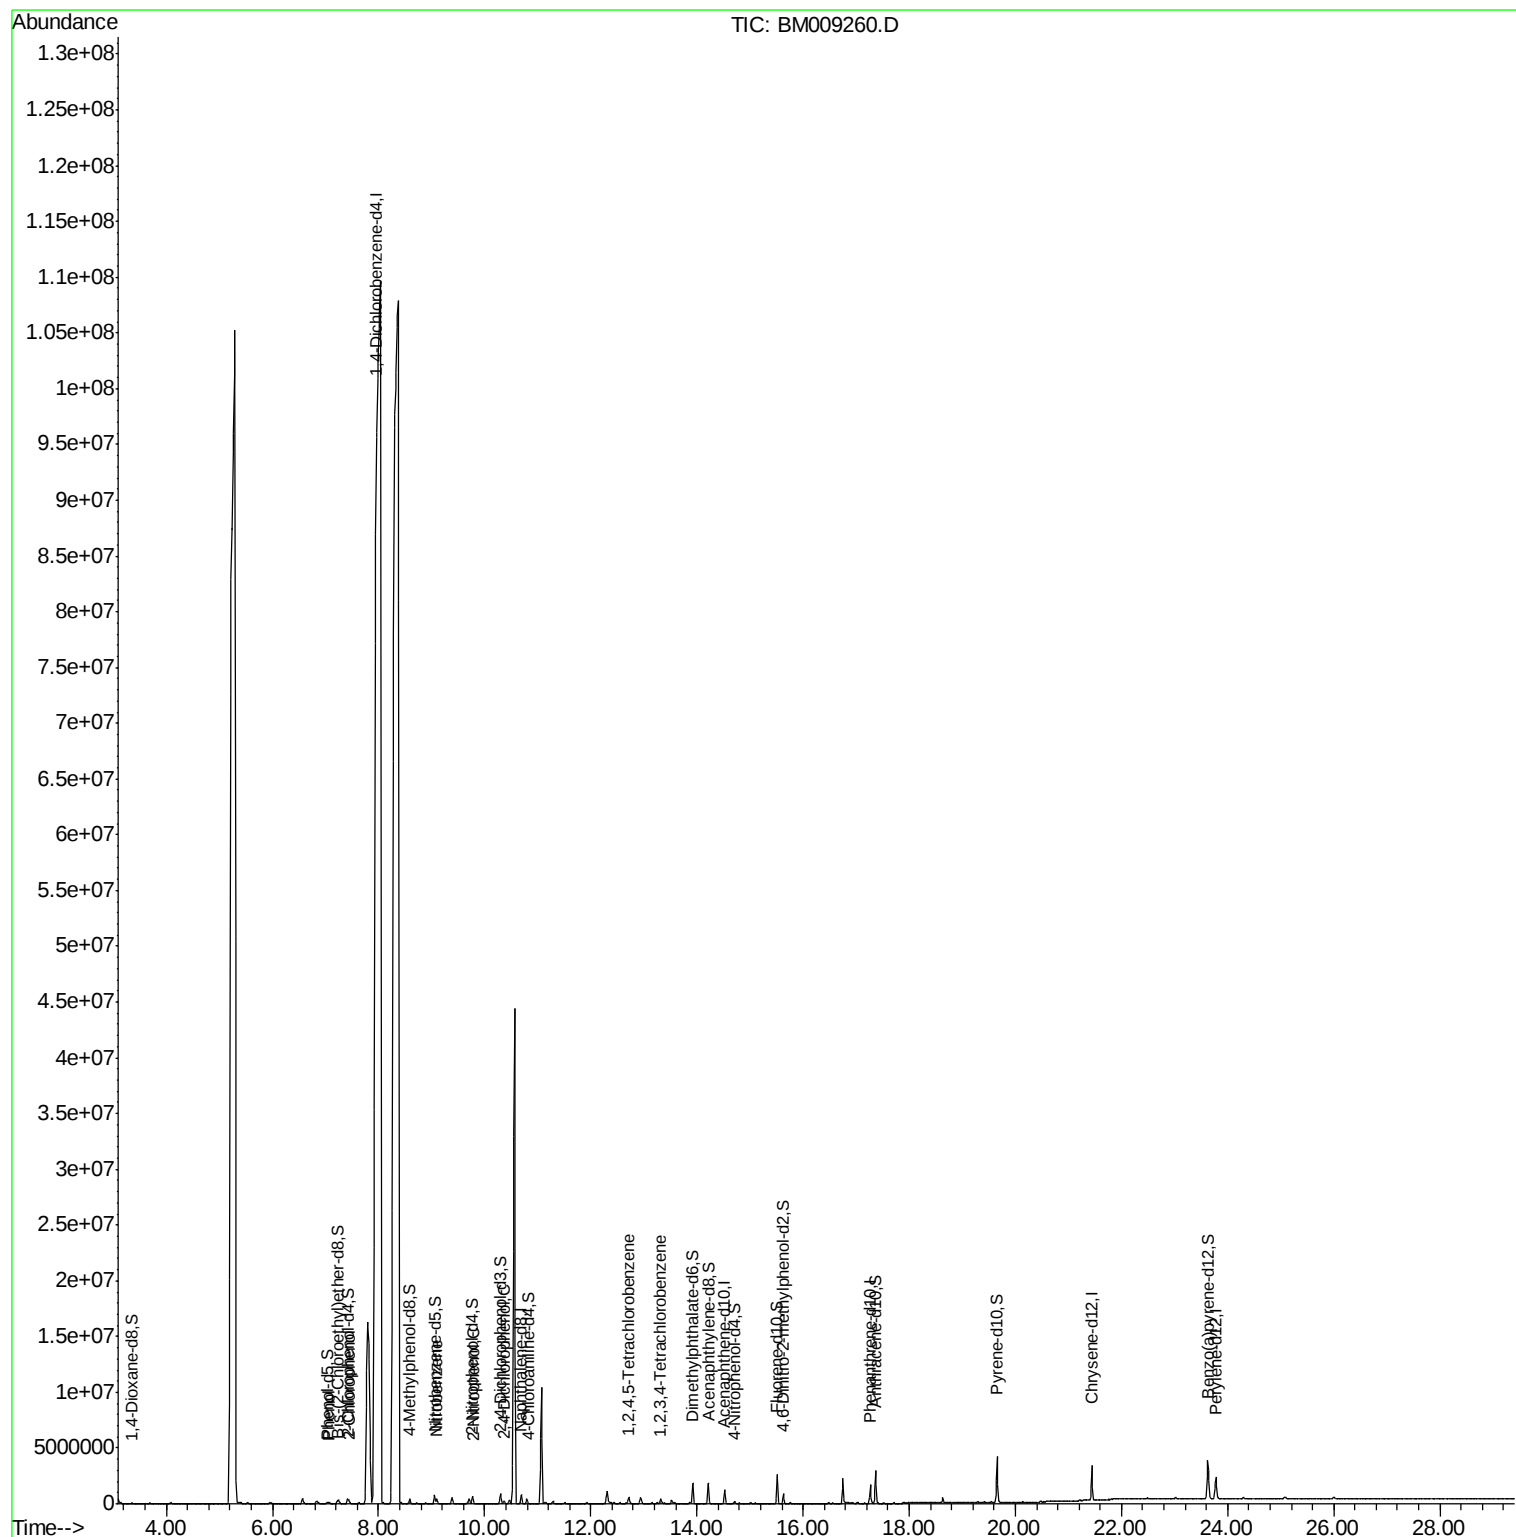

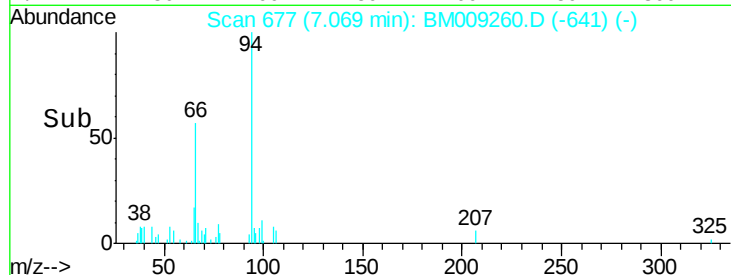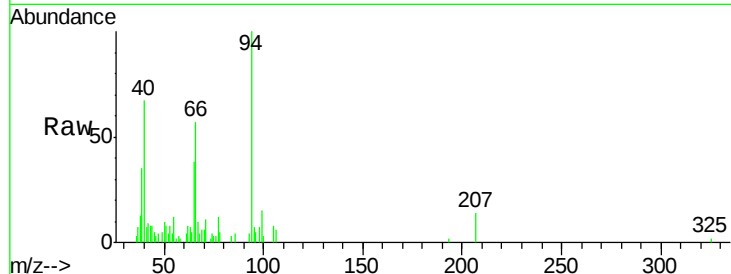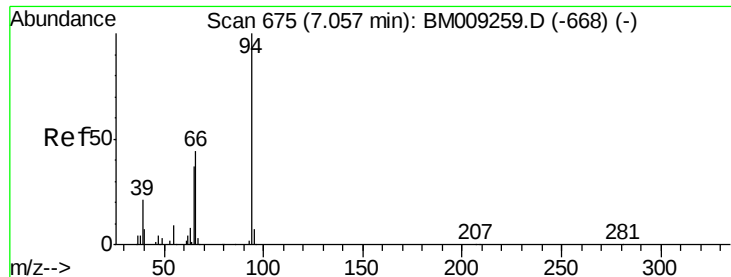

#6
Phenol
Concen: 1.24 ng/ul
RT: 7.07 min Scan# 677
Delta R.T. 0.01 min
Lab File: BM009260.D
Acq: 15 Mar 2017 11:32





Tot Ion:	94	Resp:	28246
Ion Ratio	Lower	Upper	
94	100		
65	37.6	21.0	31.6#
66	57.5	29.3	43.9#

Instrument :
BNA_M
ClientSampleId :
C0BK7RE

Manual Integrations
APPROVED


mohammad


3/16/2017 4:40:50 PM

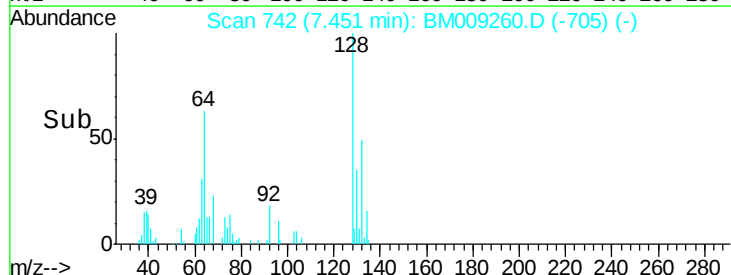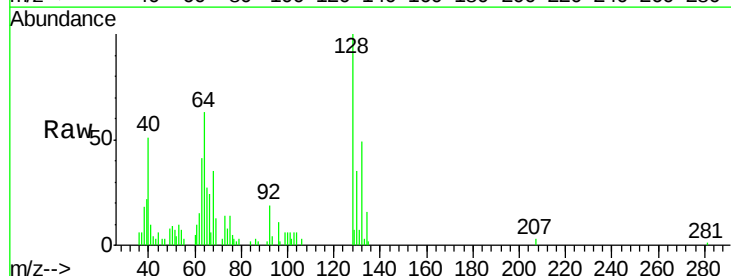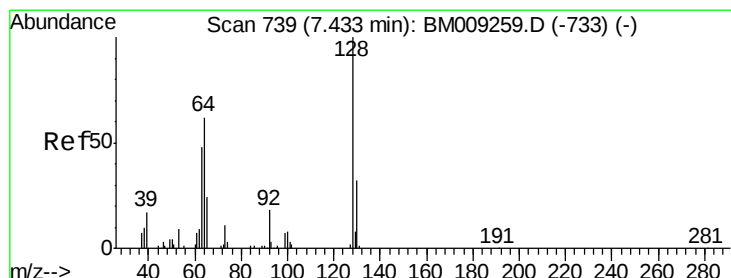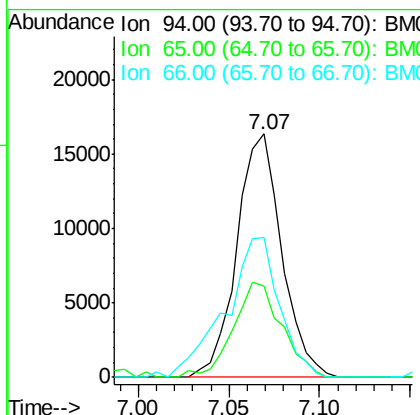

#10
2-Chlorophenol
Concen: 4.39 ng/ul
RT: 7.45 min Scan# 742
Delta R.T. 0.02 min
Lab File: BM009260.D
Acq: 15 Mar 2017 11:32

Tgt Ion:	128	Resp:	58823
Ion Ratio	Lower	Upper	
128	100		
64	63.5	31.9	47.9#
130	35.1	25.6	38.4

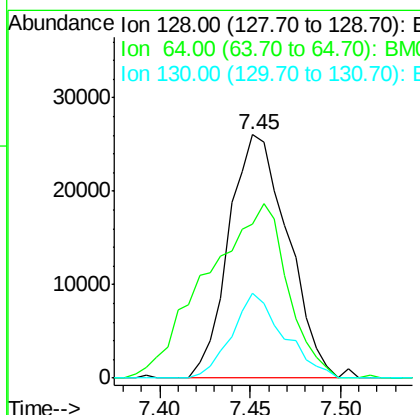

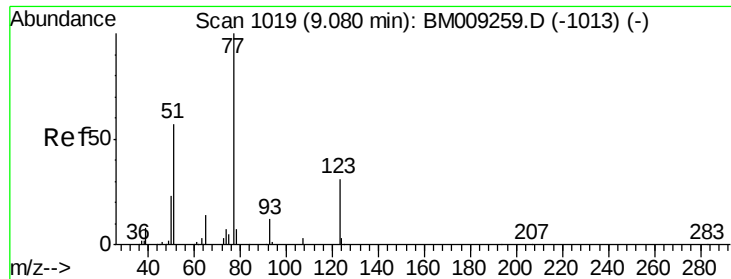

#20
Nitrobenzene
Concen: 16.81 ng/ul
RT: 9.10 min Scan# 1022
Delta R.T. 0.02 min
Lab File: BM009260.D
Acq: 15 Mar 2017 11:32





Instrument :
BNA_M
ClientSampleId :
C0BK7RE

Tot Ion	Ratio	Resp Lower	Upper
77	100		
123	34.8	39.0	58.4#
65	16.2	10.4	15.6#

Manual Integrations
APPROVED




mohammad


3/16/2017 4:40:50 PM

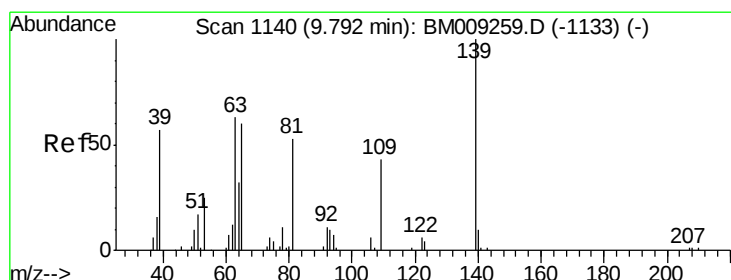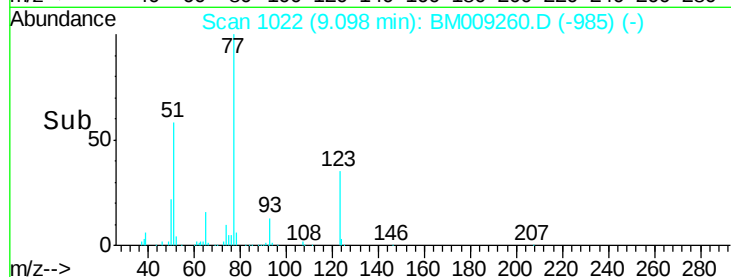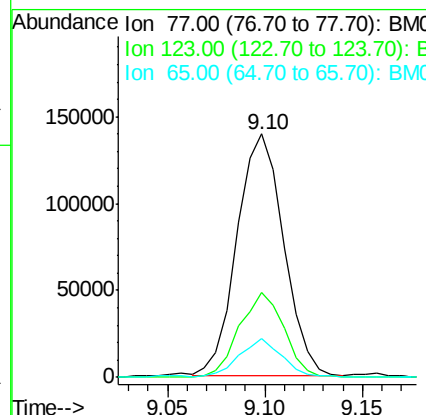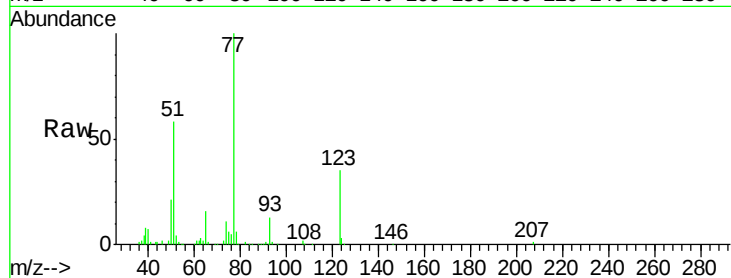

#23
2-Nitrophenol
Concen: 1.21 ng/ul
RT: 9.80 min Scan# 1141
Delta R.T. 0.01 min
Lab File: BM009260.D
Acq: 15 Mar 2017 11:32

Tgt Ion	Ratio	Resp Lower	Upper
139	100		
65	60.5	36.3	54.5#
109	40.3	26.4	39.6#

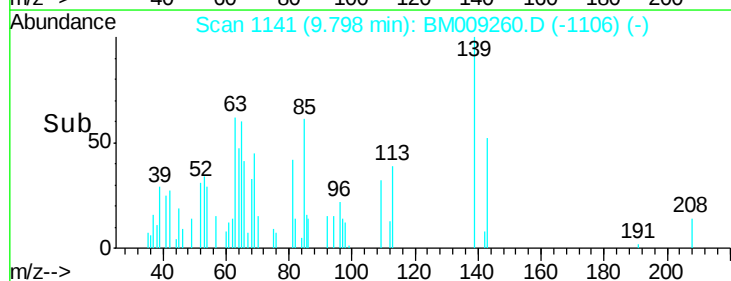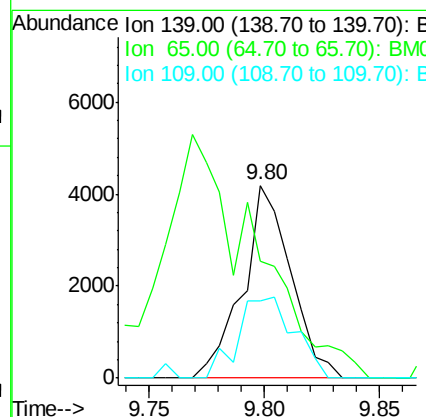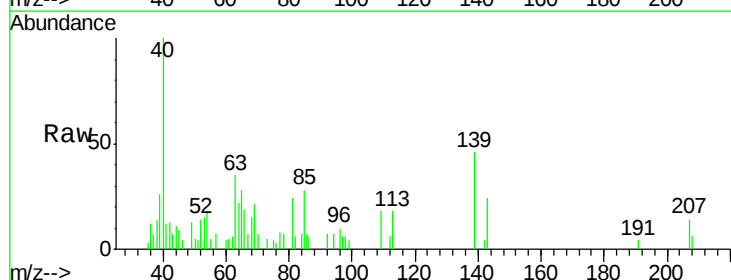

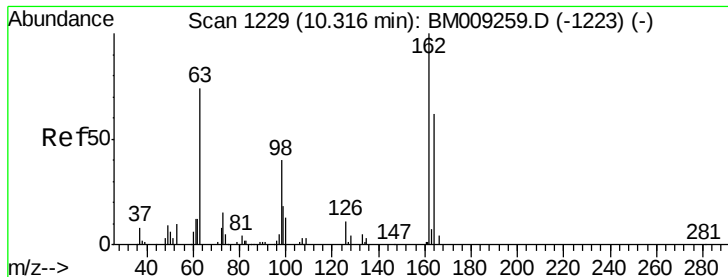

#27
 2,4-Dichlorophenol
 Concen: 8.65 ng/ul m
 RT: 10.36 min Scan# 1237
 Delta R.T. 0.05 min
 Lab File: BM009260.D
 Acq: 15 Mar 2017 11:32





Instrument :
 BNA_M
 ClientSampleId :
 C0BK7RE

Tot Ion	Ratio	Lower	Upper
162	100		
164	60.3	52.1	78.1
98	26.3	28.4	42.6

Manual Integrations
 APPROVED




mohammad


3/16/2017 4:40:50 PM

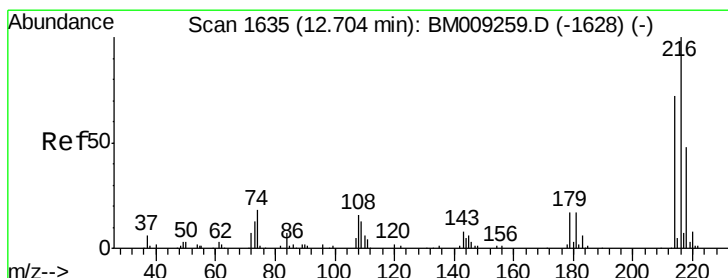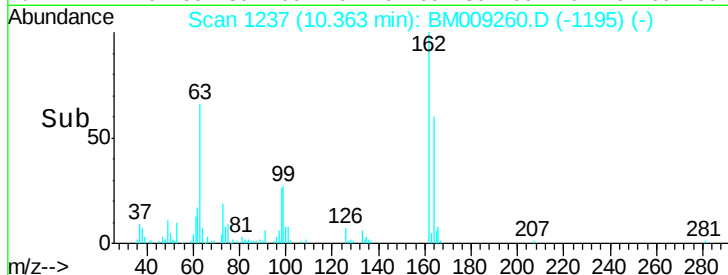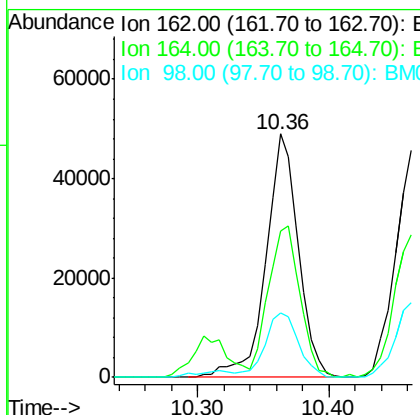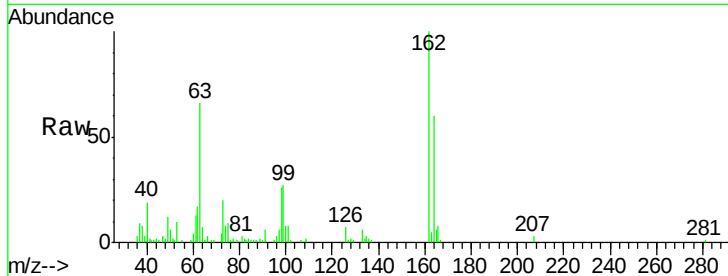

#36
 1,2,4,5-Tetrachlorobenzene
 Concen: 6.85 ng/ul
 RT: 12.70 min Scan# 1635
 Delta R.T. 0.00 min
 Lab File: BM009260.D
 Acq: 15 Mar 2017 11:32

Tgt Ion	Ratio	Lower	Upper
216	100		
214	78.2	62.5	93.7
179	21.0	18.2	27.2
108	17.0	14.2	21.2

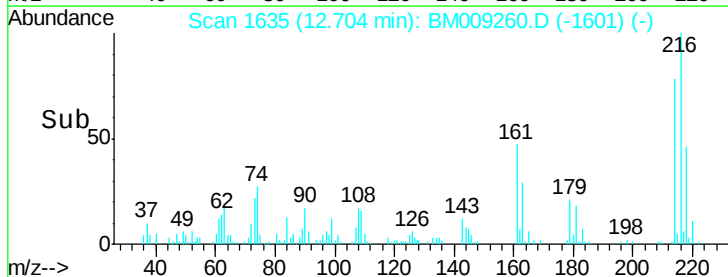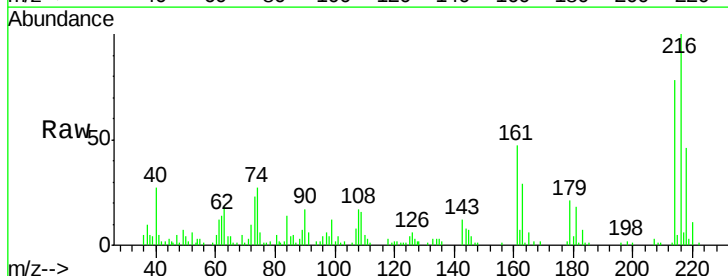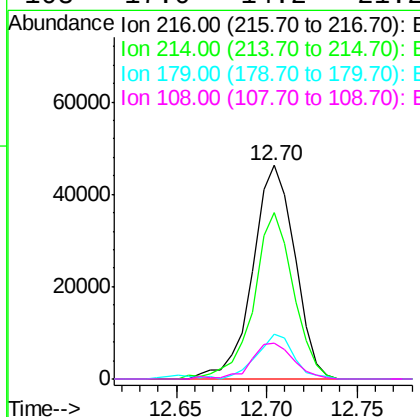

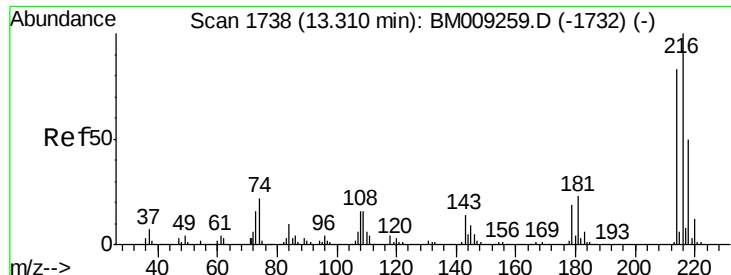

#72

1,2,3,4-Tetrachlorobenzene

Concen: 9.31 ng/uL

RT: 13.31 min Scan# 1738

Delta R.T. 0.00 min

Lab File: BM009260.D

Acq: 15 Mar 2017 11:32

Instrument :

BNA_M

ClientSampleId :

C0BK7RE

Tot Ion:	216	Resp:	104666
Ion Ratio		Lower	Upper
216	100		
214	74.4	62.5	93.7
218	49.0	38.4	57.6

Manual Integrations
APPROVED

mohammad

3/16/2017 4:40:50 PM

