
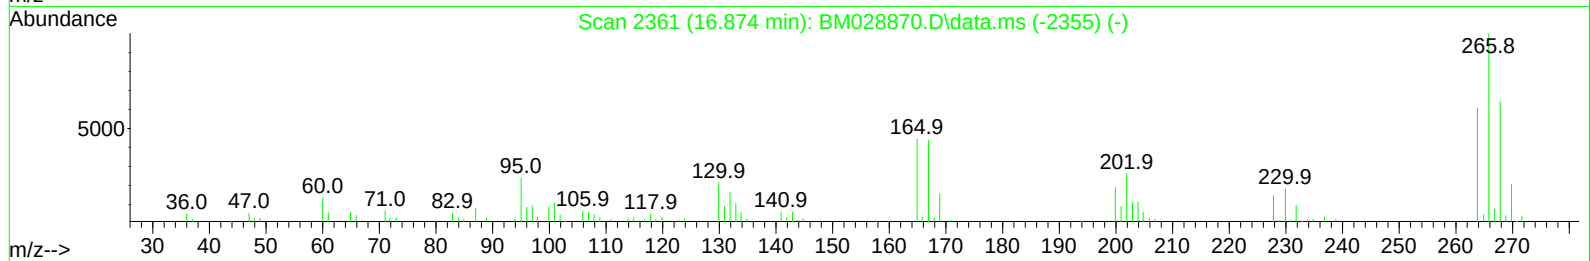
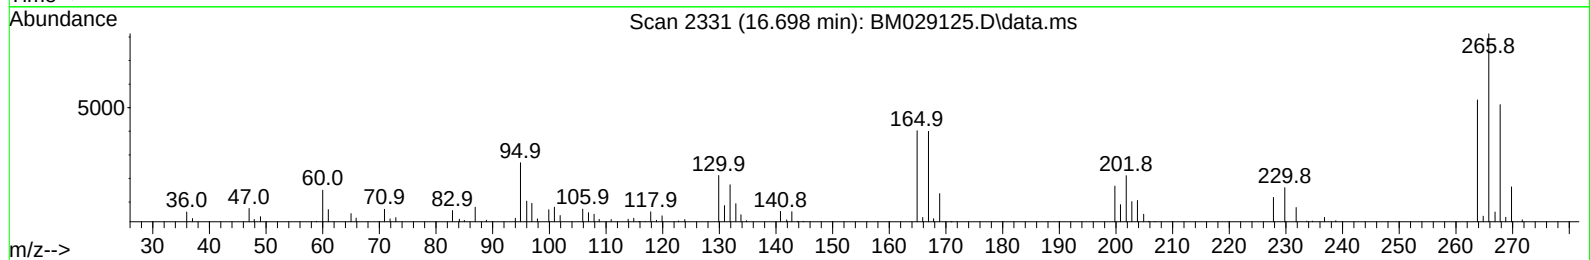


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031521\
Data File : BM029125.D
Acq On : 15 Mar 2021 12:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 12:45:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 12 12:30:15 2021
Response via : Initial Calibration

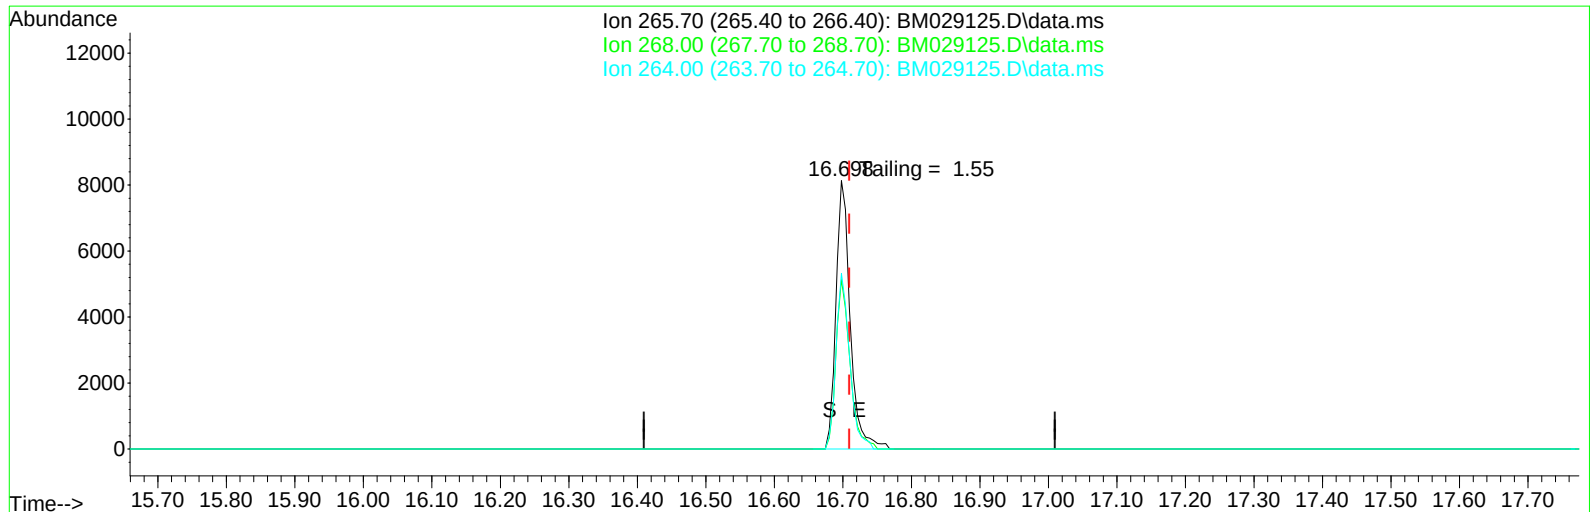

TIC: BM029125.D\data.ms

(70) Pentachlorophenol (C)




16.698min (-0.012) 0.00 ng

response 11794

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.07
264.00	63.30	65.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031521\
Data File : BM029125.D
Acq On : 15 Mar 2021 12:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 12:45:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 12 12:30:15 2021
Response via : Initial Calibration

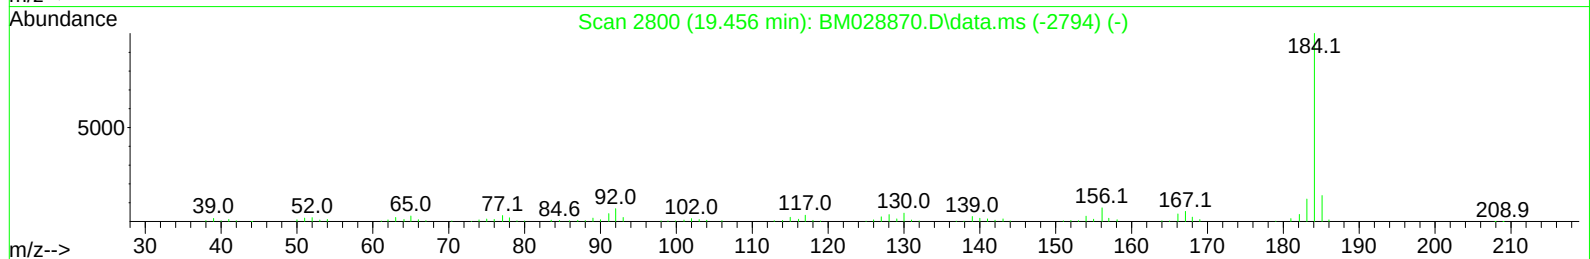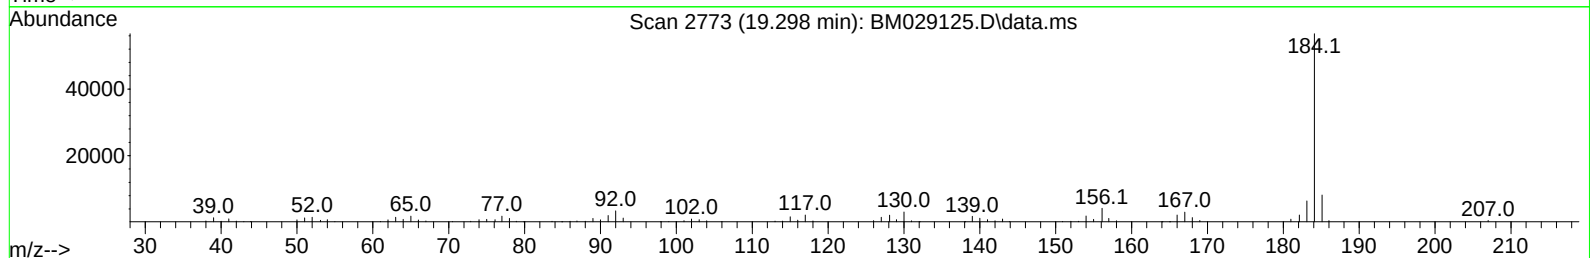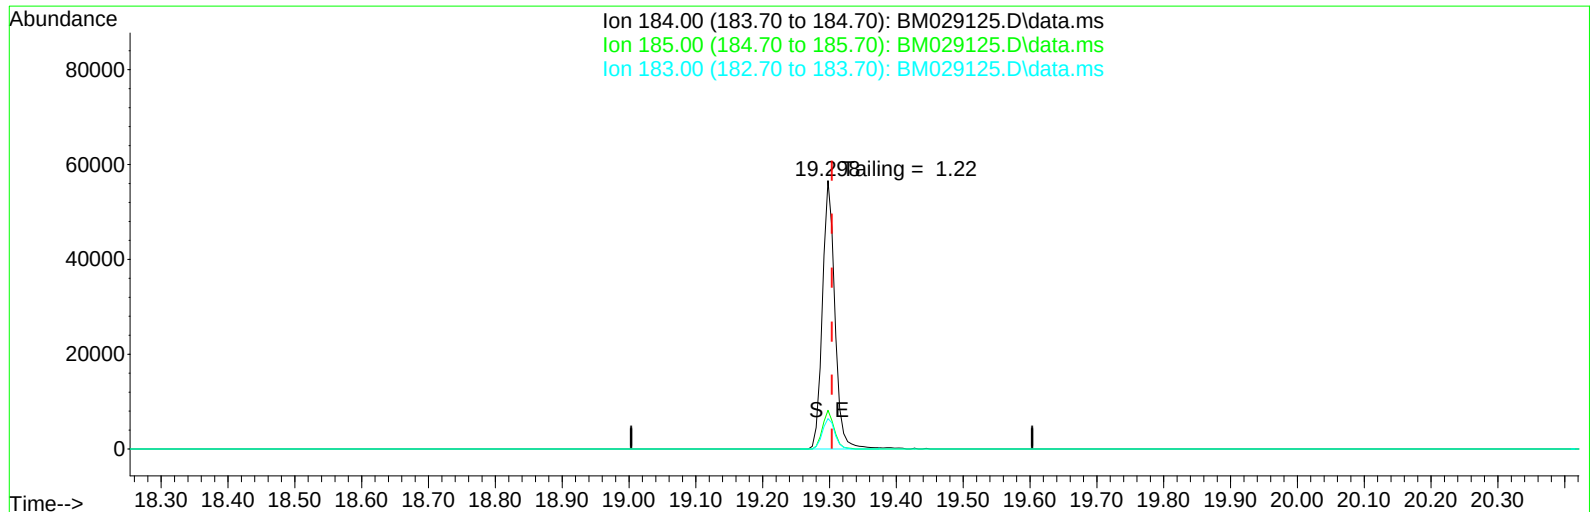

TIC: BM029125.D\data.ms

(77) Benzidine**19.298min (-0.006) 33418.82 ng****response 73784**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.44
183.00	12.10	11.32
0.00	0.00	0.00