

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031521\
 Data File : BM029133.D
 Acq On : 15 Mar 2021 16:59
 Operator : CG/JU
 Sample : M1677-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D2470-D2800(WATER)

Quant Time: Mar 15 17:33:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 12 12:30:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	6842	20.00	ng	0.00
21) Naphthalene-d8	10.404	136	27960	20.00	ng	#-0.01
39) Acenaphthene-d10	14.286	164	18983	20.00	ng	-0.01
64) Phenanthrene-d10	17.039	188	41455	20.00	ng	0.00
76) Chrysene-d12	21.215	240	41384	20.00	ng	#-0.01
86) Perylene-d12	23.356	264	41094	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.198	112	4153	10.06	ng	0.00
7) Phenol-d6	6.816	99	20807	38.16	ng	0.00
23) Nitrobenzene-d5	8.792	82	54754	105.65	ng	0.00
42) 2,4,6-Tribromophenol	15.792	330	3185	14.16	ng	0.00
45) 2-Fluorobiphenyl	12.898	172	131227	92.03	ng	0.00
79) Terphenyl-d14	19.668	244	229765	102.52	ng	0.00
Target Compounds						
10) Phenol	6.845	94	2186	4.03	ng	99
50) Dimethylphthalate	13.757	163	11117	7.73	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031521\
Data File : BM029133.D
Acq On : 15 Mar 2021 16:59
Operator : CG/JU
Sample : M1677-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D2470-D2800(WATER)

Quant Time: Mar 15 17:33:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 12 12:30:15 2021
Response via : Initial Calibration




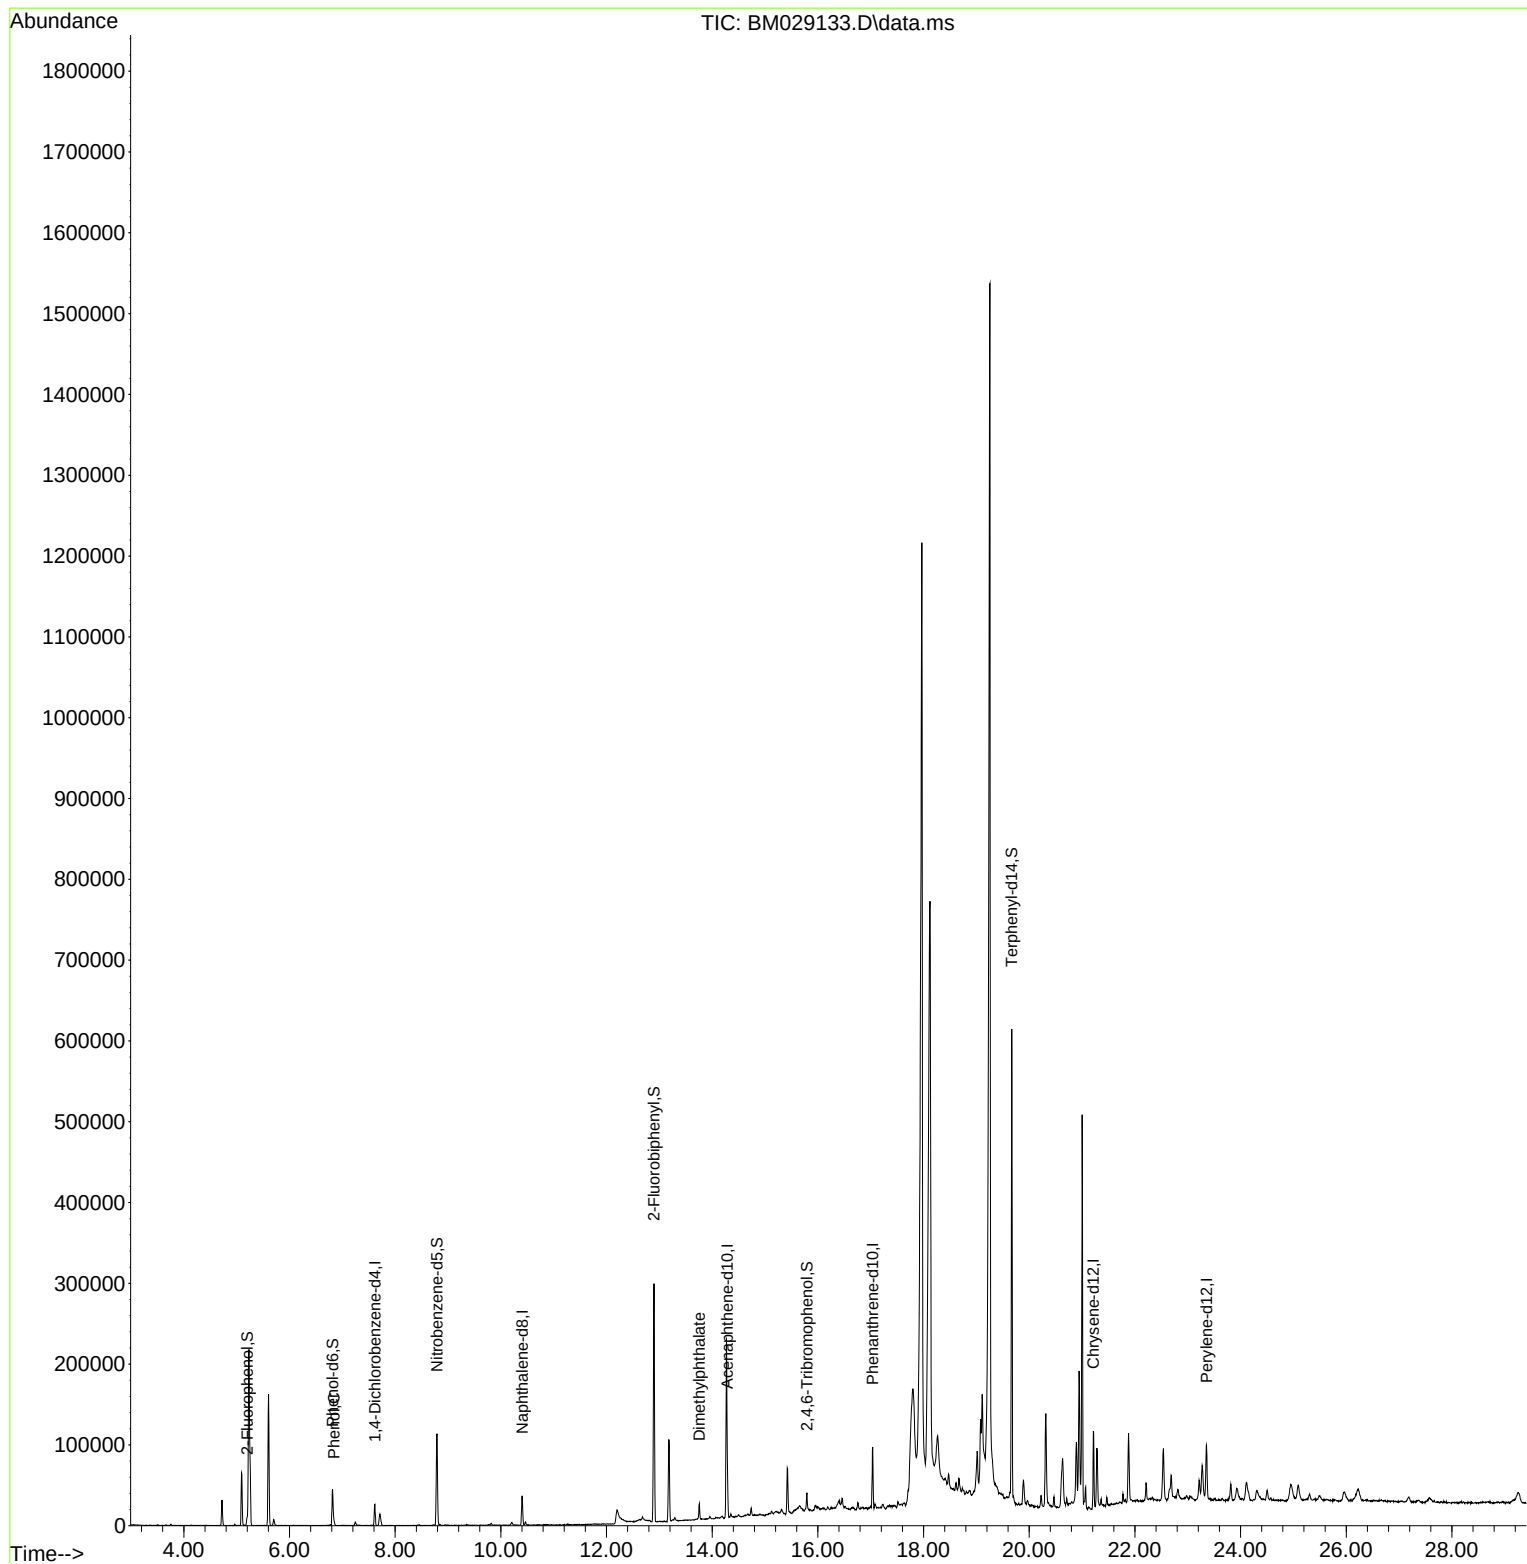




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.616 min Scan# 787
Delta R.T. -0.006 min
Lab File: BM029133.D
Acq: 15 Mar 2021 16:59




Instrument :
BNA_M
ClientSampleId :
D2470-D2800(WATER)


Tgt Ion:152 Resp: 6842
Ion Ratio Lower Upper
152 100
150 156.9 120.6 181.0
115 58.7 47.2 70.8

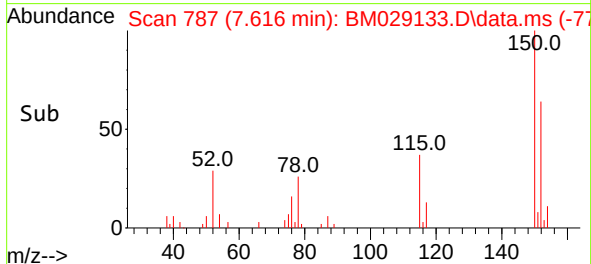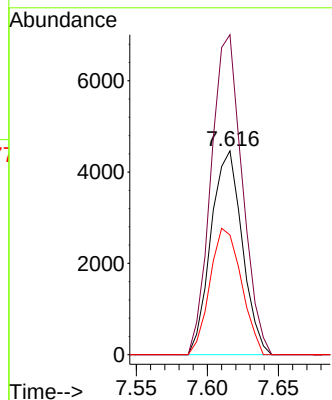

#5
2-Fluorophenol
Concen: 10.06 ng
RT: 5.198 min Scan# 376
Delta R.T. -0.000 min
Lab File: BM029133.D
Acq: 15 Mar 2021 16:59

Tgt Ion:112 Resp: 4153
Ion Ratio Lower Upper
112 100
64 60.0 50.6 76.0
63 39.8 31.0 46.6


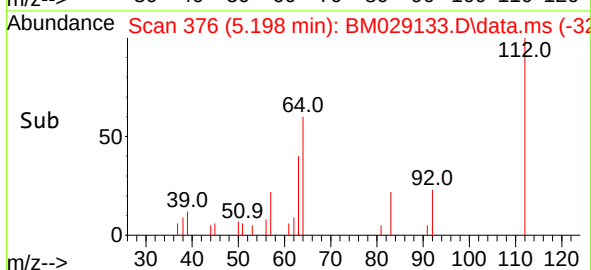
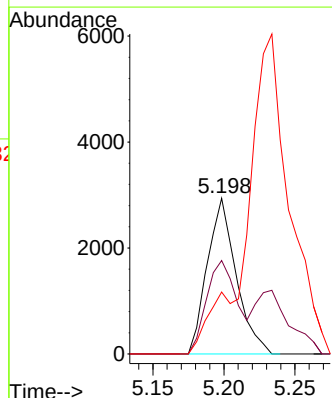





#7
Phenol-d6
Concen: 38.16 ng
RT: 6.816 min Scan# 651
Delta R.T. -0.006 min
Lab File: BM029133.D
Acq: 15 Mar 2021 16:59




Instrument :
BNA_M
ClientSampleId :
D2470-D2800(WATER)


Tgt Ion: 99 Resp: 20807
Ion Ratio Lower Upper
99 100
42 30.0 13.5 20.3#
71 41.8 39.4 59.0

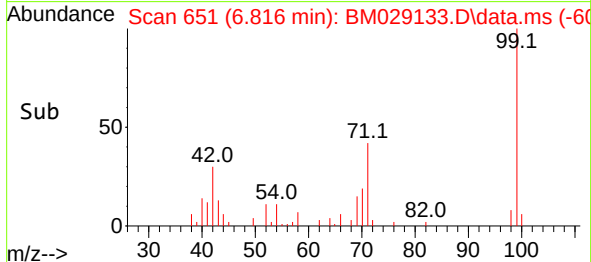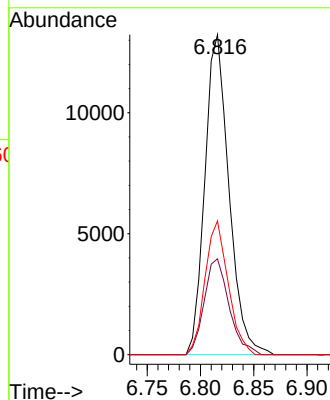

#10
Phenol
Concen: 4.03 ng
RT: 6.845 min Scan# 656
Delta R.T. -0.006 min
Lab File: BM029133.D
Acq: 15 Mar 2021 16:59


Tgt Ion: 94 Resp: 2186
Ion Ratio Lower Upper
94 100
65 35.2 16.4 56.4
66 49.8 30.2 70.2

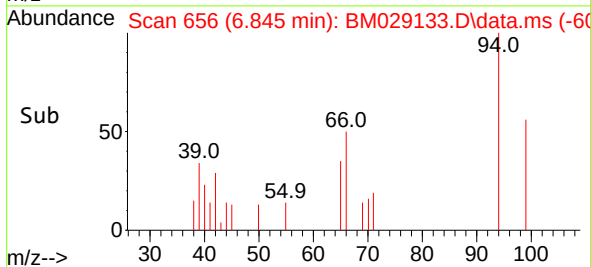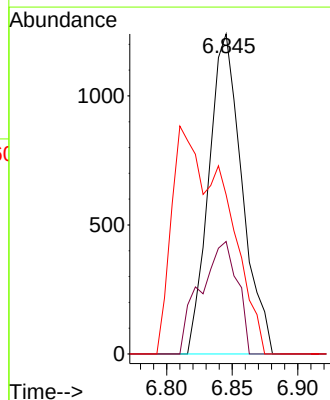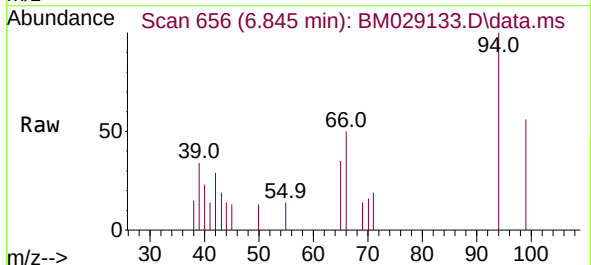






#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.404 min Scan# 1261
Delta R.T. -0.012 min
Lab File: BM029133.D
Acq: 15 Mar 2021 16:59

Instrument :
BNA_M
ClientSampleId :
D2470-D2800(WATER)







Tgt Ion:136 Resp: 27960
Ion Ratio Lower Upper
136 100
137 10.8 8.6 12.8
54 9.5 4.6 7.0#
68 4.7 4.1 6.1

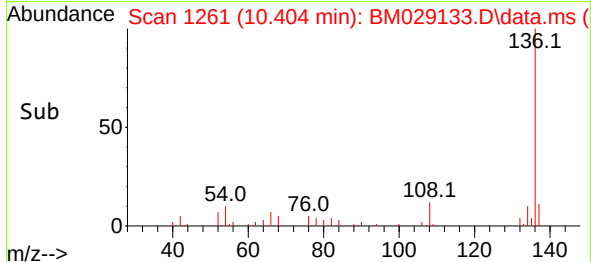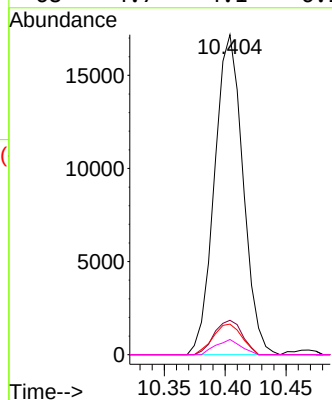

#23
Nitrobenzene-d5
Concen: 105.65 ng
RT: 8.792 min Scan# 987
Delta R.T. -0.006 min
Lab File: BM029133.D
Acq: 15 Mar 2021 16:59

Tgt Ion: 82 Resp: 54754
Ion Ratio Lower Upper
82 100
128 44.6 27.4 41.0#
54 66.5 31.4 47.0#


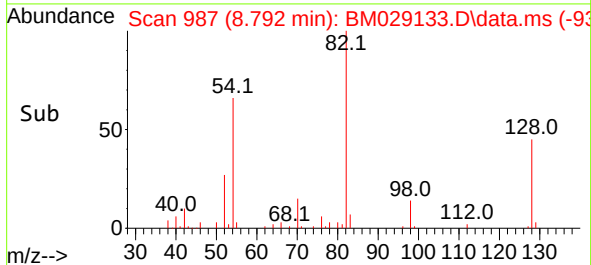
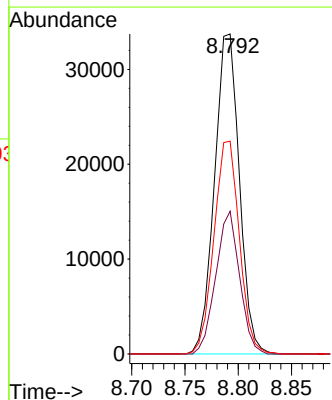
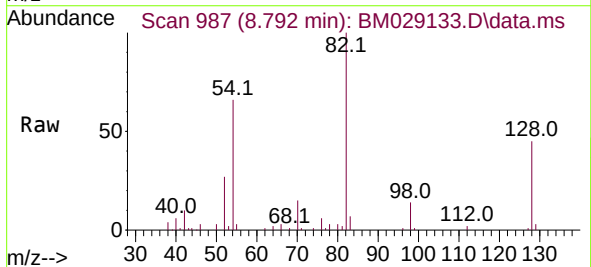




#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.286 min Scan# 1921
Delta R.T. -0.012 min
Lab File: BM029133.D
Acq: 15 Mar 2021 16:59




Instrument :
BNA_M
ClientSampleId :
D2470-D2800(WATER)


Tgt Ion:164 Resp: 18983
Ion Ratio Lower Upper
164 100
162 101.6 80.4 120.6
160 44.7 35.9 53.9

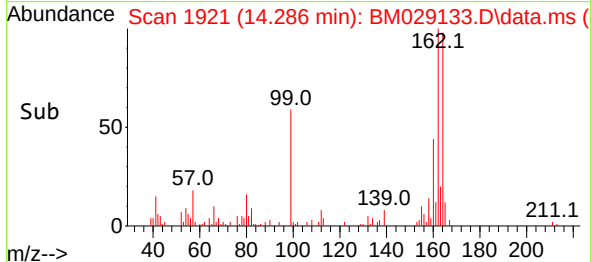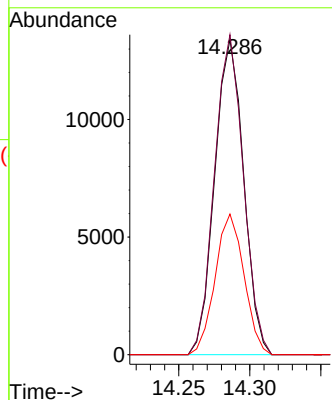

#42
2,4,6-Tribromophenol
Concen: 14.16 ng
RT: 15.792 min Scan# 2177
Delta R.T. -0.006 min
Lab File: BM029133.D
Acq: 15 Mar 2021 16:59

Tgt Ion:330 Resp: 3185
Ion Ratio Lower Upper
330 100
332 92.9 77.8 116.8
141 49.8 28.4 42.6#


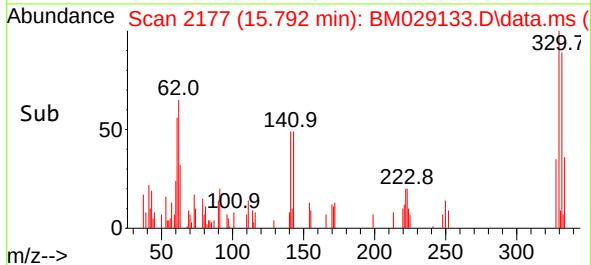
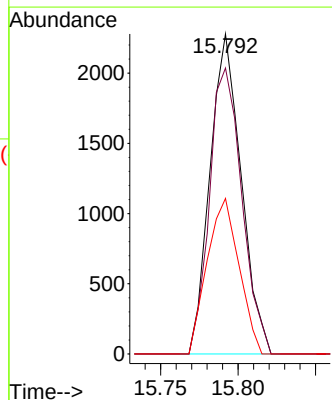
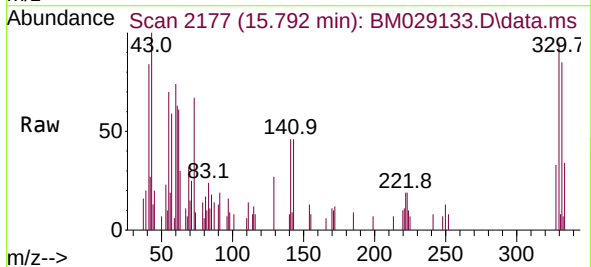




#45
2-Fluorobiphenyl
Concen: 92.03 ng
RT: 12.898 min Scan# 1685
Delta R.T. -0.006 min
Lab File: BM029133.D
Acq: 15 Mar 2021 16:59




Instrument :
BNA_M
ClientSampleId :
D2470-D2800(WATER)


Tgt Ion:	172	Resp:	131227
Ion Ratio	Lower	Upper	
172	100		
171	34.8	27.8	41.8
170	22.2	18.6	27.8

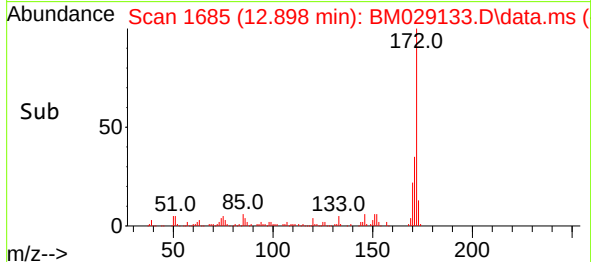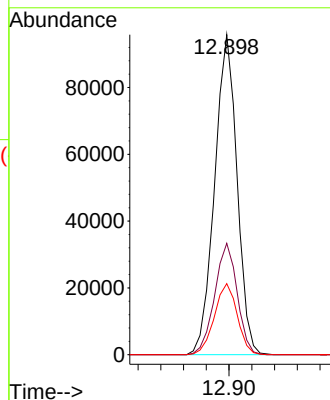

#50
Dimethylphthalate
Concen: 7.73 ng
RT: 13.757 min Scan# 1831
Delta R.T. -0.012 min
Lab File: BM029133.D
Acq: 15 Mar 2021 16:59

Tgt Ion:	163	Resp:	11117
Ion Ratio	Lower	Upper	
163	100		
194	4.3	3.4	5.2
164	10.0	8.1	12.1


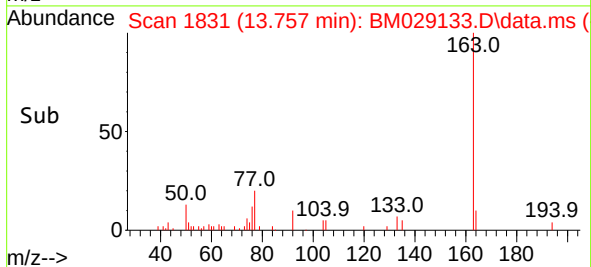
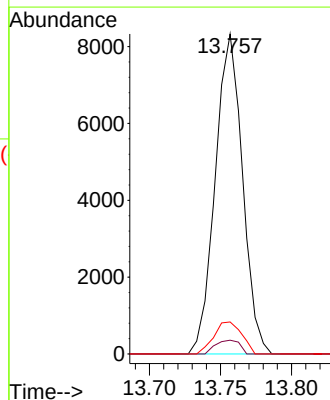
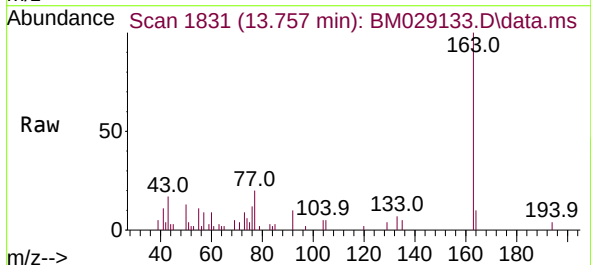




#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.039 min Scan# 2389
Delta R.T. -0.006 min
Lab File: BM029133.D
Acq: 15 Mar 2021 16:59




Instrument :
BNA_M
ClientSampleId :
D2470-D2800(WATER)


Tgt Ion:188 Resp: 41455
Ion Ratio Lower Upper
188 100
94 7.5 6.2 9.4
80 8.8 7.5 11.3

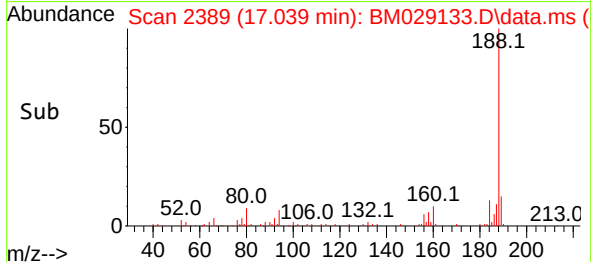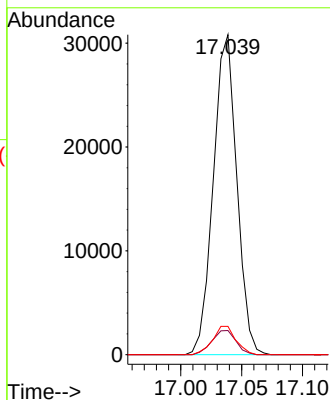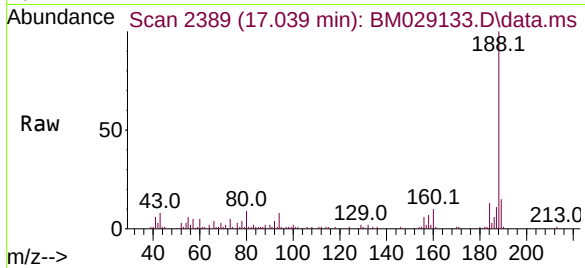

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.215 min Scan# 3099
Delta R.T. -0.012 min
Lab File: BM029133.D
Acq: 15 Mar 2021 16:59

Tgt Ion:240 Resp: 41384
Ion Ratio Lower Upper
240 100
120 11.3 6.4 9.6#
236 25.9 20.1 30.1


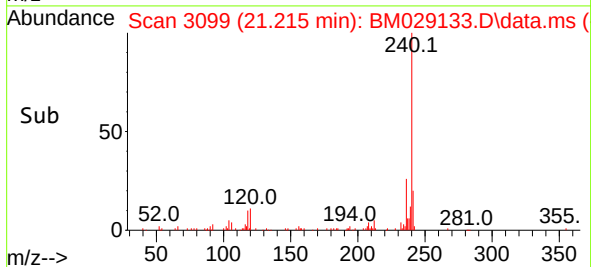
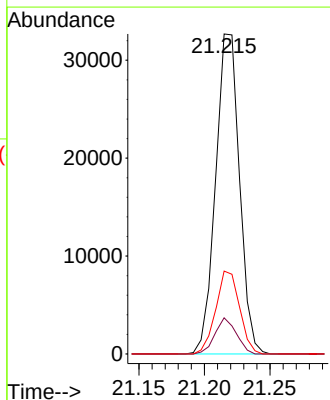
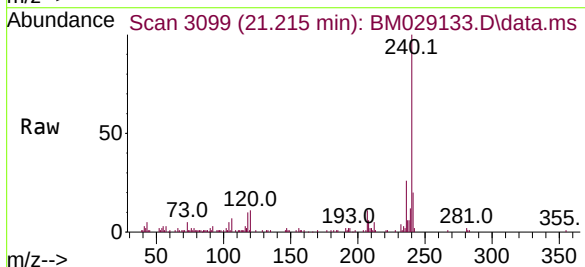




#79
Terphenyl-d14
Concen: 102.52 ng
RT: 19.668 min Scan# 2836
Delta R.T. -0.006 min
Lab File: BM029133.D
Acq: 15 Mar 2021 16:59

Instrument :
BNA_M
ClientSampleId :
D2470-D2800(WATER)

Tgt Ion:244 Resp: 229765
Ion Ratio Lower Upper
244 100
212 7.3 5.8 8.8
122 11.1 6.5 9.7#

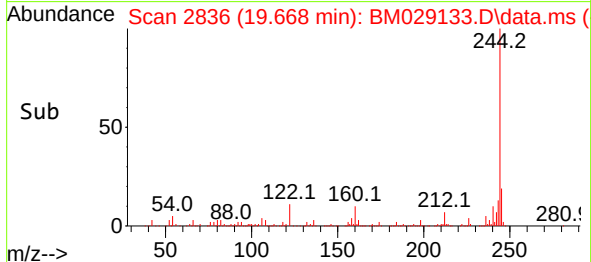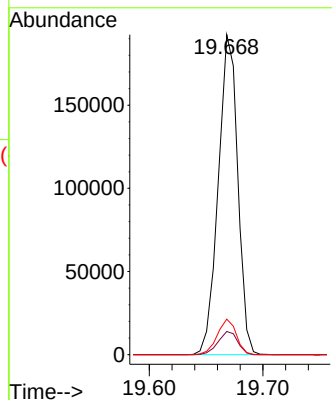

#86
Perylene-d12
Concen: 20.00 ng
RT: 23.356 min Scan# 3463
Delta R.T. -0.012 min
Lab File: BM029133.D
Acq: 15 Mar 2021 16:59

Tgt Ion:264 Resp: 41094
Ion Ratio Lower Upper
264 100
260 23.4 19.0 28.4
265 21.3 17.7 26.5

