

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031521\
 Data File : BM029127.D
 Acq On : 15 Mar 2021 13:16
 Operator : CG/JU
 Sample : PB135132BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB135132BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029127.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.193	370	375	393	rBB	211732	296631	65.64%	13.042%
2	6.816	645	651	669	rBB	191567	292575	64.74%	12.864%
3	7.616	782	787	795	rBB	34138	49405	10.93%	2.172%
4	8.792	981	987	1001	rBV	118993	188060	41.61%	8.268%
5	10.404	1255	1261	1270	rBB	40990	63987	14.16%	2.813%
6	12.898	1679	1685	1693	rBV	267141	371040	82.10%	16.313%
7	14.286	1916	1921	1927	rBB2	52435	73317	16.22%	3.223%
8	15.786	2171	2176	2185	rBB	178367	241144	53.36%	10.602%
9	17.039	2383	2389	2396	rBB	57075	76478	16.92%	3.362%
10	19.668	2831	2836	2841	rVB	400219	451916	100.00%	19.869%
11	21.215	3095	3099	3104	rBV	69243	81347	18.00%	3.577%
12	23.356	3457	3463	3469	rVB	51450	88556	19.60%	3.894%




Sum of corrected areas: 2274456

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031521\
Data File : BM029127.D
Acq On : 15 Mar 2021 13:16
Operator : CG/JU
Sample : PB135132BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135132BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

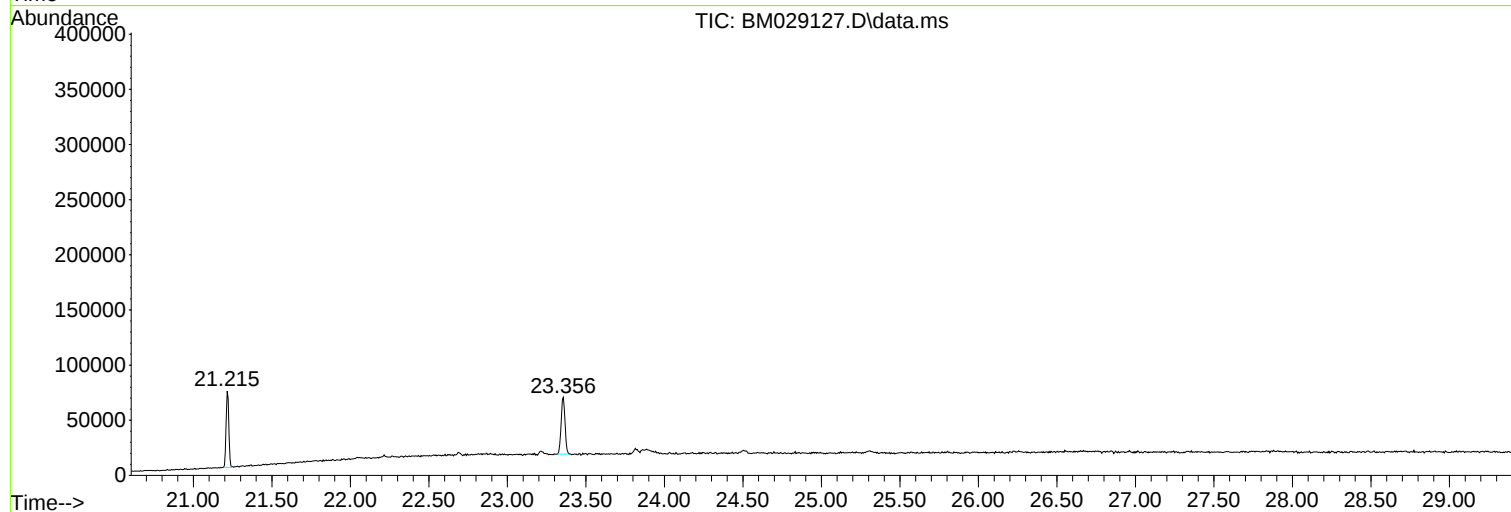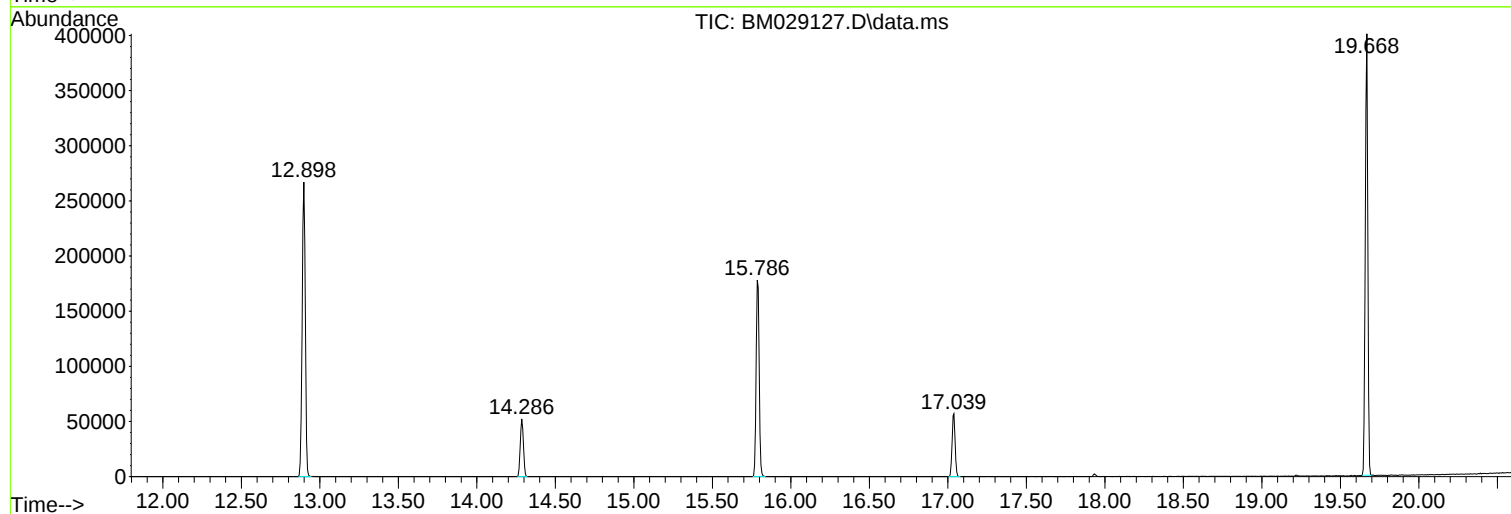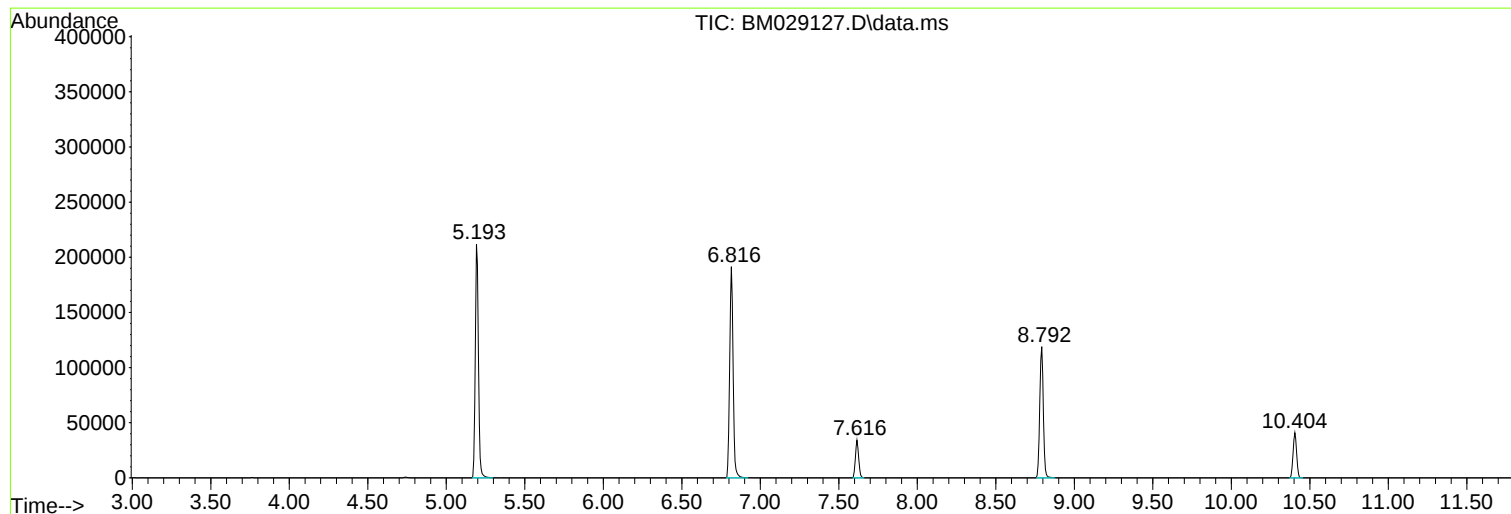

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031521\
Data File : BM029127.D
Acq On : 15 Mar 2021 13:16
Operator : CG/JU
Sample : PB135132BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135132BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031521\
Data File : BM029127.D
Acq On : 15 Mar 2021 13:16
Operator : CG/JU
Sample : PB135132BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135132BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------