

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031521\
 Data File : BM029131.D
 Acq On : 15 Mar 2021 15:43
 Operator : CG/JU
 Sample : PB135159BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB135159BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029131.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.193	370	375	389	rBV	170601	239573	56.15%	12.338%
2	6.816	645	651	667	rBV	154319	238183	55.82%	12.266%
3	7.616	782	787	795	rBB	27925	40843	9.57%	2.103%
4	8.793	981	987	1001	rBB	95675	152957	35.85%	7.877%
5	10.404	1255	1261	1270	rBV	35640	54835	12.85%	2.824%
6	12.898	1679	1685	1693	rBV	223075	303107	71.04%	15.610%
7	14.287	1916	1921	1927	rBB2	45818	63333	14.84%	3.262%
8	15.786	2171	2176	2185	rBB	152531	202779	47.52%	10.443%
9	17.033	2383	2388	2395	rBB	47949	66185	15.51%	3.409%
10	19.669	2830	2836	2840	rBV	361850	426681	100.00%	21.974%
11	21.215	3095	3099	3105	rBV	63129	71737	16.81%	3.694%
12	23.357	3457	3463	3471	rVB2	45917	81539	19.11%	4.199%




Sum of corrected areas: 1941752

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031521\
Data File : BM029131.D
Acq On : 15 Mar 2021 15:43
Operator : CG/JU
Sample : PB135159BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135159BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

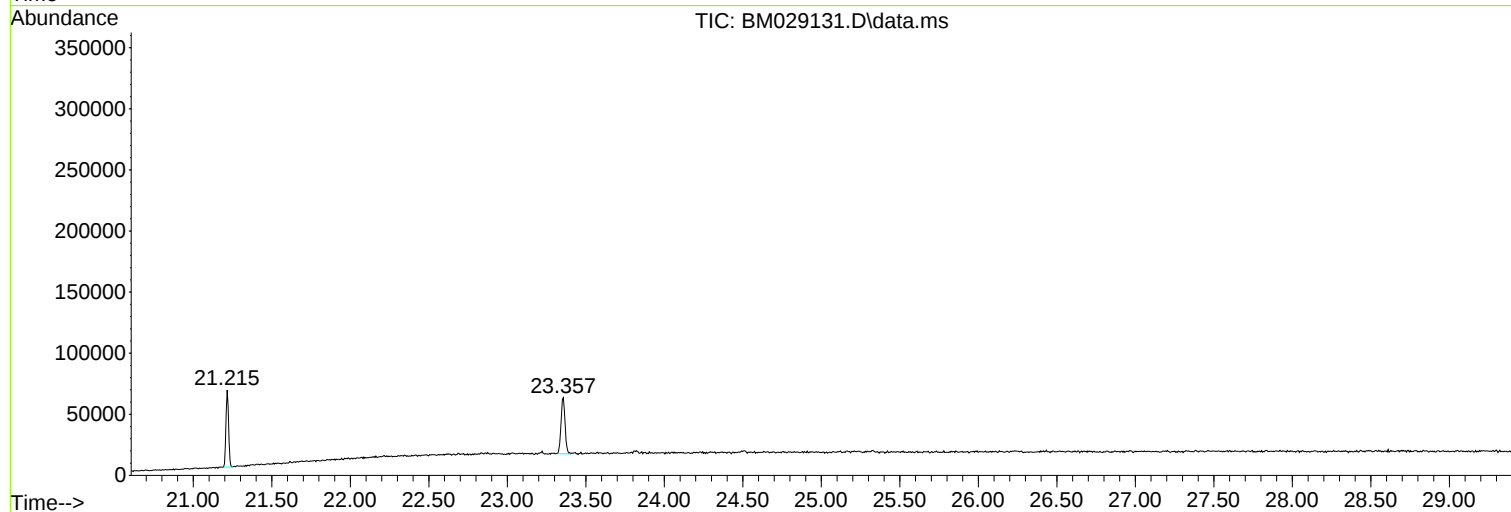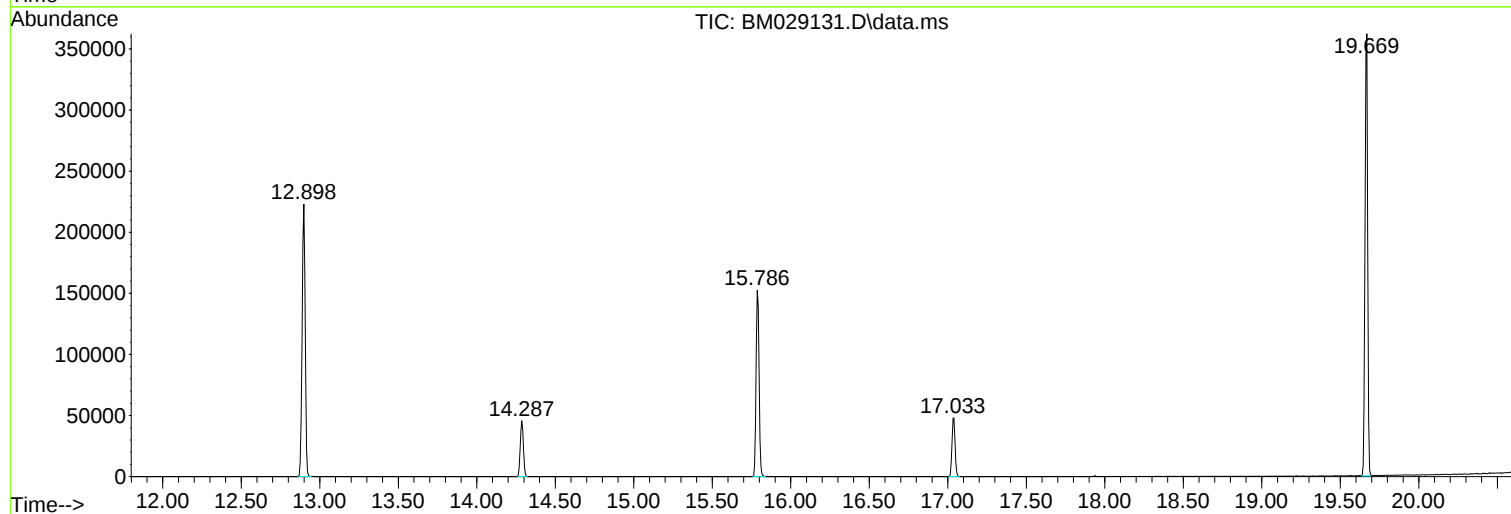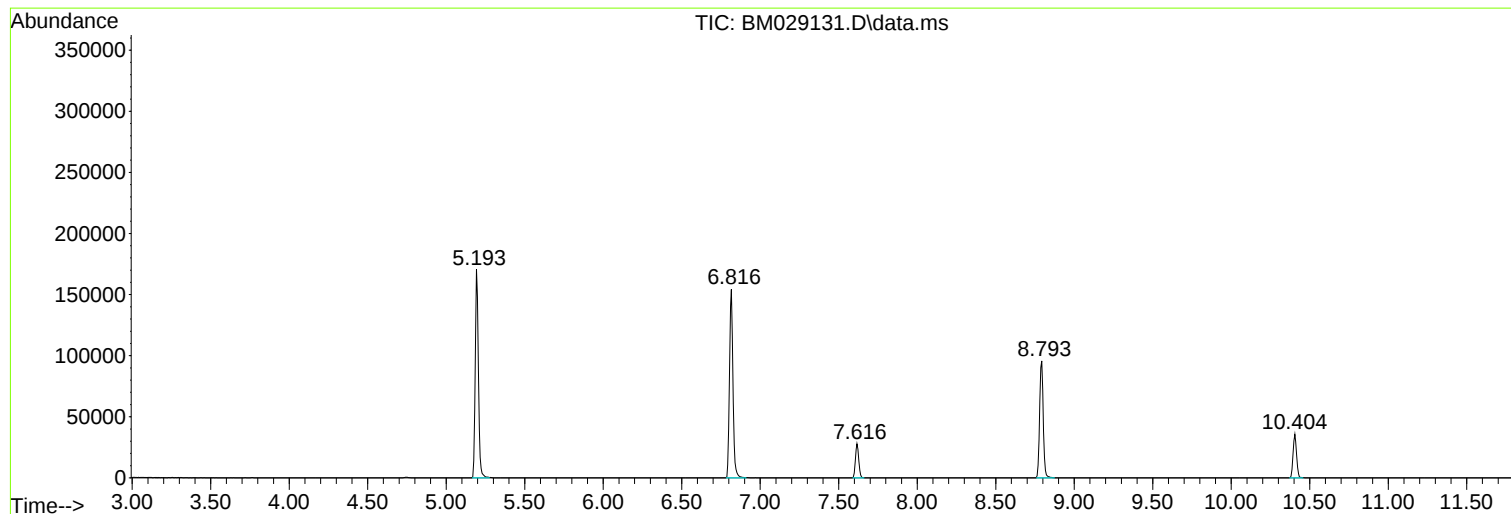

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031521\
Data File : BM029131.D
Acq On : 15 Mar 2021 15:43
Operator : CG/JU
Sample : PB135159BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135159BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031521\
Data File : BM029131.D
Acq On : 15 Mar 2021 15:43
Operator : CG/JU
Sample : PB135159BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135159BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------