

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031521\  
 Data File : BM029132.D  
 Acq On : 15 Mar 2021 16:19  
 Operator : CG/JU  
 Sample : PB135154BL  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 PB135154BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029132.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.193       | 370           | 375         | 390          | rBV      | 228394         | 317387        | 64.26%          | 12.931%       |
| 2         | 6.816       | 645           | 651         | 666          | rBV      | 210577         | 315473        | 63.87%          | 12.853%       |
| 3         | 7.616       | 782           | 787         | 795          | rBB      | 35568          | 51965         | 10.52%          | 2.117%        |
| 4         | 8.792       | 981           | 987         | 1001         | rBV      | 128757         | 203674        | 41.24%          | 8.298%        |
| 5         | 10.404      | 1255          | 1261        | 1270         | rBB      | 43146          | 69059         | 13.98%          | 2.813%        |
| 6         | 12.898      | 1679          | 1685        | 1692         | rBV      | 303326         | 405717        | 82.14%          | 16.529%       |
| 7         | 14.286      | 1916          | 1921        | 1927         | rBB      | 59236          | 80445         | 16.29%          | 3.277%        |
| 8         | 15.792      | 2171          | 2177        | 2186         | rBB      | 195553         | 267442        | 54.15%          | 10.896%       |
| 9         | 17.039      | 2384          | 2389        | 2397         | rBB      | 63771          | 83585         | 16.92%          | 3.405%        |
| 10        | 19.668      | 2831          | 2836        | 2841         | rBV      | 438919         | 493929        | 100.00%         | 20.123%       |
| 11        | 21.215      | 3095          | 3099        | 3106         | rVB2     | 69096          | 80978         | 16.39%          | 3.299%        |
| 12        | 23.356      | 3457          | 3463        | 3469         | rVB2     | 50173          | 84906         | 17.19%          | 3.459%        |




Sum of corrected areas: 2454560

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031521\  
Data File : BM029132.D  
Acq On : 15 Mar 2021 16:19  
Operator : CG/JU  
Sample : PB135154BL  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB135154BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

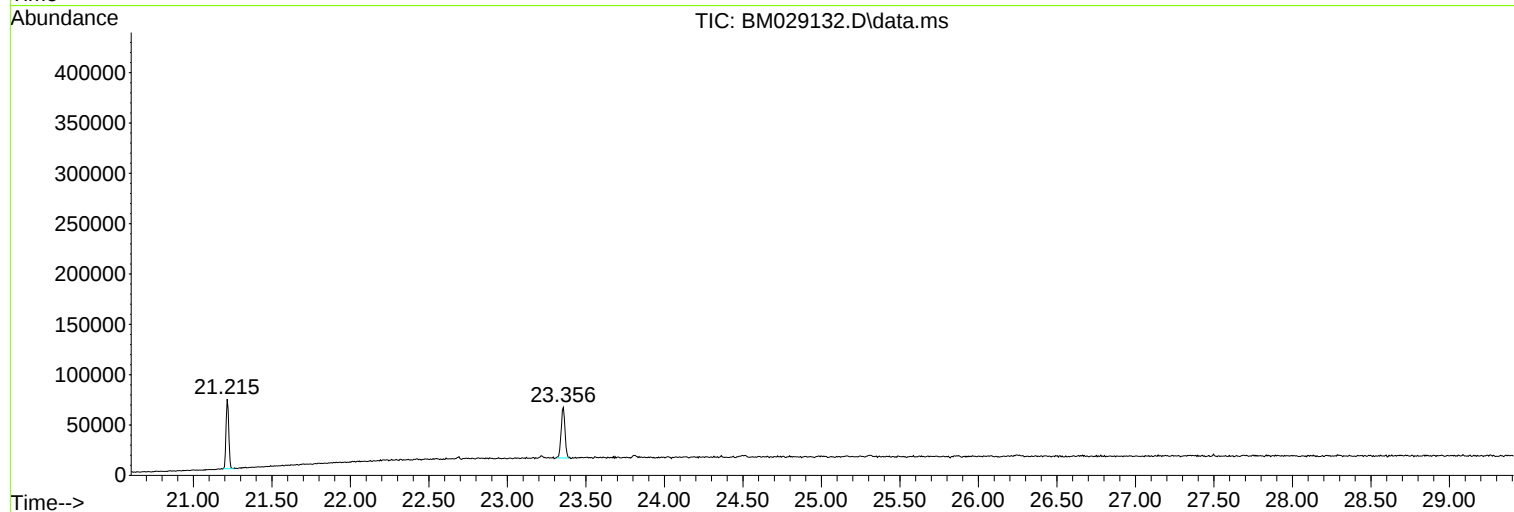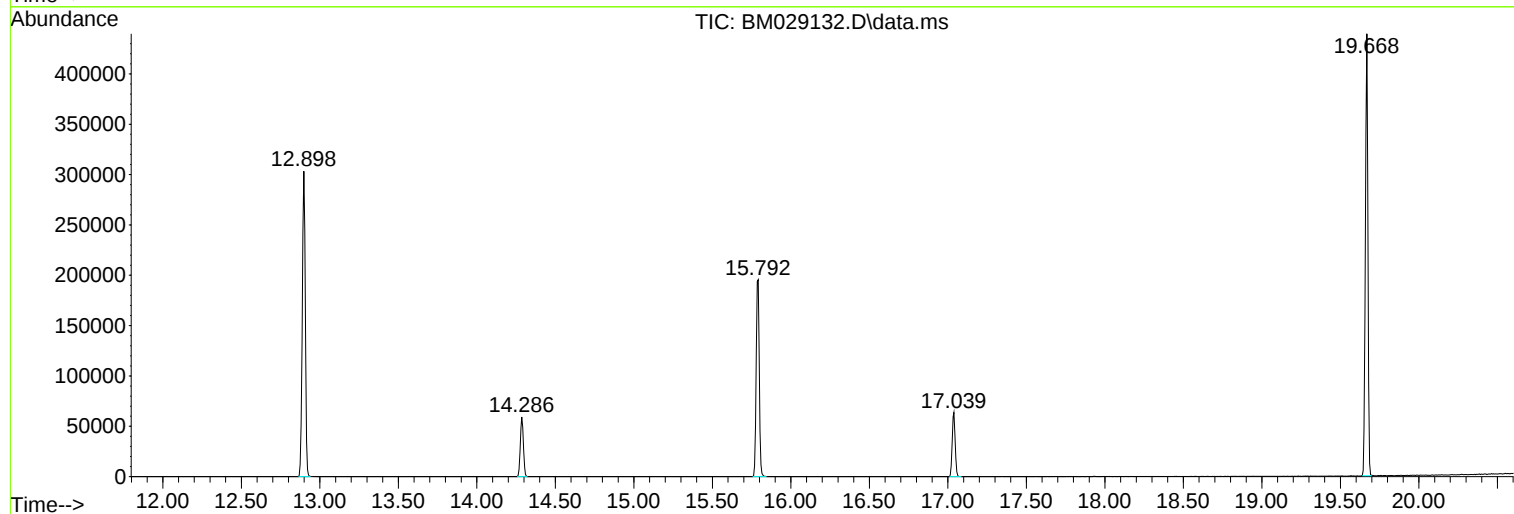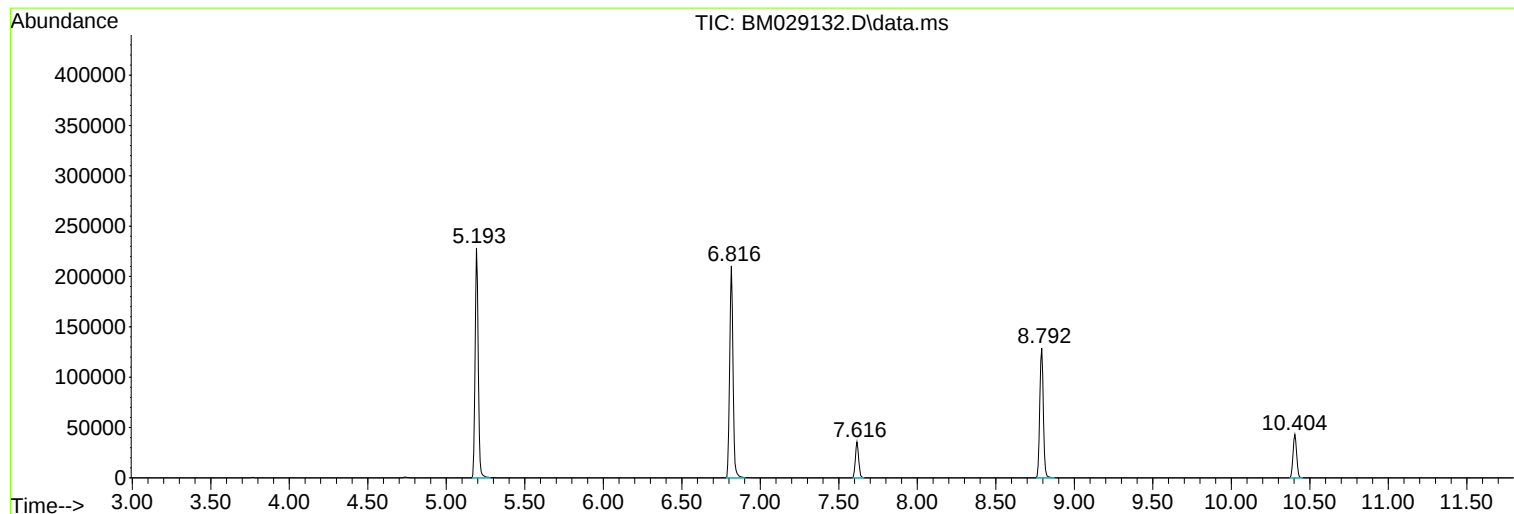

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031521\  
Data File : BM029132.D  
Acq On : 15 Mar 2021 16:19  
Operator : CG/JU  
Sample : PB135154BL  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB135154BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031521\  
Data File : BM029132.D  
Acq On : 15 Mar 2021 16:19  
Operator : CG/JU  
Sample : PB135154BL  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB135154BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|