
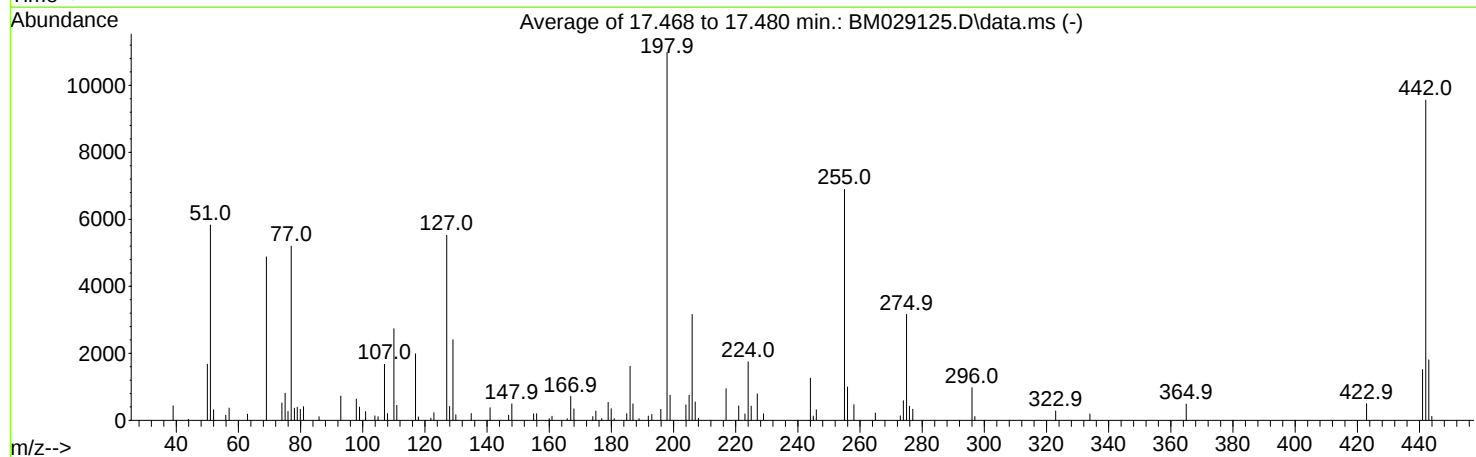


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031521\  
 Data File : BM029125.D  
 Acq On : 15 Mar 2021 12:04  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Mar 12 12:30:15 2021

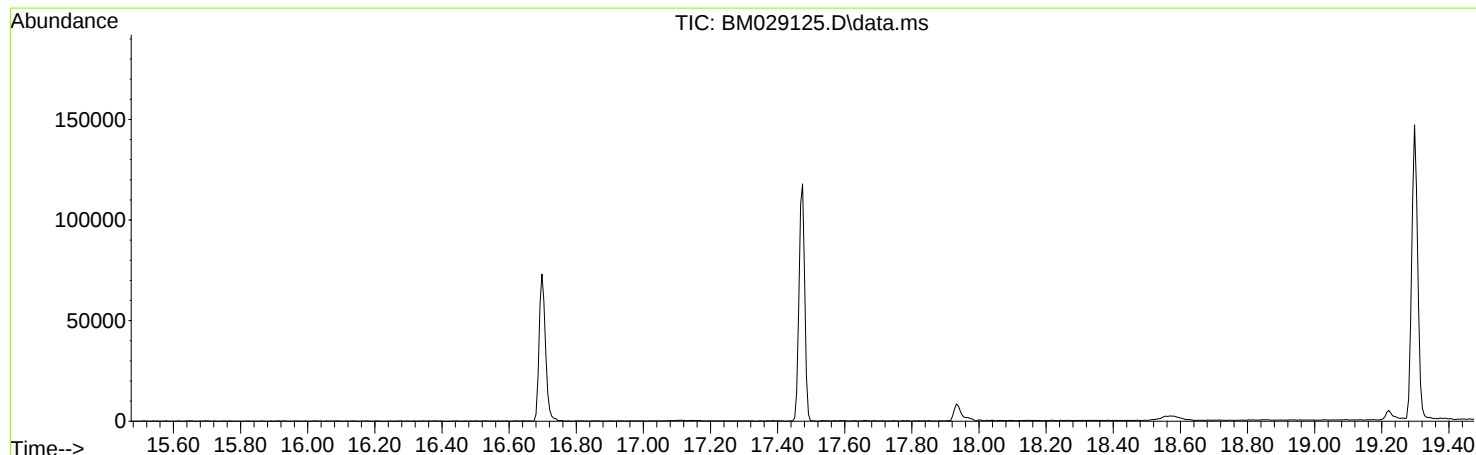

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456




| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 53.1         | 5831       | PASS                |
| 68             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 69             | 198             | 0.00            | 100             | 44.4         | 4879       | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 50.3         | 5523       | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 10979      | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 750        | PASS                |
| 275            | 198             | 10              | 60              | 28.8         | 3160       | PASS                |
| 365            | 198             | 1               | 100             | 4.4          | 485        | PASS                |
| 441            | 198             | 0.01            | 100             | 13.8         | 1513       | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 9561       | PASS                |
| 443            | 442             | 15              | 24              | 18.9         | 1803       | PASS                |

|                      |                         |                           |
|----------------------|-------------------------|---------------------------|
|                      | <b>DDT Breakdown</b>    |                           |
|                      |                         |                           |
|                      |                         |                           |
| <b>Date</b>          | <b>Instrument Name</b>  | <b>DFTPP Data File</b>    |
| <b>3/15/2021</b>     | <b>BNA_M</b>            | <b><u>BM029125.D</u></b>  |
|                      |                         |                           |
|                      |                         |                           |
| <b>Compound Name</b> | <b>Response</b>         | <b>Retention Time</b>     |
|                      |                         |                           |
| <b>DDT</b>           | <b>37342</b>            | <b>20.51</b>              |
| <b>DDD</b>           | <b>548</b>              | <b>20.08</b>              |
| <b>DDE</b>           | <b>0</b>                | <b>19.95</b>              |
|                      |                         |                           |
|                      |                         |                           |
| <b>SUM(DDD+DDE)</b>  | <b>SUM(DDT+DDD+DDE)</b> | <b>% Breakdown Of DDT</b> |
|                      |                         |                           |
| <b>548</b>           | <b>37890</b>            | <b>1.45</b>               |
|                      |                         |                           |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031521\  
Data File : BM029125.D  
Acq On : 15 Mar 2021 12:04  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Mar 15 12:45:14 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 12 12:30:15 2021  
Response via : Initial Calibration

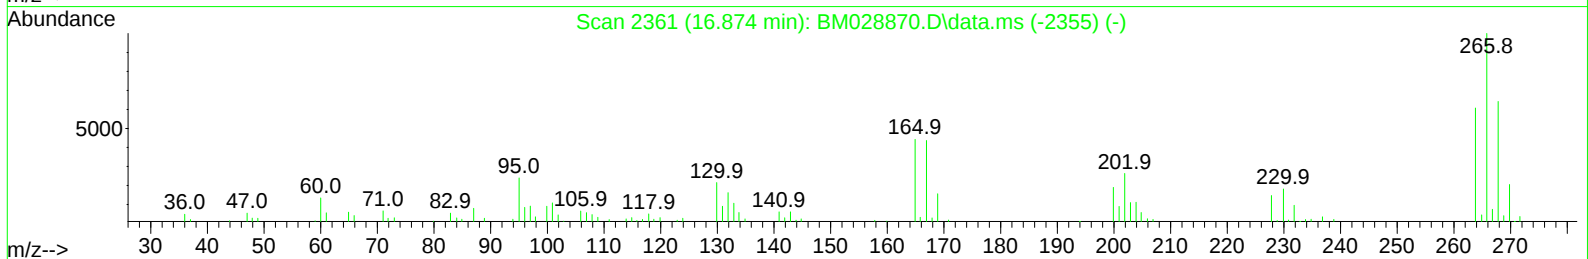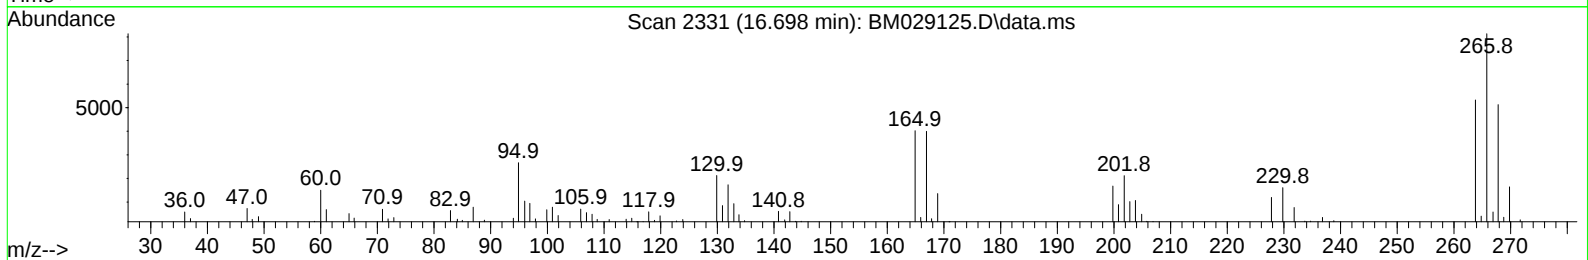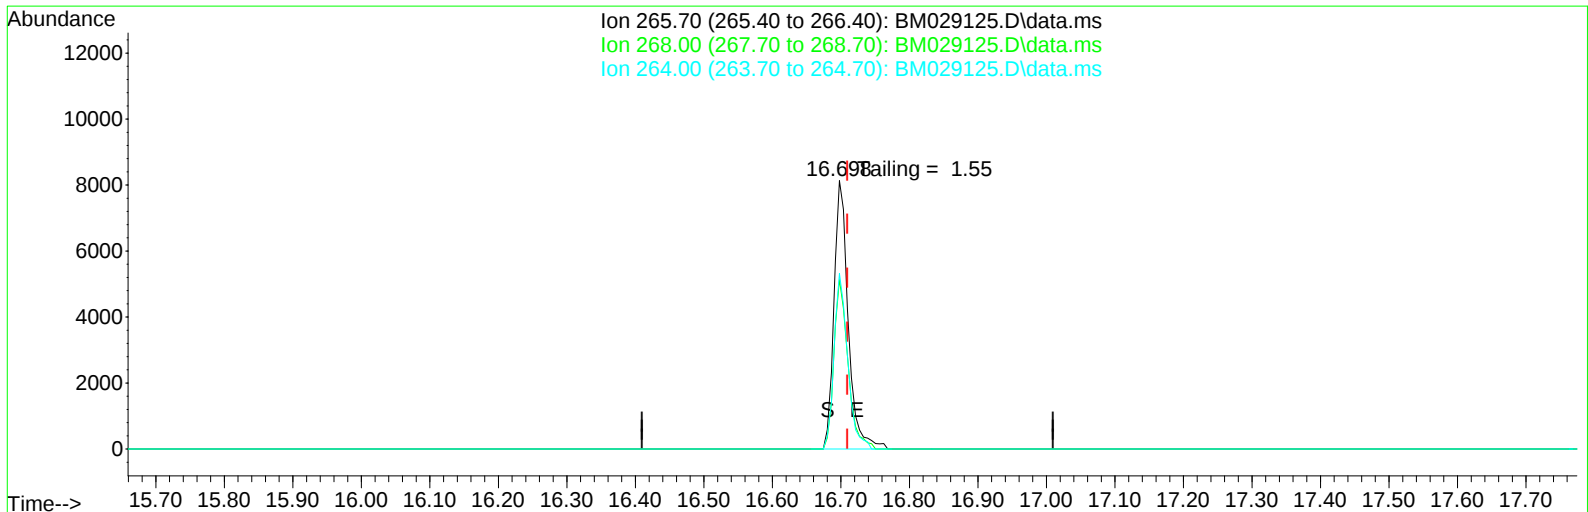

TIC: BM029125.D\data.ms

**(70) Pentachlorophenol (C)**

**16.698min (-0.012) 0.00 ng**




**response 11794**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.40  | 63.07  |
| 264.00 | 63.30  | 65.43  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031521\  
Data File : BM029125.D  
Acq On : 15 Mar 2021 12:04  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Mar 15 12:45:14 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 12 12:30:15 2021  
Response via : Initial Calibration

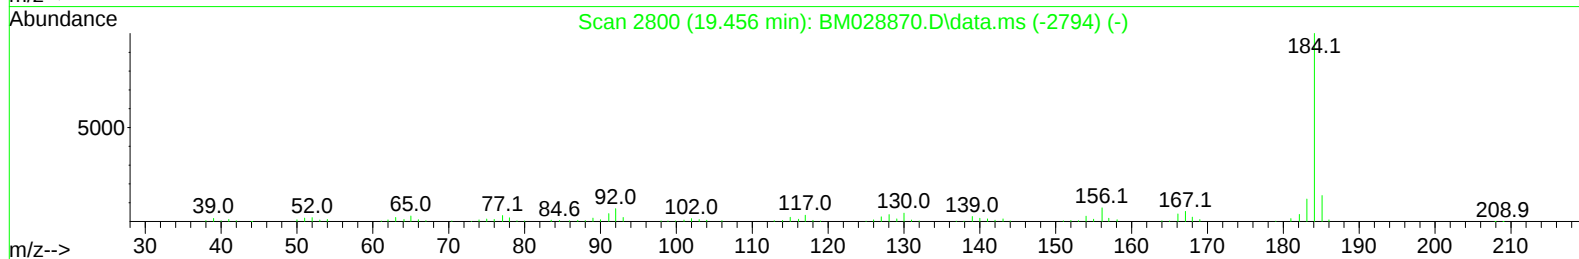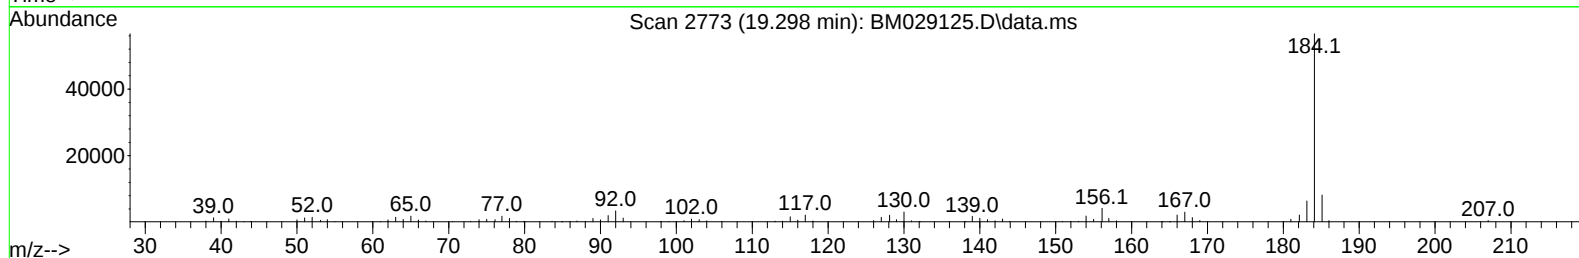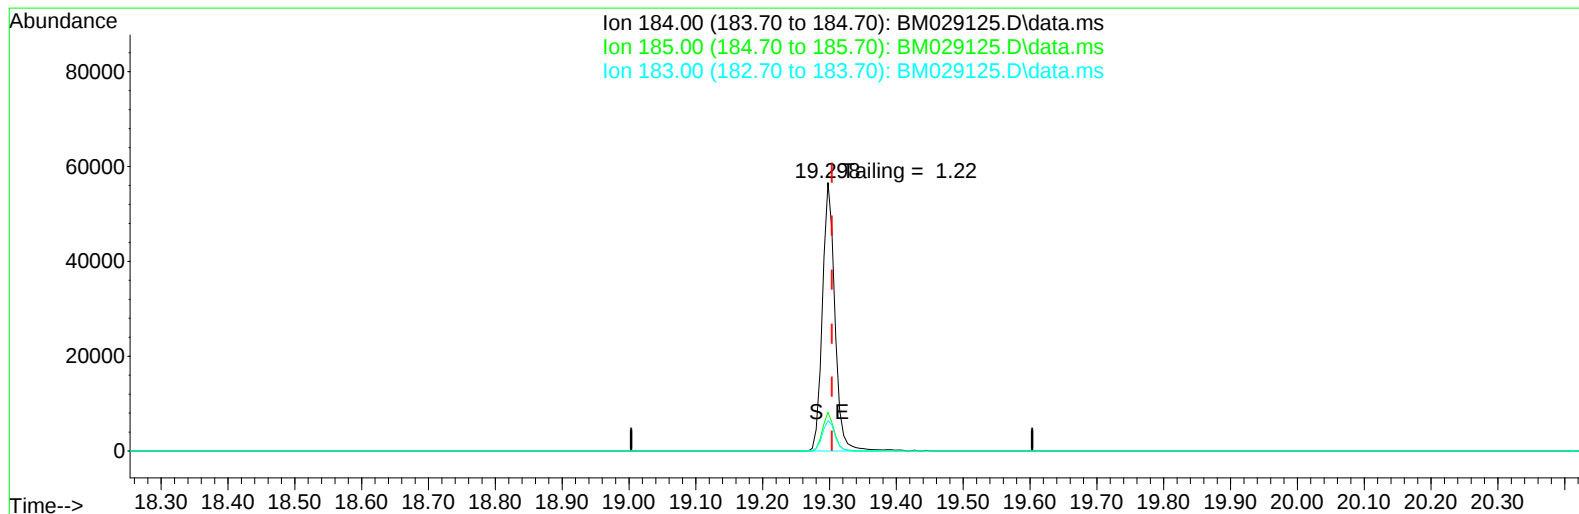

TIC: BM029125.D\data.ms

**(77) Benzidine**

**19.298min (-0.006) 33418.82 ng**

**response 73784**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.80  | 14.44  |
| 183.00 | 12.10  | 11.32  |
| 0.00   | 0.00   | 0.00   |