
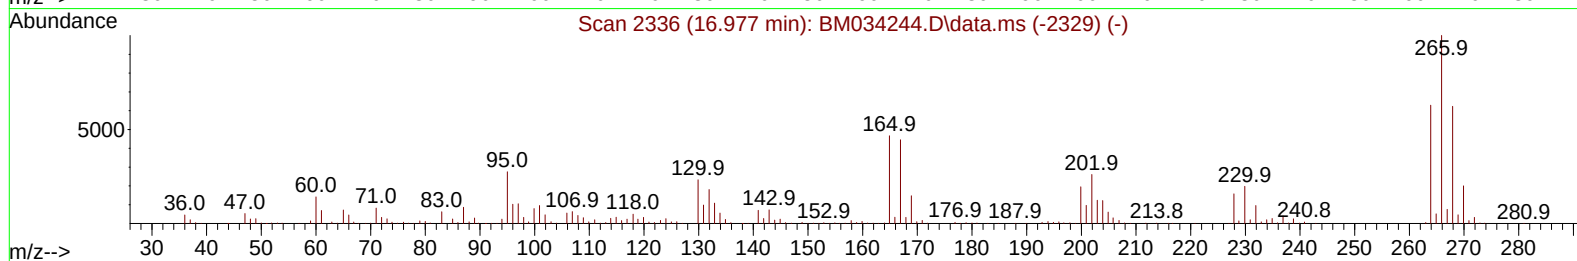
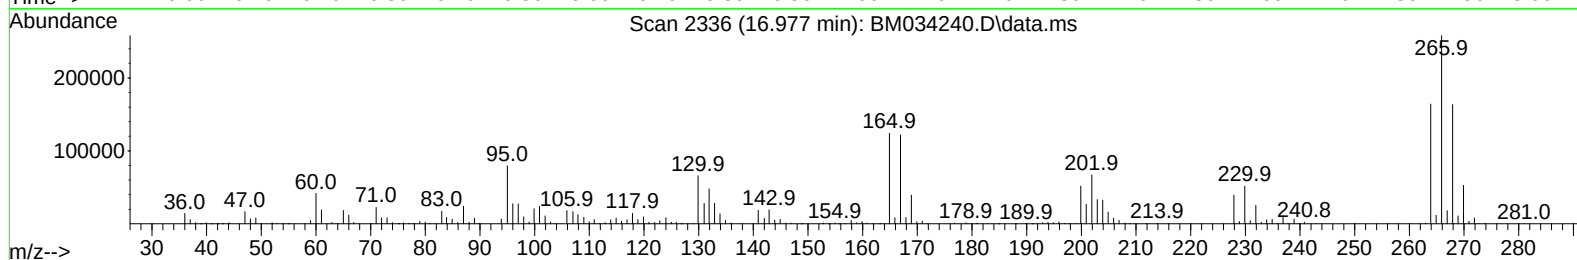


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031522\
Data File : BM034240.D
Acq On : 15 Mar 2022 15:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 03:11:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 16 02:38:26 2022
Response via : Initial Calibration

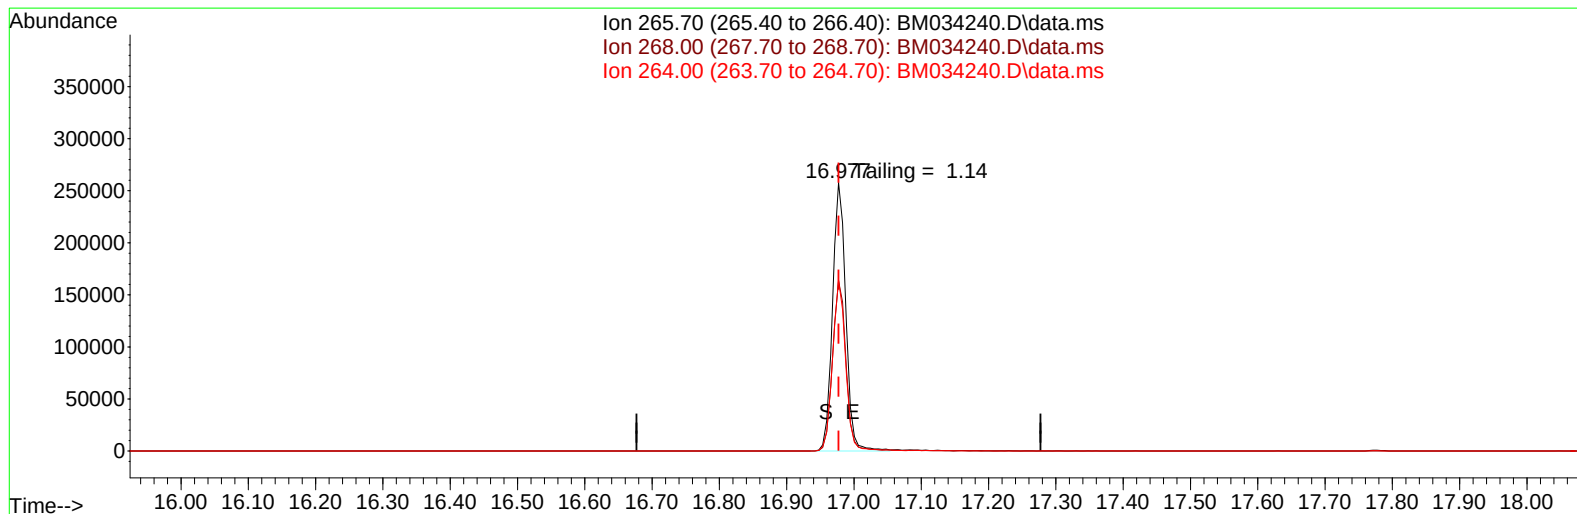

TIC: BM034240.D\data.ms

(70) Pentachlorophenol (C)




16.977min (+ 0.000) 0.00 ng

response 355273

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.41
264.00	62.90	63.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031522\
Data File : BM034240.D
Acq On : 15 Mar 2022 15:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 03:11:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 16 02:38:26 2022
Response via : Initial Calibration

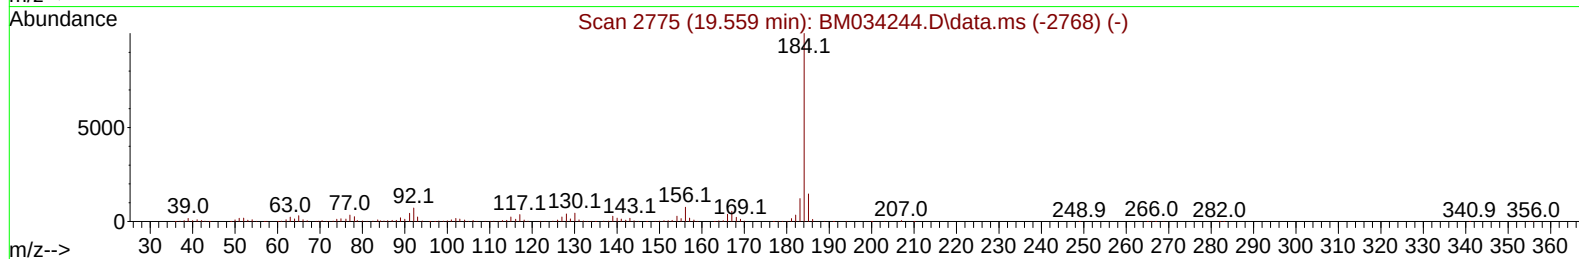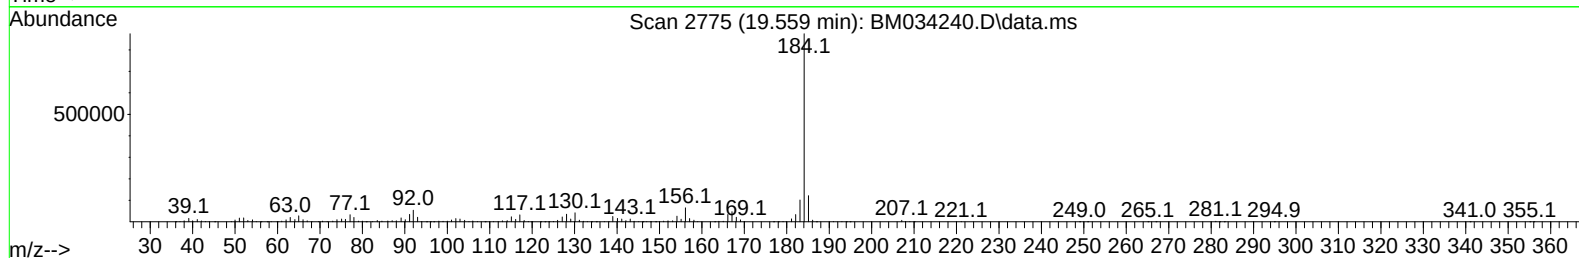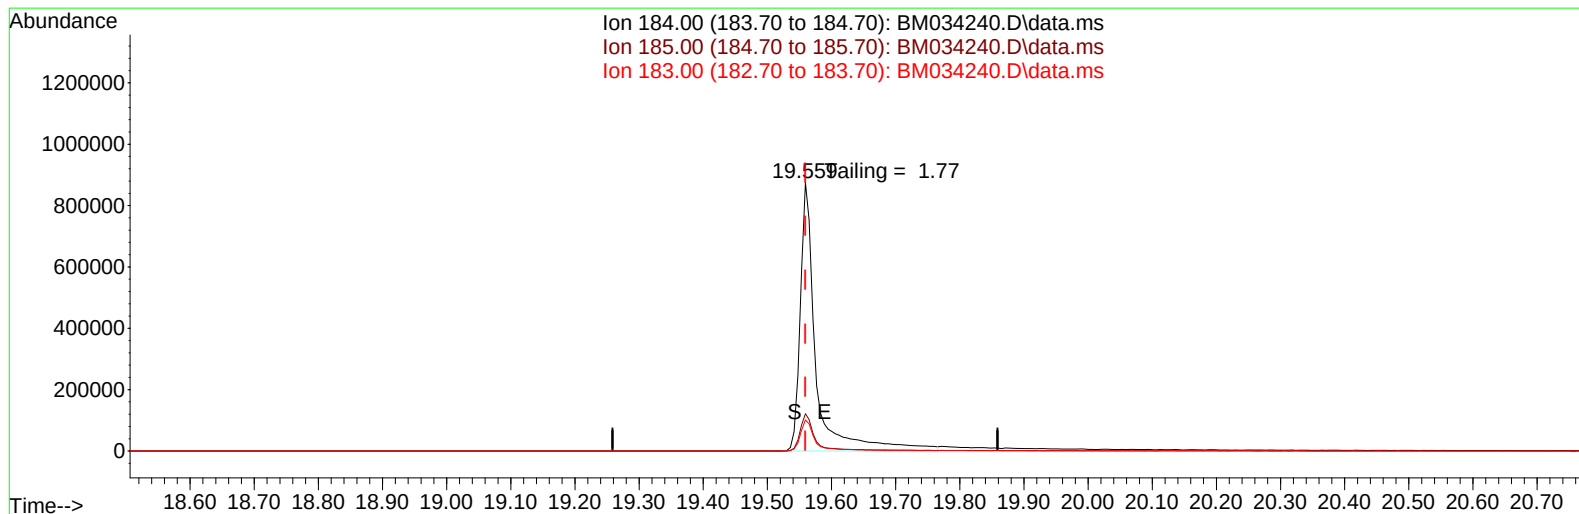

TIC: BM034240.D\data.ms

(77) Benzidine**19.559min (+ 0.000) 1076612.98 ng****response 1514599**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.90
183.00	12.20	11.60
0.00	0.00	0.00