

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031522\
 Data File : BM034249.D
 Acq On : 15 Mar 2022 22:01
 Operator : CG/JU
 Sample : PB143311BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB143311BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034249.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.502	378	385	398	rBV	3396215	4816450	70.95%	12.670%
2	7.107	650	658	671	rBV	3080226	4877295	71.84%	12.830%
3	7.948	794	801	813	rVB	568140	896739	13.21%	2.359%
4	9.113	991	999	1017	rBV	1872957	3137435	46.22%	8.253%
5	10.760	1272	1279	1290	rBV	651675	1119512	16.49%	2.945%
6	13.219	1690	1697	1709	rBV	4725130	6739334	99.27%	17.728%
7	14.589	1923	1930	1944	rBV	925601	1405773	20.71%	3.698%
8	16.071	2175	2182	2201	rBV	3218403	4663299	68.69%	12.267%
9	17.324	2389	2395	2408	rBV	943152	1399211	20.61%	3.681%
10	19.942	2834	2840	2856	rBV	5512834	6788675	100.00%	17.858%
11	21.495	3099	3104	3116	rBV	676024	1089699	16.05%	2.866%
12	23.912	3508	3515	3531	rBV2	451761	1081853	15.94%	2.846%




Sum of corrected areas: 38015275

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031522\
Data File : BM034249.D
Acq On : 15 Mar 2022 22:01
Operator : CG/JU
Sample : PB143311BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143311BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

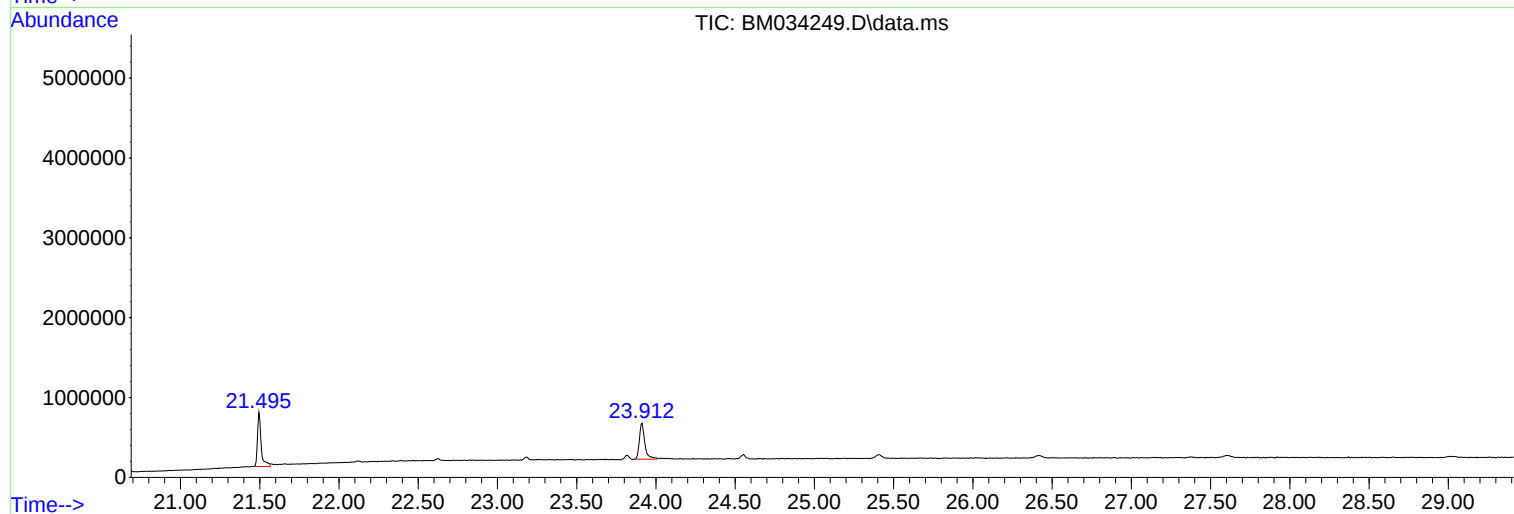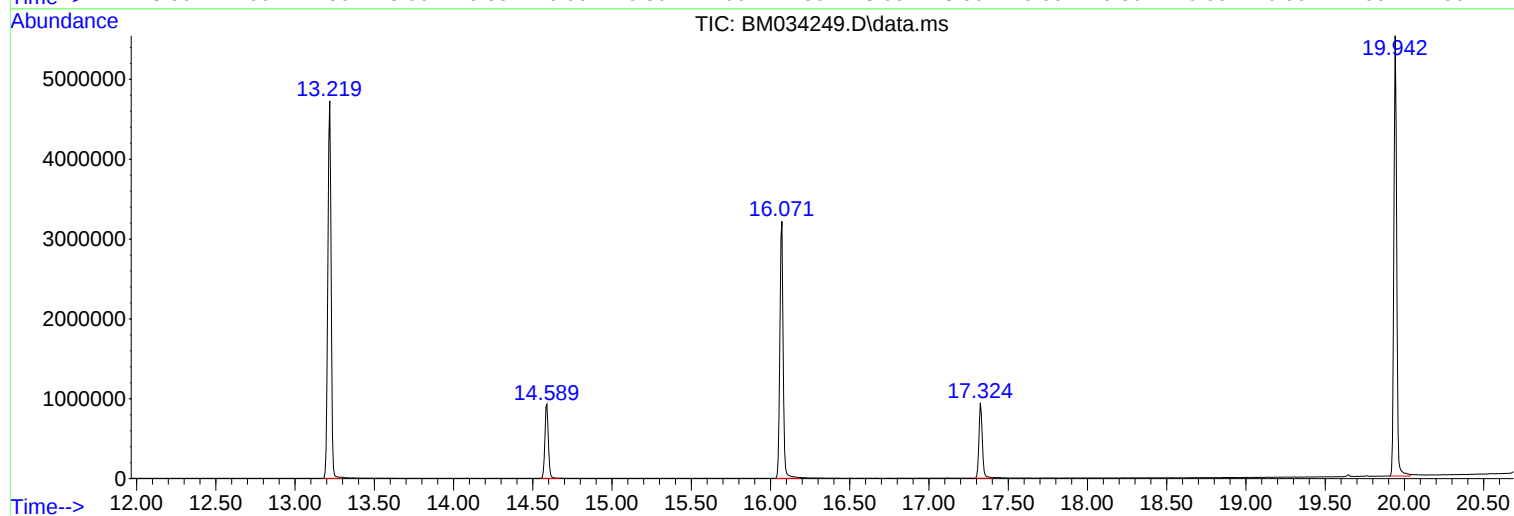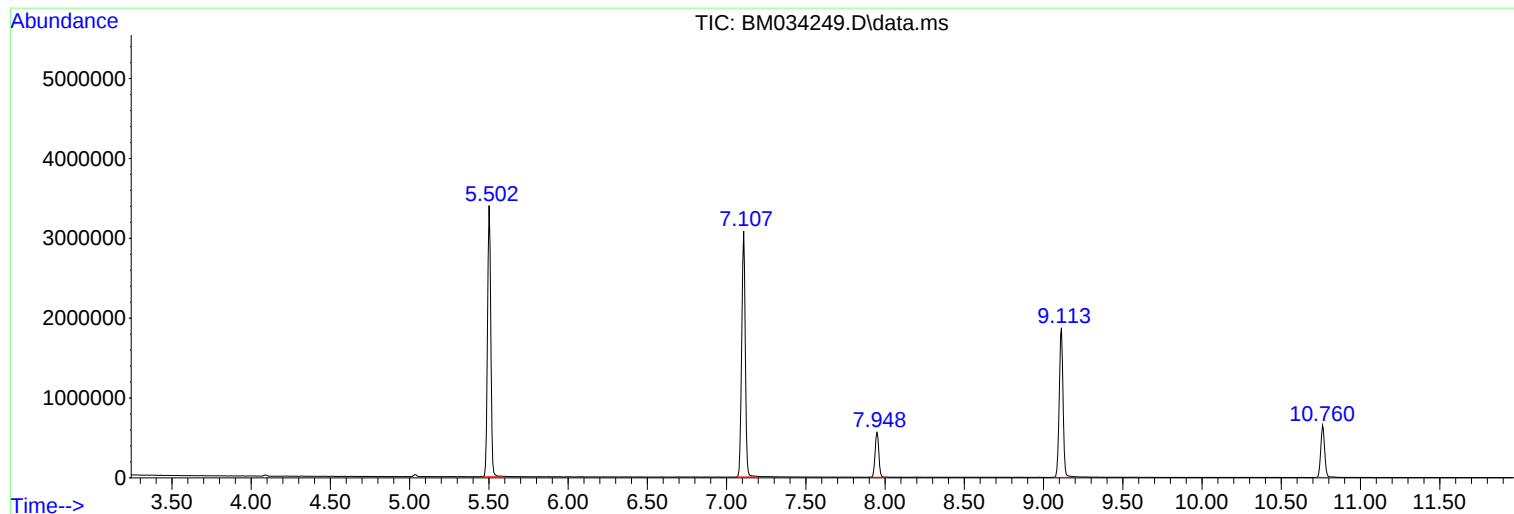

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031522\
Data File : BM034249.D
Acq On : 15 Mar 2022 22:01
Operator : CG/JU
Sample : PB143311BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143311BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031522\
Data File : BM034249.D
Acq On : 15 Mar 2022 22:01
Operator : CG/JU
Sample : PB143311BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143311BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------