


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031615\
Data File : BM000710.D
Acq On : 16 Mar 2015 10:39
Operator : TP/IZ
Sample : DFTPP37
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP38

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM031615.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 17 04:53:53 2015

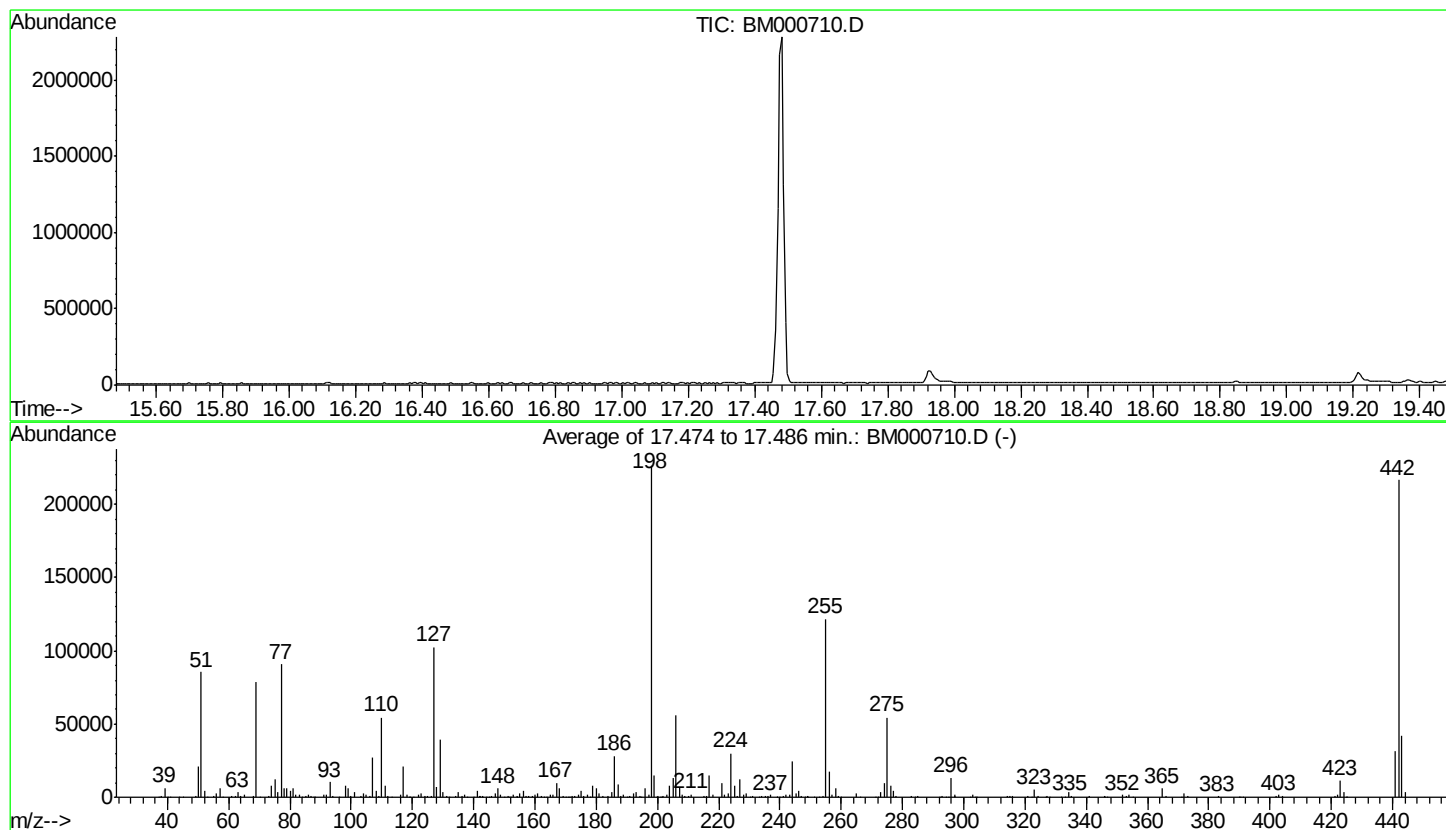

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	85357	PASS
68	69	0.00	2	1.5	1205	PASS
69	198	0.00	100	34.8	78917	PASS
70	69	0.00	2	0.4	317	PASS
127	198	10	80	45.2	102381	PASS
197	198	0.00	2	0.6	1393	PASS
198	198	100	100	100.0	226474	PASS
199	198	5	9	6.8	15297	PASS
275	198	10	60	24.1	54658	PASS
365	198	1	100	2.6	5806	PASS
441	443	0.01	100	75.1	31568	PASS
442	198	50	100	95.6	216448	PASS
443	442	15	24	19.4	42048	PASS