

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031616\
 Data File : BM004630.D
 Acq On : 16 Mar 2016 11:24
 Operator : UM/SJ
 Sample : PB88896BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 17 00:57:48 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM031516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 17 00:56:57 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	56155	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	247922	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.47	164	145867	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.22	188	346586	20.00	ng/ul	0.00
78) Chrysene-d12	21.40	240	395407	20.00	ng/ul	0.00
86) Perylene-d12	23.70	264	388558	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.33	96	9483	5.83	ng/uL	0.00
5) Phenol-d5	7.00	99	163554	35.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	98580	37.69	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	131906	35.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.54	113	128822	34.63	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	59120	34.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	62843	33.74	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	121023	33.13	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	184754	42.26	ng/ul	0.00
44) Dimethylphthalate-d6	13.89	166	410910	36.04	ng/ul	0.00
47) Acenaphthylene-d8	14.17	160	492887	35.25	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	65566	29.75	ng/ul	0.00
58) Fluorene-d10	15.47	176	363235	36.55	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.58	200	44004	24.16	ng/ul	0.00
71) Anthracene-d10	17.32	188	591981	37.10	ng/ul	0.00
79) Pyrene-d10	19.61	212	680596	37.71	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.56	264	716980	41.31	ng/ul	0.00


Target Compounds					Ovalue
46) 2,6-Dinitrotoluene	13.89	165	2798	1.36 ng/ul#	39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031616\
Data File : BM004630.D
Acq On : 16 Mar 2016 11:24
Operator : UM/SJ
Sample : PB88896BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 17 00:57:48 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 17 00:56:57 2016
Response via : Initial Calibration

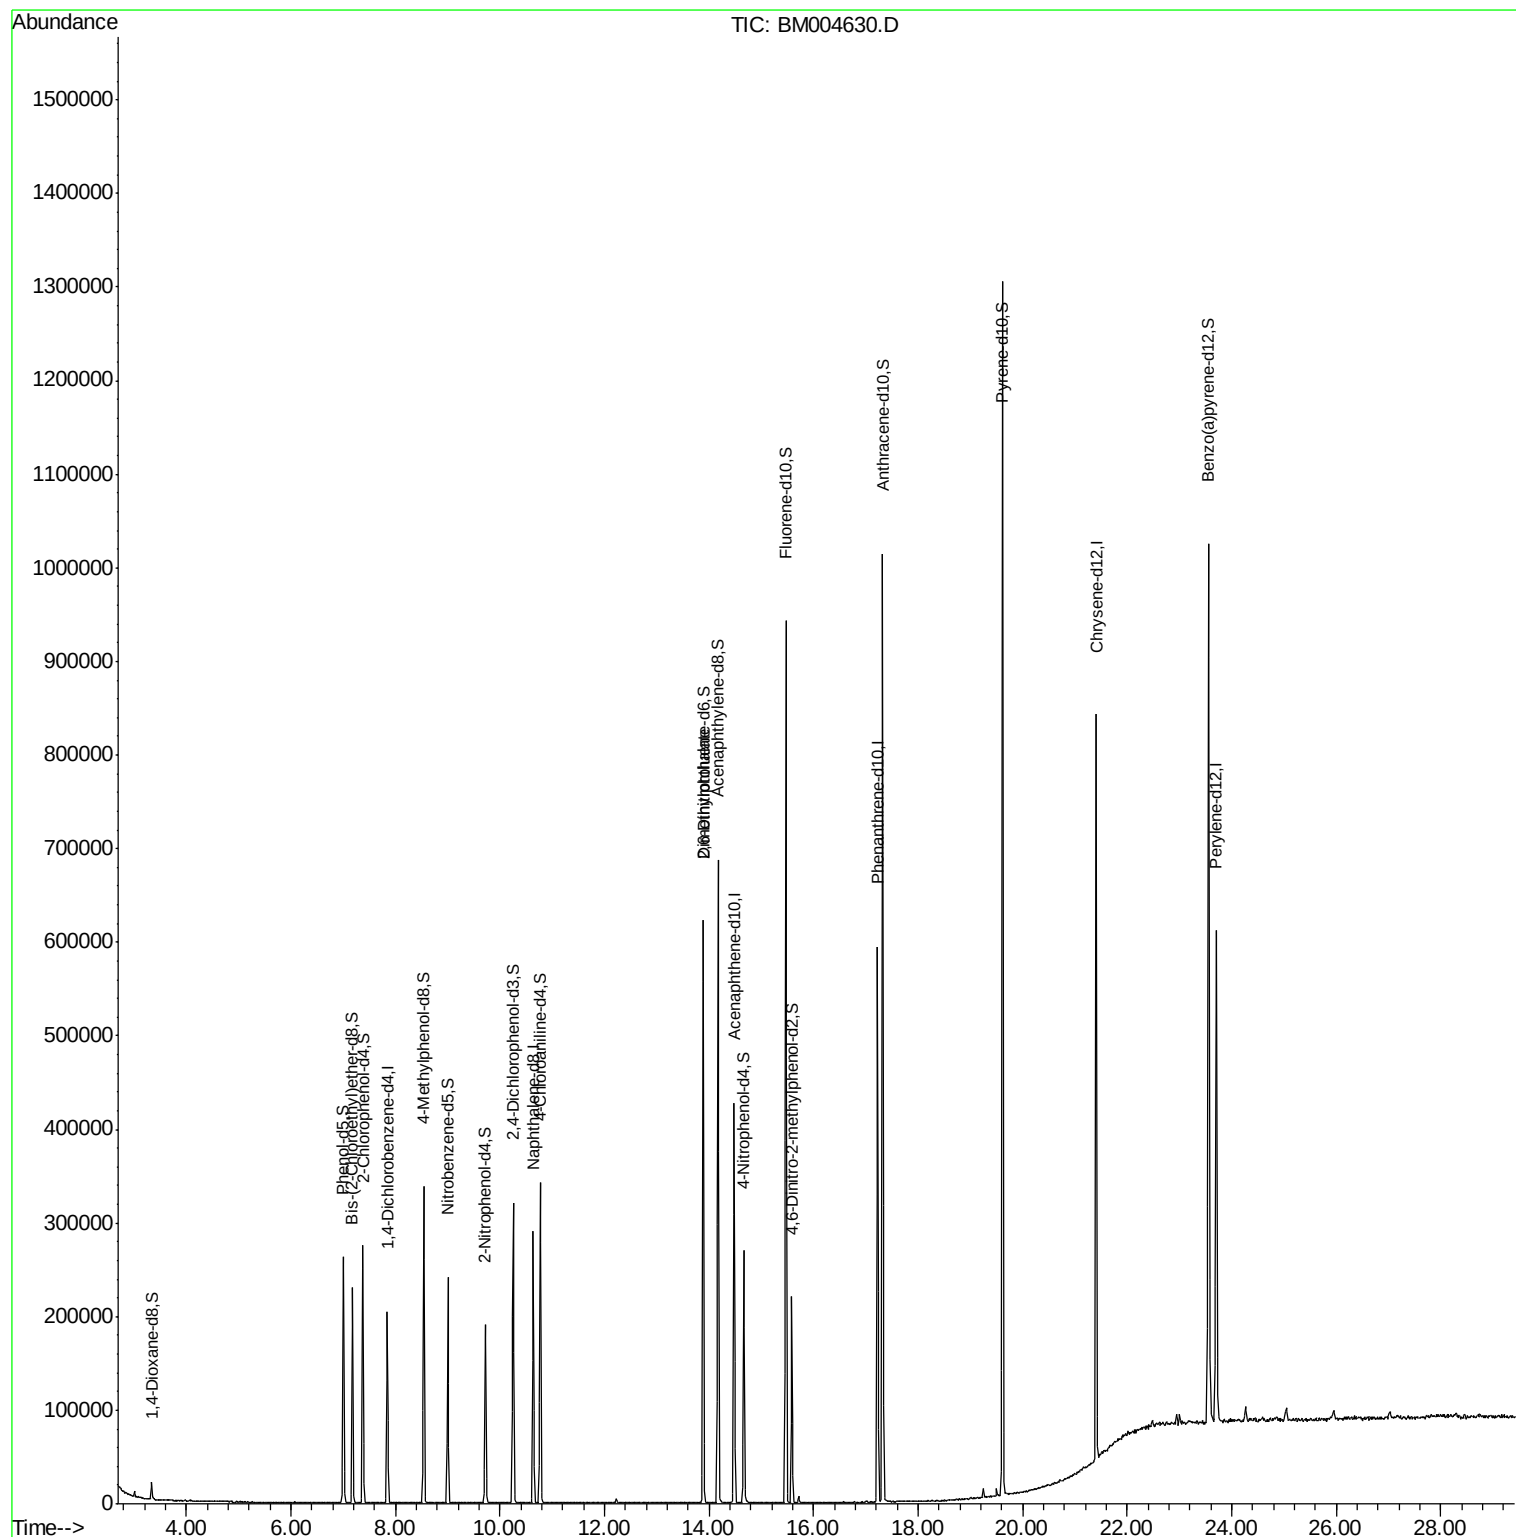

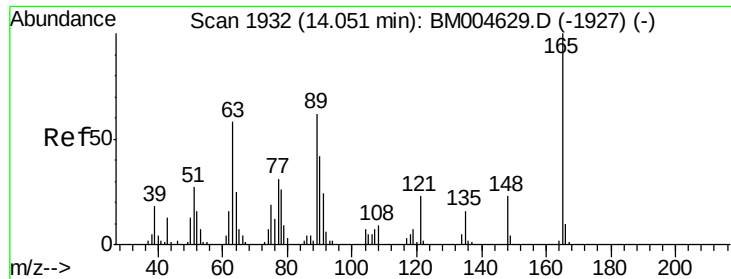

#46
 2,6-Dinitrotoluene
 Concen: 1.36 ng/ul
 RT: 13.89 min Scan# 1904
 Delta R.T. -0.16 min
 Lab File: BM004630.D
 Acq: 16 Mar 2016 11:24

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
89	0.0	42.4	63.6#
121	33.2	16.6	24.8#

