

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031616\
 Data File : BM004631.D
 Acq On : 16 Mar 2016 12:01
 Operator : UM/SJ
 Sample : PB88897BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 17 00:57:55 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM031516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 17 00:56:57 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	58353	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	260690	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.47	164	153997	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.22	188	360396	20.00	ng/ul	0.00
78) Chrysene-d12	21.40	240	412488	20.00	ng/ul	0.00
86) Perylene-d12	23.70	264	397682	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.33	96	8518	5.04	ng/uL	0.00
5) Phenol-d5	7.00	99	149678	31.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	89905	33.08	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	120632	31.25	ng/ul	0.00
13) 4-Methylphenol-d8	8.54	113	119487	30.91	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	53463	29.49	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	56939	29.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	110848	28.86	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	172799	37.59	ng/ul	0.00
44) Dimethylphthalate-d6	13.89	166	399713	33.20	ng/ul	0.00
47) Acenaphthylene-d8	14.17	160	468404	31.73	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	63659	27.36	ng/ul	0.00
58) Fluorene-d10	15.47	176	352512	33.60	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.58	200	42926	22.66	ng/ul	0.00
71) Anthracene-d10	17.32	188	579601	34.93	ng/ul	0.00
79) Pyrene-d10	19.61	212	669433	35.55	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.56	264	702881	39.57	ng/ul	0.00


Target Compounds					Ovalue
46) 2,6-Dinitrotoluene	13.89	165	2766	1.27 ng/ul#	41




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031616\
Data File : BM004631.D
Acq On : 16 Mar 2016 12:01
Operator : UM/SJ
Sample : PB88897BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 17 00:57:55 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 17 00:56:57 2016
Response via : Initial Calibration

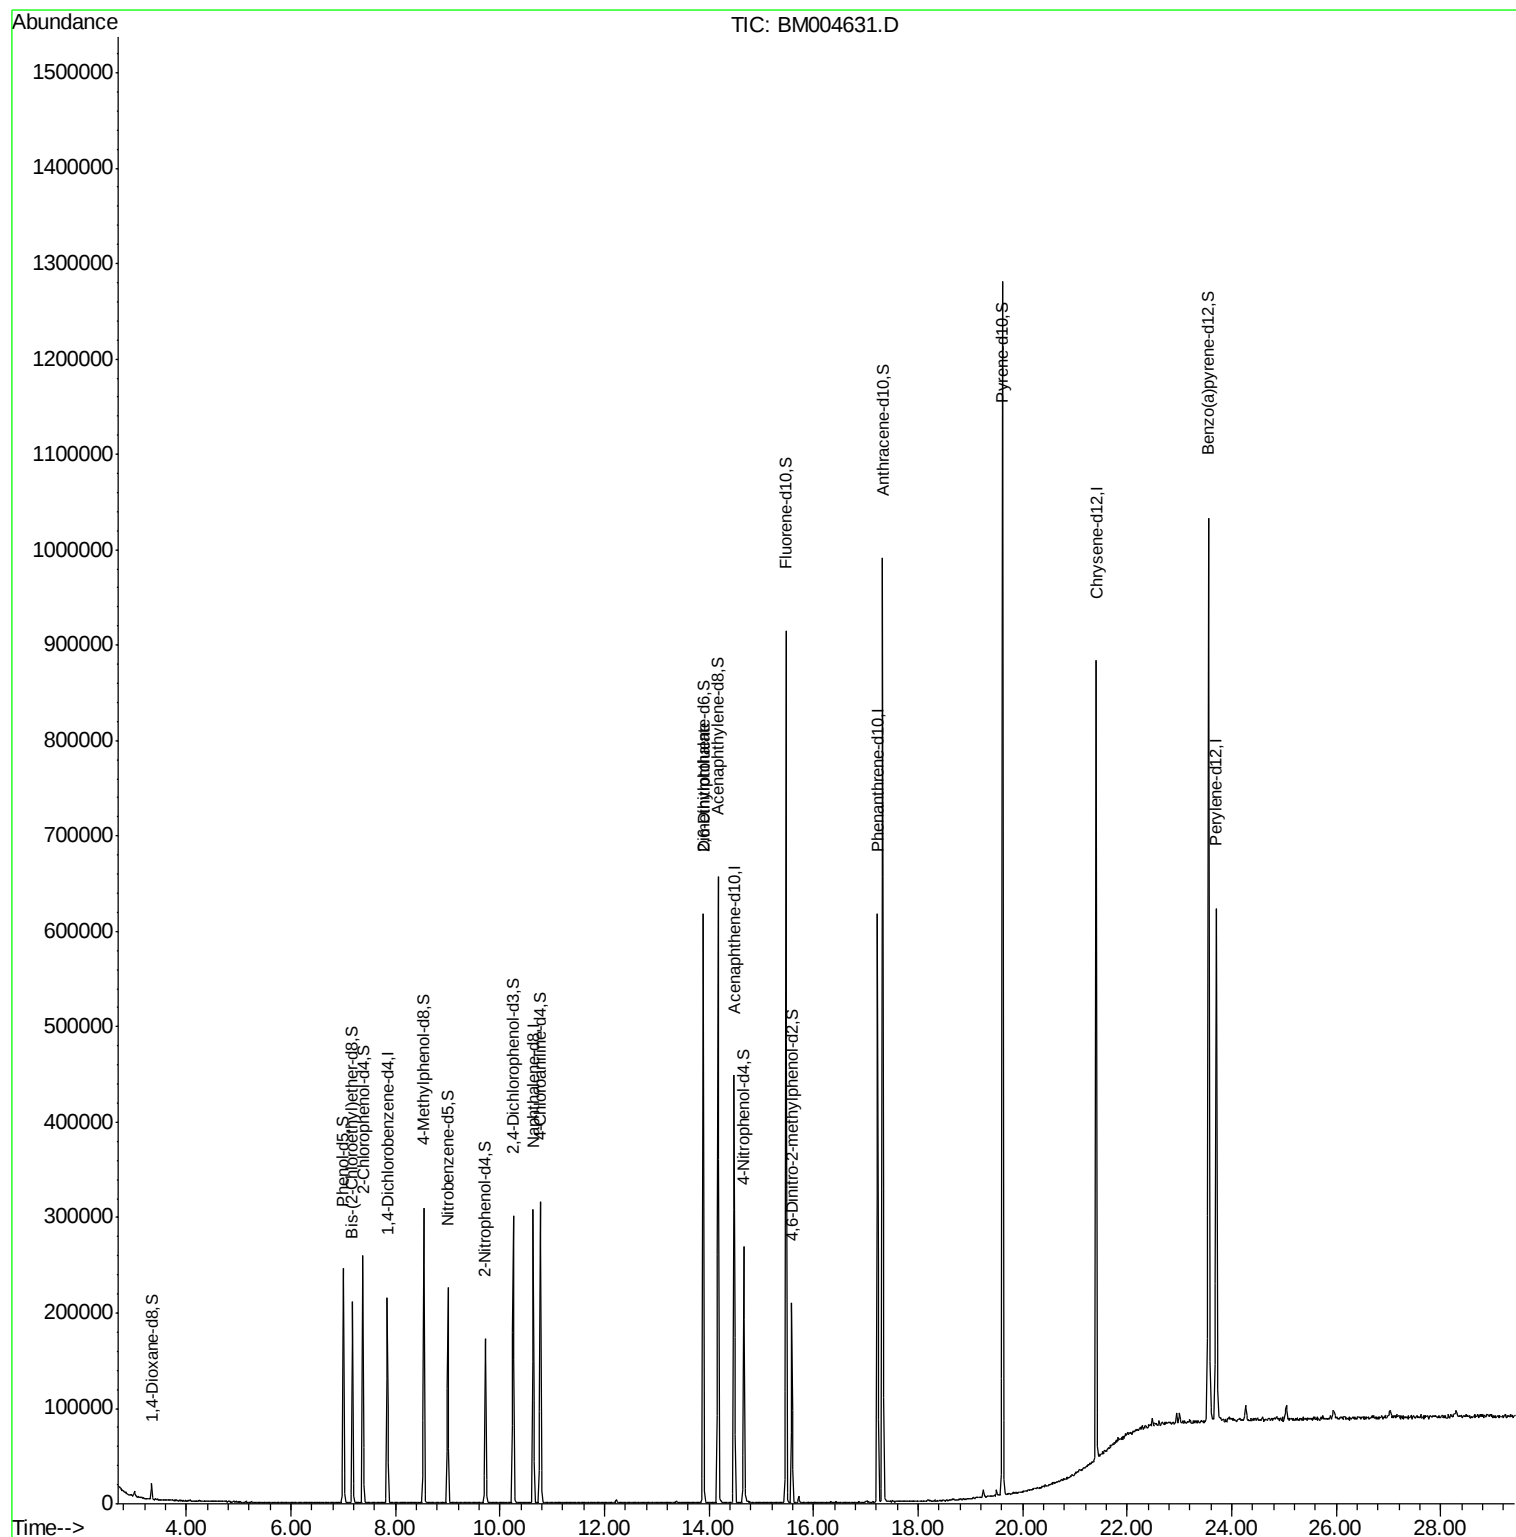

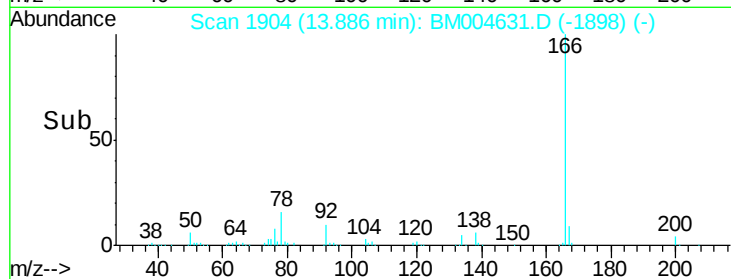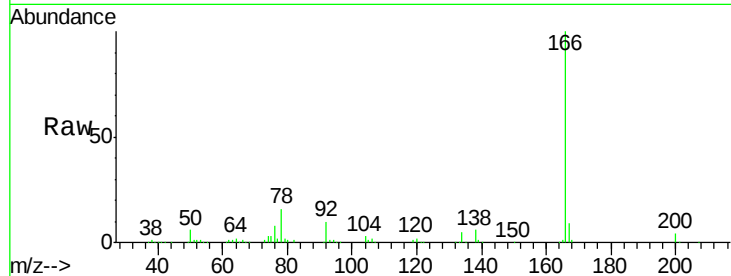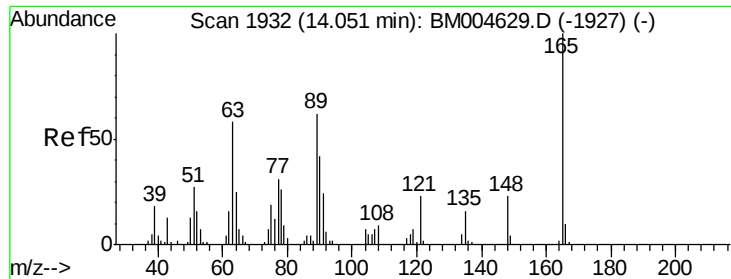

#46

2,6-Dinitrotoluene

Concen: 1.27 ng/ul

RT: 13.89 min Scan# 1904

Delta R.T. -0.16 min

Lab File: BM004631.D

Acq: 16 Mar 2016 12:01

Instrument :

BNA_M

ClientSampleId :

Tot Ion:165 Resp: 2766

Ion Ratio Lower Upper

165 100

89 0.0 42.4 63.6#

121 30.0 16.6 24.8#

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

