

Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM031616\  
 Data File : BM004639.D  
 Acq On : 16 Mar 2016 16:52  
 Operator : UM/SJ  
 Sample : H1783-06  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 C0AA6

Quant Time: Mar 17 01:47:18 2016  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM02.2-EPA-BM031516.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Mar 17 00:56:57 2016  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.87  | 152  | 41484    | 20.00 | ng/ul | 0.02     |
| 18) Naphthalene-d8        | 10.66 | 136  | 263002   | 20.00 | ng/ul | 0.03     |
| 36) Acenaphthene-d10      | 14.47 | 164  | 137630   | 20.00 | ng/ul | 0.00     |
| 62) Phenanthrene-d10      | 17.22 | 188  | 300170   | 20.00 | ng/ul | 0.00     |
| 78) Chrysene-d12          | 21.40 | 240  | 346350   | 20.00 | ng/ul | 0.00     |
| 86) Perylene-d12          | 23.70 | 264  | 342549   | 20.00 | ng/ul | 0.00     |

## System Monitoring Compounds

|                                |       |     |        |       |       |      |
|--------------------------------|-------|-----|--------|-------|-------|------|
| 3) 1,4-Dioxane-d8              | 3.34  | 96  | 2080   | 1.73  | ng/uL | 0.00 |
| 5) Phenol-d5                   | 7.00  | 99  | 38676  | 11.35 | ng/ul | 0.00 |
| 7) Bis-(2-Chloroethyl)ether-d  | 7.19  | 67  | 110551 | 57.22 | ng/ul | 0.02 |
| 9) 2-Chlorophenol-d4           | 7.39  | 132 | 120662 | 43.97 | ng/ul | 0.01 |
| 13) 4-Methylphenol-d8          | 8.55  | 113 | 72673  | 26.45 | ng/ul | 0.00 |
| 19) Nitrobenzene-d5            | 9.01  | 128 | 68965  | 37.70 | ng/ul | 0.01 |
| 22) 2-Nitrophenol-d4           | 9.73  | 143 | 71625  | 36.25 | ng/ul | 0.01 |
| 26) 2,4-Dichlorophenol-d3      | 10.26 | 165 | 124234 | 32.06 | ng/ul | 0.00 |
| 29) 4-Chloroaniline-d4         | 10.78 | 131 | 1051   | 0.23  | ng/ul | 0.01 |
| 44) Dimethylphthalate-d6       | 13.89 | 166 | 379820 | 35.30 | ng/ul | 0.00 |
| 47) Acenaphthylene-d8          | 14.17 | 160 | 493676 | 37.42 | ng/ul | 0.00 |
| 52) 4-Nitrophenol-d4           | 14.66 | 143 | 8910   | 4.28  | ng/ul | 0.00 |
| 58) Fluorene-d10               | 15.47 | 176 | 346571 | 36.96 | ng/ul | 0.00 |
| 63) 4,6-Dinitro-2-methylphenol | 15.58 | 200 | 41845  | 26.53 | ng/ul | 0.00 |
| 71) Anthracene-d10             | 17.32 | 188 | 527276 | 38.15 | ng/ul | 0.00 |
| 79) Pyrene-d10                 | 19.61 | 212 | 601752 | 38.06 | ng/ul | 0.00 |
| 90) Benzo(a)pyrene-d12         | 23.56 | 264 | 649520 | 42.45 | ng/ul | 0.00 |

## Target Compounds


|                                |       |     |        |        |        | Qvalue |
|--------------------------------|-------|-----|--------|--------|--------|--------|
| 6) Phenol                      | 7.03  | 94  | 4183   | 1.17   | ng/ul# | 91     |
| 10) 2-Chlorophenol             | 7.42  | 128 | 13207  | 4.56   | ng/ul# | 89     |
| 20) Nitrobenzene               | 9.05  | 77  | 435864 | 96.57  | ng/ul  | 97     |
| 23) 2-Nitrophenol              | 9.76  | 139 | 2293   | 1.05   | ng/ul# | 76     |
| 28) Naphthalene                | 10.70 | 128 | 51356  | 3.74   | ng/ul  | 99     |
| 37) 1,2,4,5-Tetrachlorobenzene | 12.66 | 216 | 165947 | 37.74  | ng/ul  | 98     |
| 73) 1,2,3,4-Tetrachlorobenzene | 13.27 | 216 | 476093 | 115.28 | ng/uL  | 100    |
| 74) Pentachlorobenzene         | 14.79 | 250 | 8661   | 2.17   | ng/uL  | 91     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM031616\  
Data File : BM004639.D  
Acq On : 16 Mar 2016 16:52  
Operator : UM/SJ  
Sample : H1783-06  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
C0AA6

Quant Time: Mar 17 01:47:18 2016  
Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM02.2-EPA-BM031516.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Thu Mar 17 00:56:57 2016  
Response via : Initial Calibration

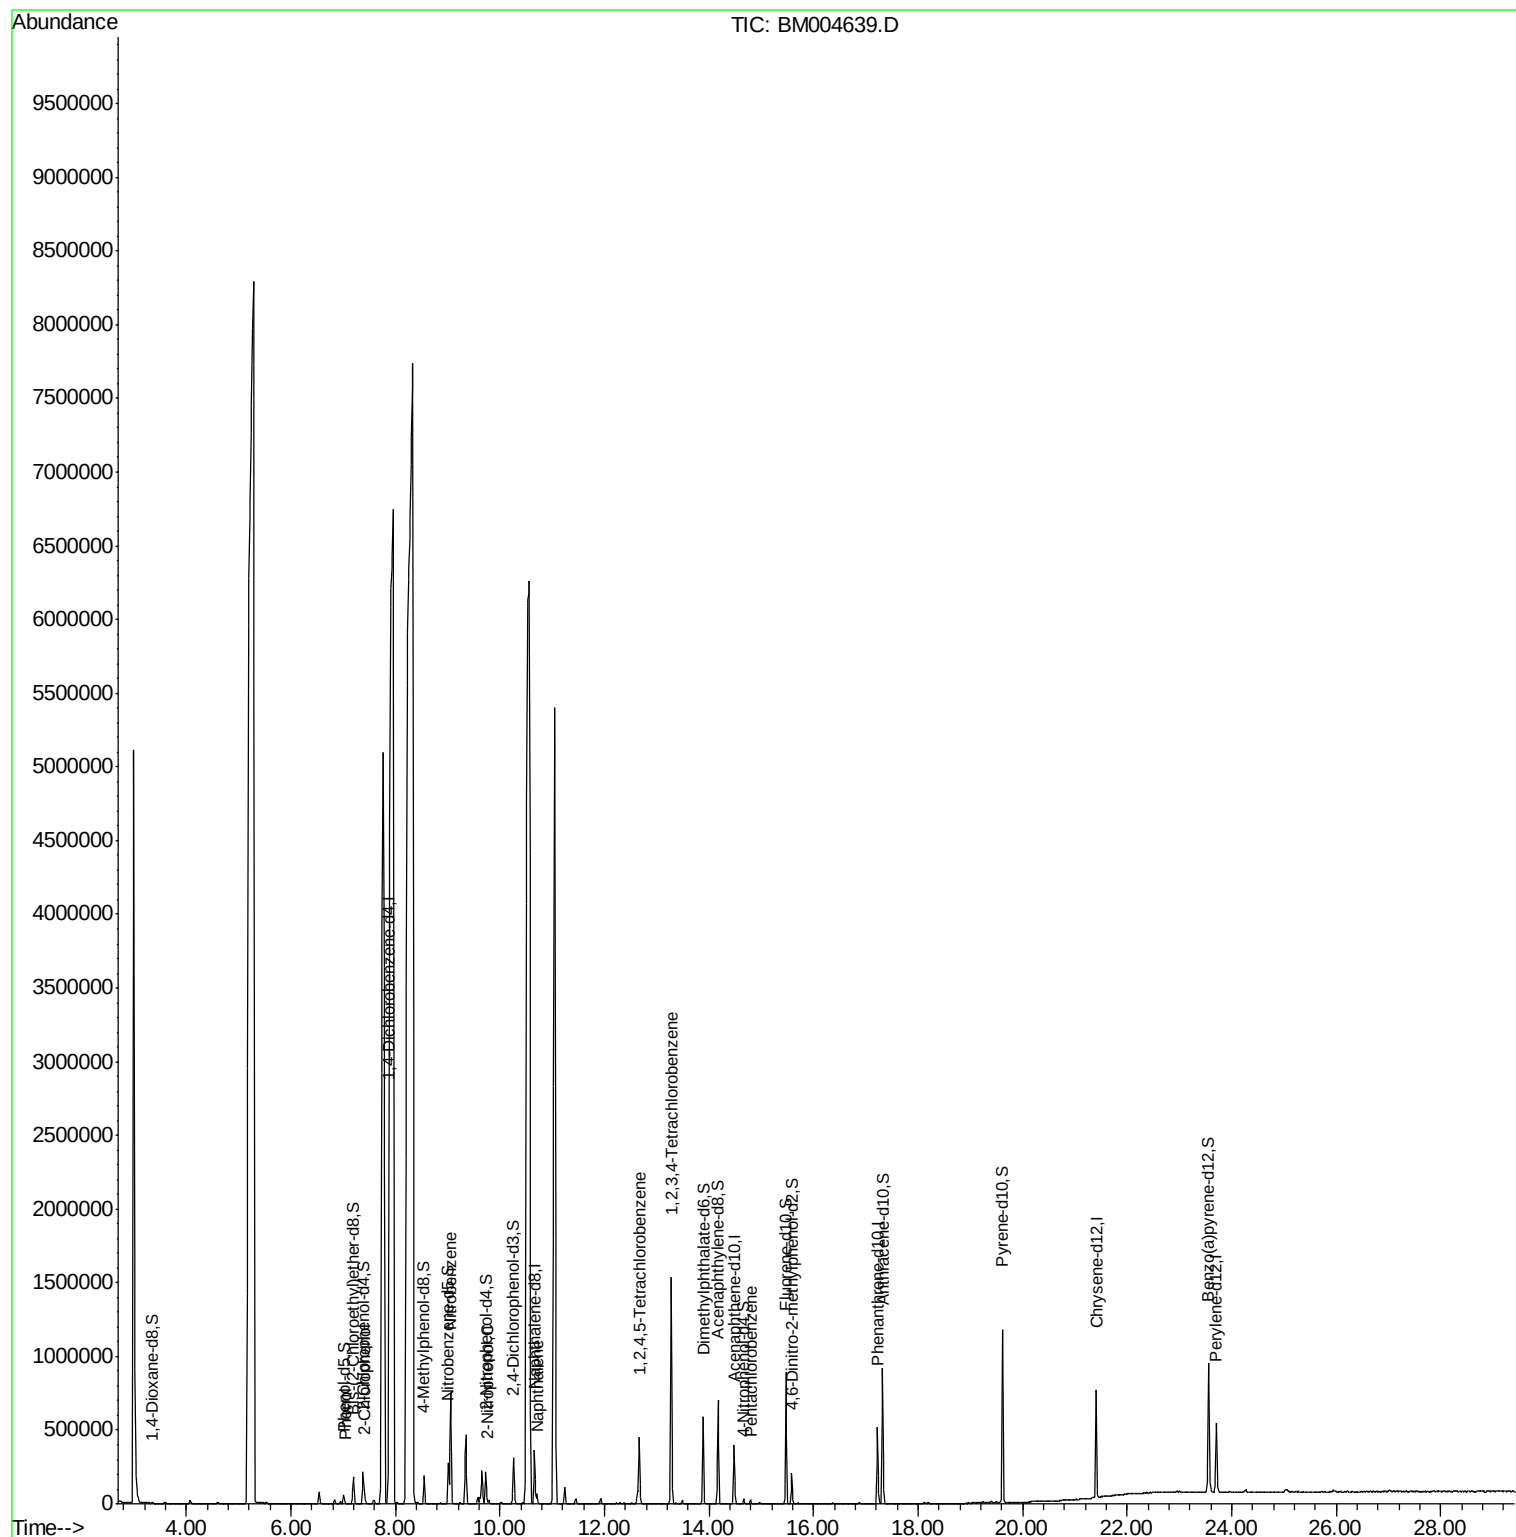

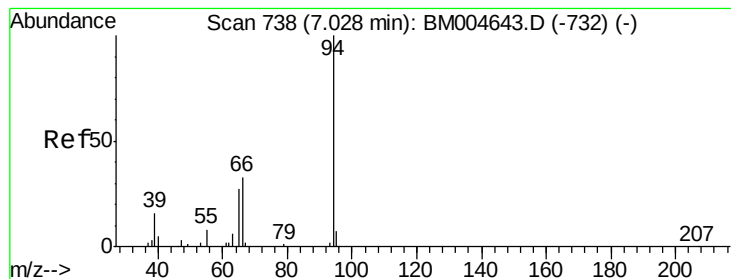

#6

Phenol

Concen: 1.17 ng/ul

RT: 7.03 min Scan# 739

Delta R.T. 0.01 min

Lab File: BM004639.D

Acq: 16 Mar 2016 16:52

Instrument :

BNA\_M

ClientSampleId :

C0AA6


Tgt Ion: 94 Resp: 4183

Ion Ratio Lower Upper

94 100

65 26.9 21.0 31.6




66 45.7 29.3 43.9#

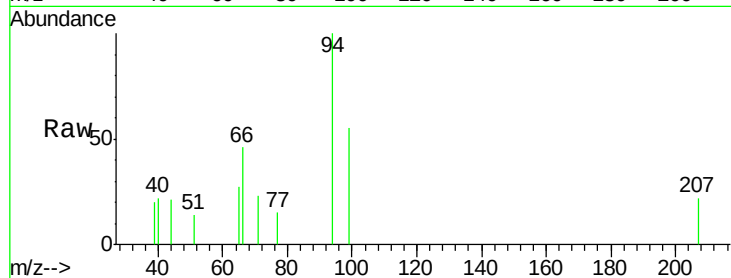

Abundance Ion 94.00 (93.70 to 94.70): BM004643.D (-732) (-)

Ion 65.00 (64.70 to 65.70): BM004643.D (-732) (-)

Ion 66.00 (65.70 to 66.70): BM004643.D (-732) (-)

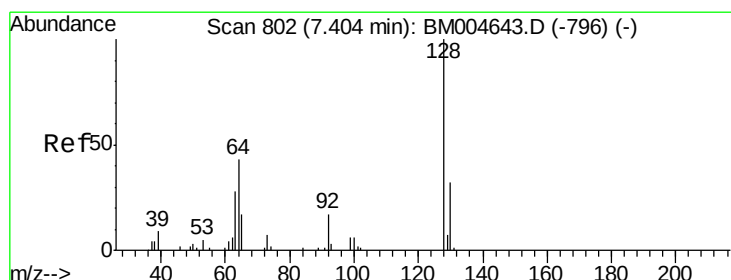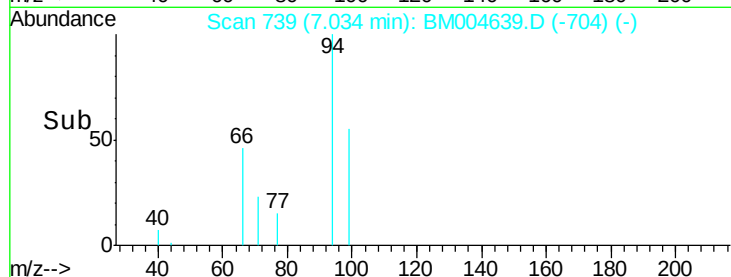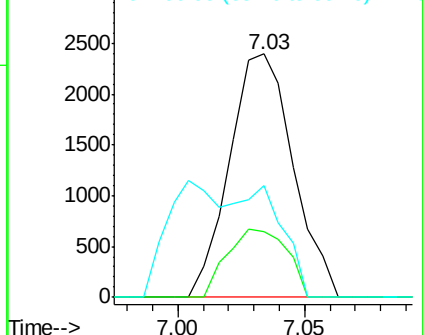

#10

2-Chlorophenol

Concen: 4.56 ng/ul

RT: 7.42 min Scan# 804

Delta R.T. 0.01 min

Lab File: BM004639.D

Acq: 16 Mar 2016 16:52


Tgt Ion: 128 Resp: 13207

Ion Ratio Lower Upper

128 100

64 49.7 31.9 47.9#



130 35.0 25.6 38.4

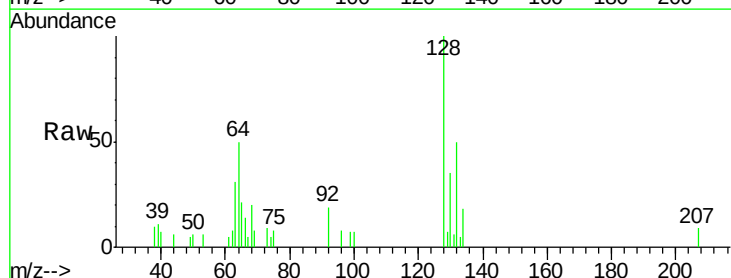


Abundance Ion 128.00 (127.70 to 128.70): BM004643.D (-796) (-)

Ion 64.00 (63.70 to 64.70): BM004643.D (-796) (-)

Ion 130.00 (129.70 to 130.70): BM004643.D (-796) (-)



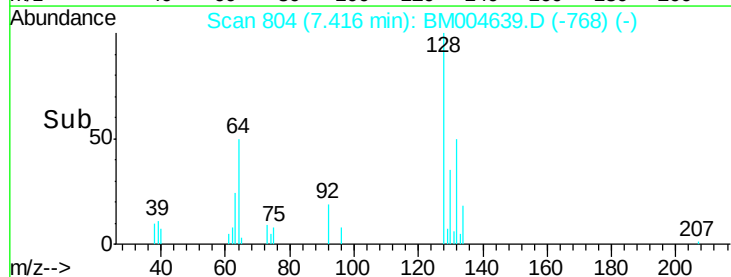
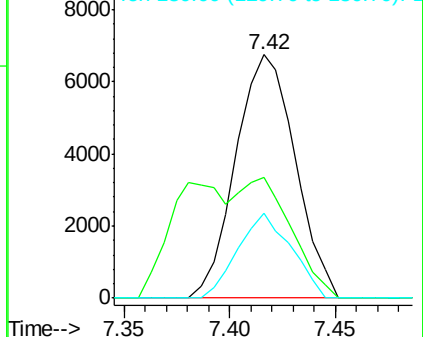


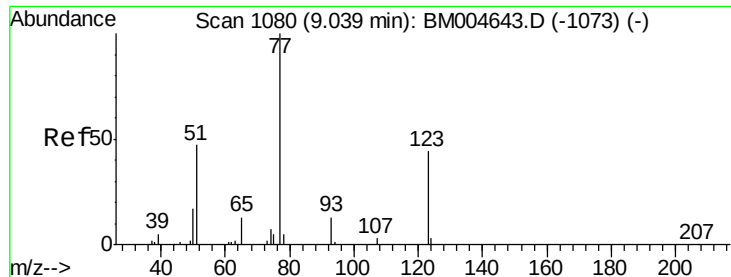

#20  
Nitrobenzene  
Concen: 96.57 ng/ul  
RT: 9.05 min Scan# 1082  
Delta R.T. 0.01 min  
Lab File: BM004639.D  
Acq: 16 Mar 2016 16:52




Instrument :  
BNA\_M  
ClientSampleId :  
C0AA6


| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 77      | 100   |       |       |
| 123     | 46.1  | 39.0  | 58.4  |
| 65      | 13.3  | 10.4  | 15.6  |

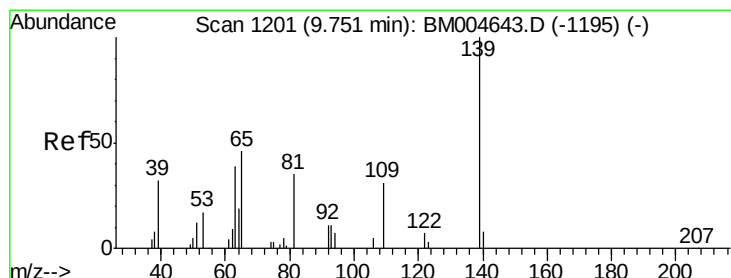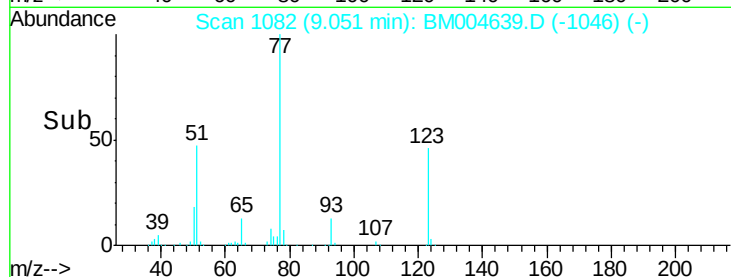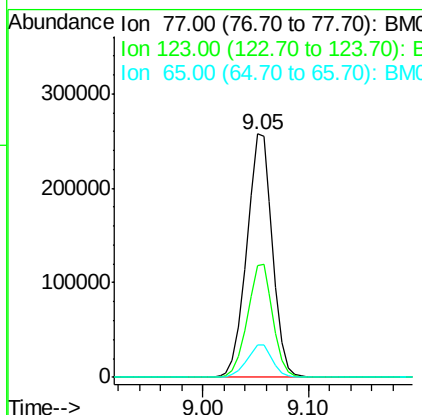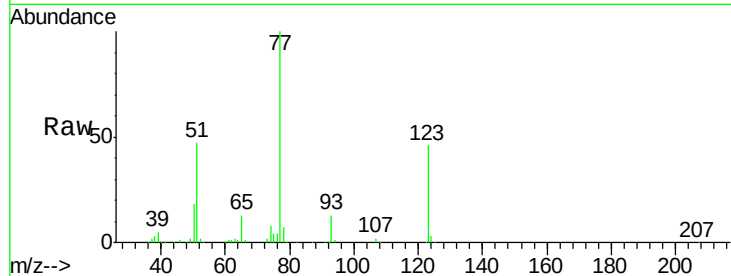

#23  
2-Nitrophenol  
Concen: 1.05 ng/ul  
RT: 9.76 min Scan# 1202  
Delta R.T. 0.01 min  
Lab File: BM004639.D  
Acq: 16 Mar 2016 16:52

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 139     | 100   |       |       |
| 65      | 65.9  | 36.3  | 54.5# |
| 109     | 40.2  | 26.4  | 39.6# |

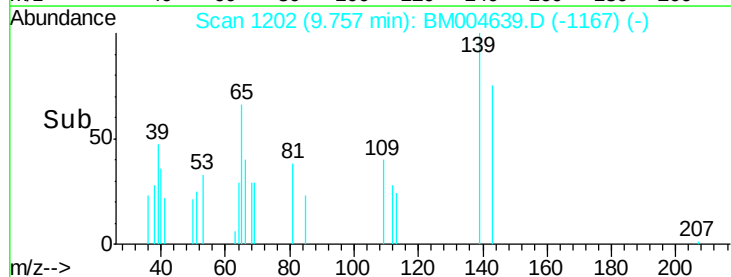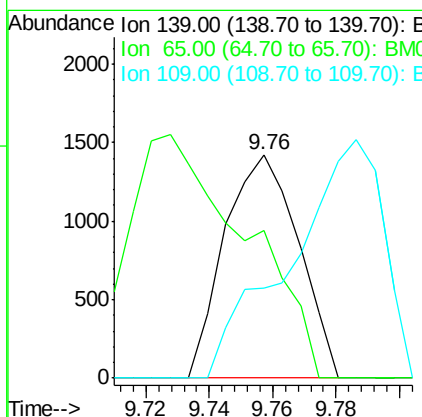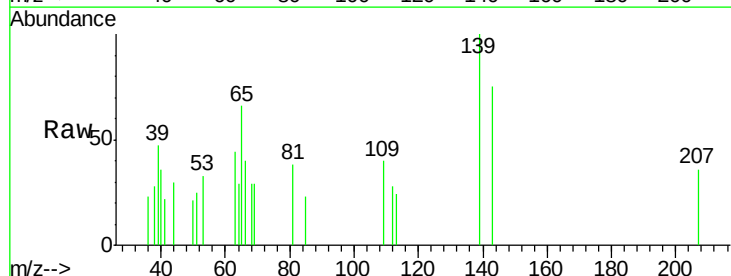

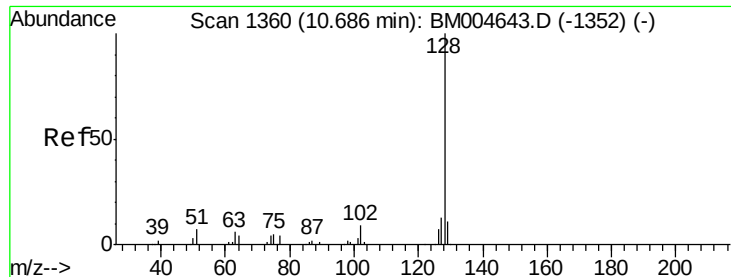

#28

Naphthalene

Concen: 3.74 ng/ul

RT: 10.70 min Scan# 1363

Delta R.T. 0.02 min

Lab File: BM004639.D

Acq: 16 Mar 2016 16:52

Instrument :

BNA\_M

ClientSampleId :

C0AA6


Tgt Ion:128 Resp: 51356

Ion Ratio Lower Upper

128 100

129 10.7 8.8 13.2




127 12.3 10.5 15.7

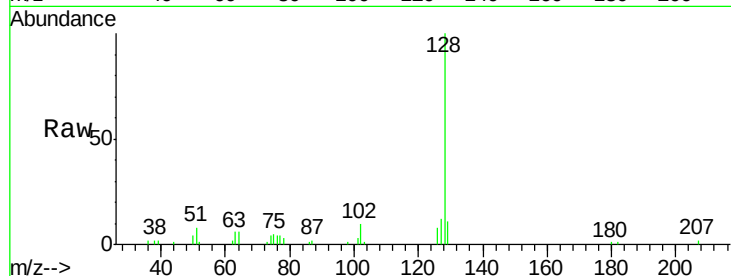

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

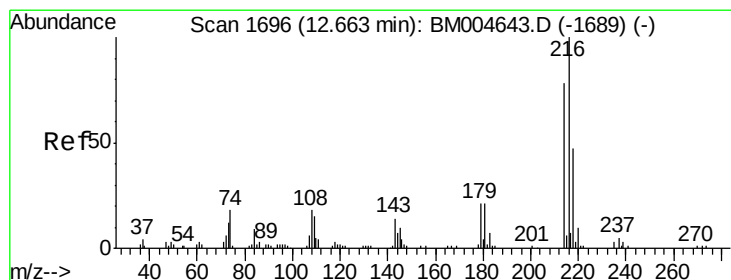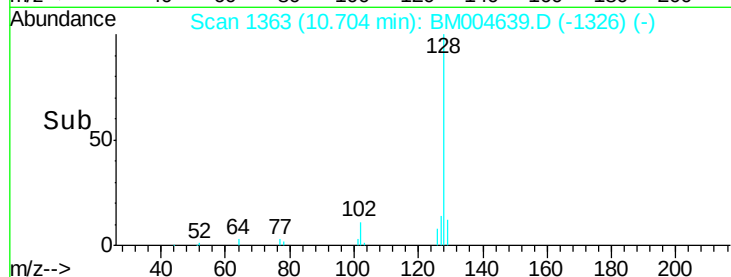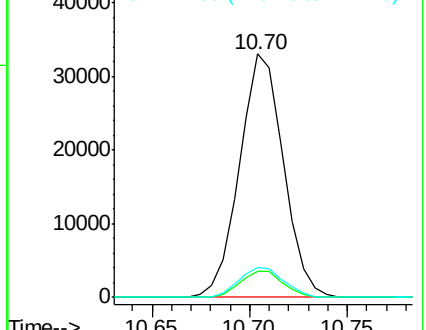

#37

1,2,4,5-Tetrachlorobenzene

Concen: 37.74 ng/ul

RT: 12.66 min Scan# 1696

Delta R.T. 0.00 min

Lab File: BM004639.D

Acq: 16 Mar 2016 16:52

Tgt Ion:216 Resp: 165947


Ion Ratio Lower Upper

216 100

214 79.7 62.5 93.7

179 21.5 18.2 27.2

108 18.4 14.2 21.2


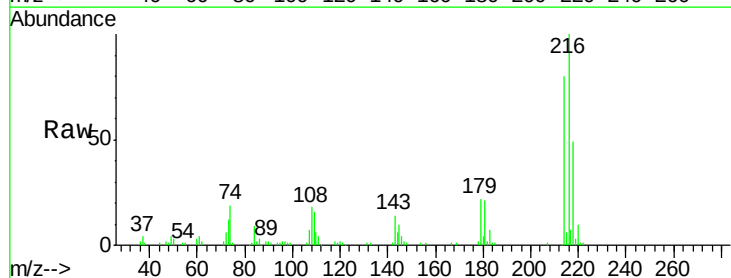



Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 108.00 (107.70 to 108.70): E

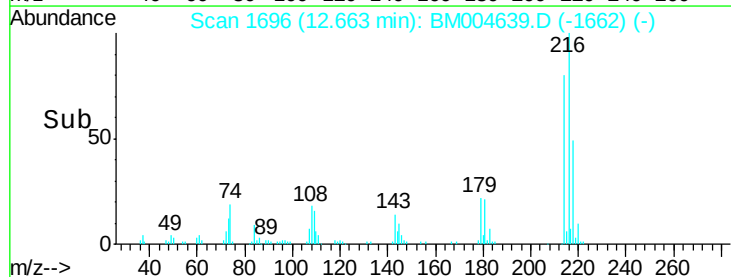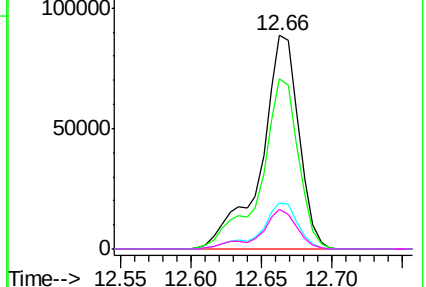


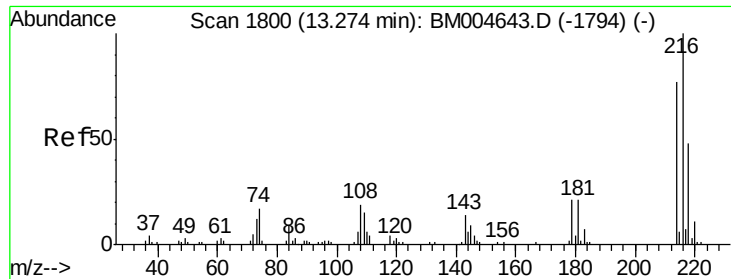




#73  
 1,2,3,4-Tetrachlorobenzene  
 Concen: 115.28 ng/uL  
 RT: 13.27 min Scan# 1800  
 Delta R.T. 0.00 min  
 Lab File: BM004639.D  
 Acq: 16 Mar 2016 16:52

Instrument :  
 BNA\_M  
 ClientSampleId :  
 C0AA6

Tgt Ion:216 Resp: 476093  
 Ion Ratio Lower Upper  
 216 100  
 214 78.7 62.5 93.7  
 218 47.9 38.4 57.6

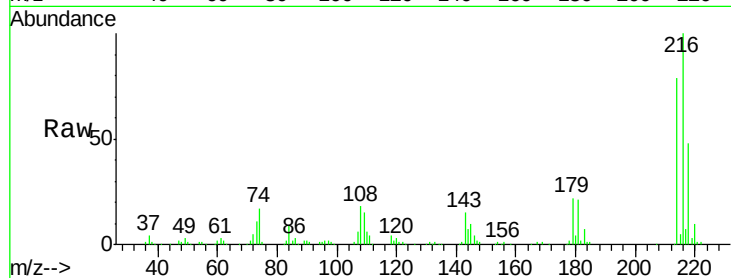


Abundance Ion 216.00 (215.70 to 216.70): E  
 Ion 214.00 (213.70 to 214.70): E  
 Ion 218.00 (217.70 to 218.70): E

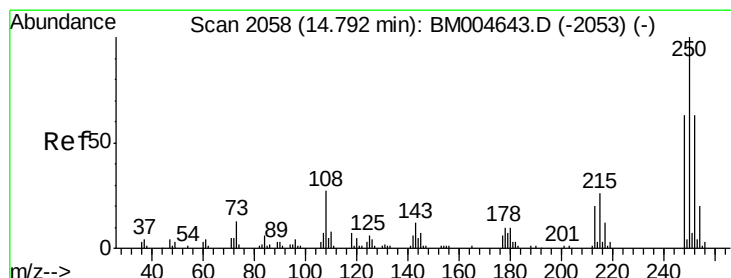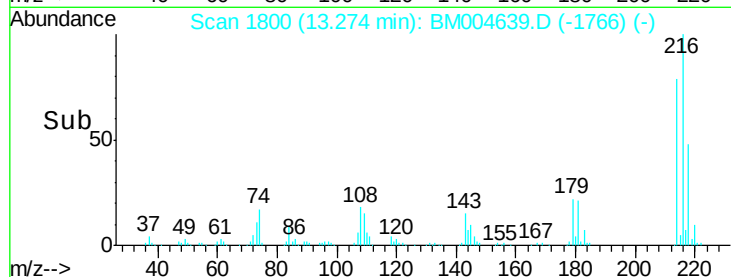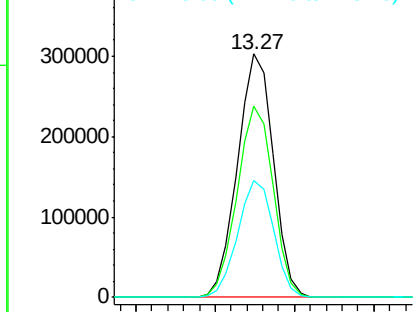

#74  
 Pentachlorobenzene  
 Concen: 2.17 ng/uL  
 RT: 14.79 min Scan# 2058  
 Delta R.T. 0.00 min  
 Lab File: BM004639.D  
 Acq: 16 Mar 2016 16:52

Tgt Ion:250 Resp: 8661  
 Ion Ratio Lower Upper  
 250 100  
 248 56.0 50.6 75.8  
 252 57.5 51.4 77.0

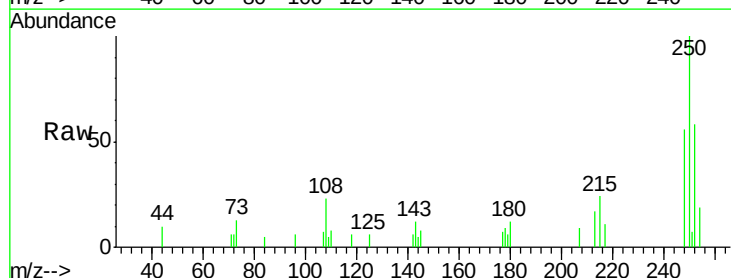

Abundance Ion 250.00 (249.70 to 250.70): E  
 Ion 248.00 (247.70 to 248.70): E  
 Ion 252.00 (251.70 to 252.70): E

