

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031618\
 Data File : BM014624.D
 Acq On : 17 Mar 2018 02:21
 Operator : SJ/JU
 Sample : J1918-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BE8H8

Quant Time: Mar 17 04:49:43 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM031518-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 17 03:22:03 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.45	152	79256	20.00	ng/ul	0.00
2) Naphthalene-d8	10.22	136	324234	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.12	164	174294	20.00	ng/ul	0.00
12) Phenanthrene-d10	16.89	188	349174	20.00	ng/ul	0.00
18) Chrysene-d12	21.11	240	278516	20.00	ng/ul	0.00
23) Perylene-d12	23.27	264	266927	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	9.89	165	60543	12.08	ng/ul	0.01
7) Acenaphthylene-d8	13.81	160	313659	16.84	ng/ul	0.00
10) Fluorene-d10	15.13	176	204107	16.73	ng/ul	0.00
15) Anthracene-d10	16.99	188	277565	16.60	ng/ul	0.00
19) Pyrene-d10	19.30	212	275925	16.48	ng/ul	0.00
26) Benzo(a)pyrene-d12	23.14	264	220889	17.11	ng/ul	0.00
Target Compounds				Qvalue		
25) Benzo(k)fluoranthene	22.64	252	18657	1.170	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031618\
Data File : BM014624.D
Acq On : 17 Mar 2018 02:21
Operator : SJ/JU
Sample : J1918-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE8H8

Quant Time: Mar 17 04:49:43 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM031518-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 17 03:22:03 2018
Response via : Initial Calibration

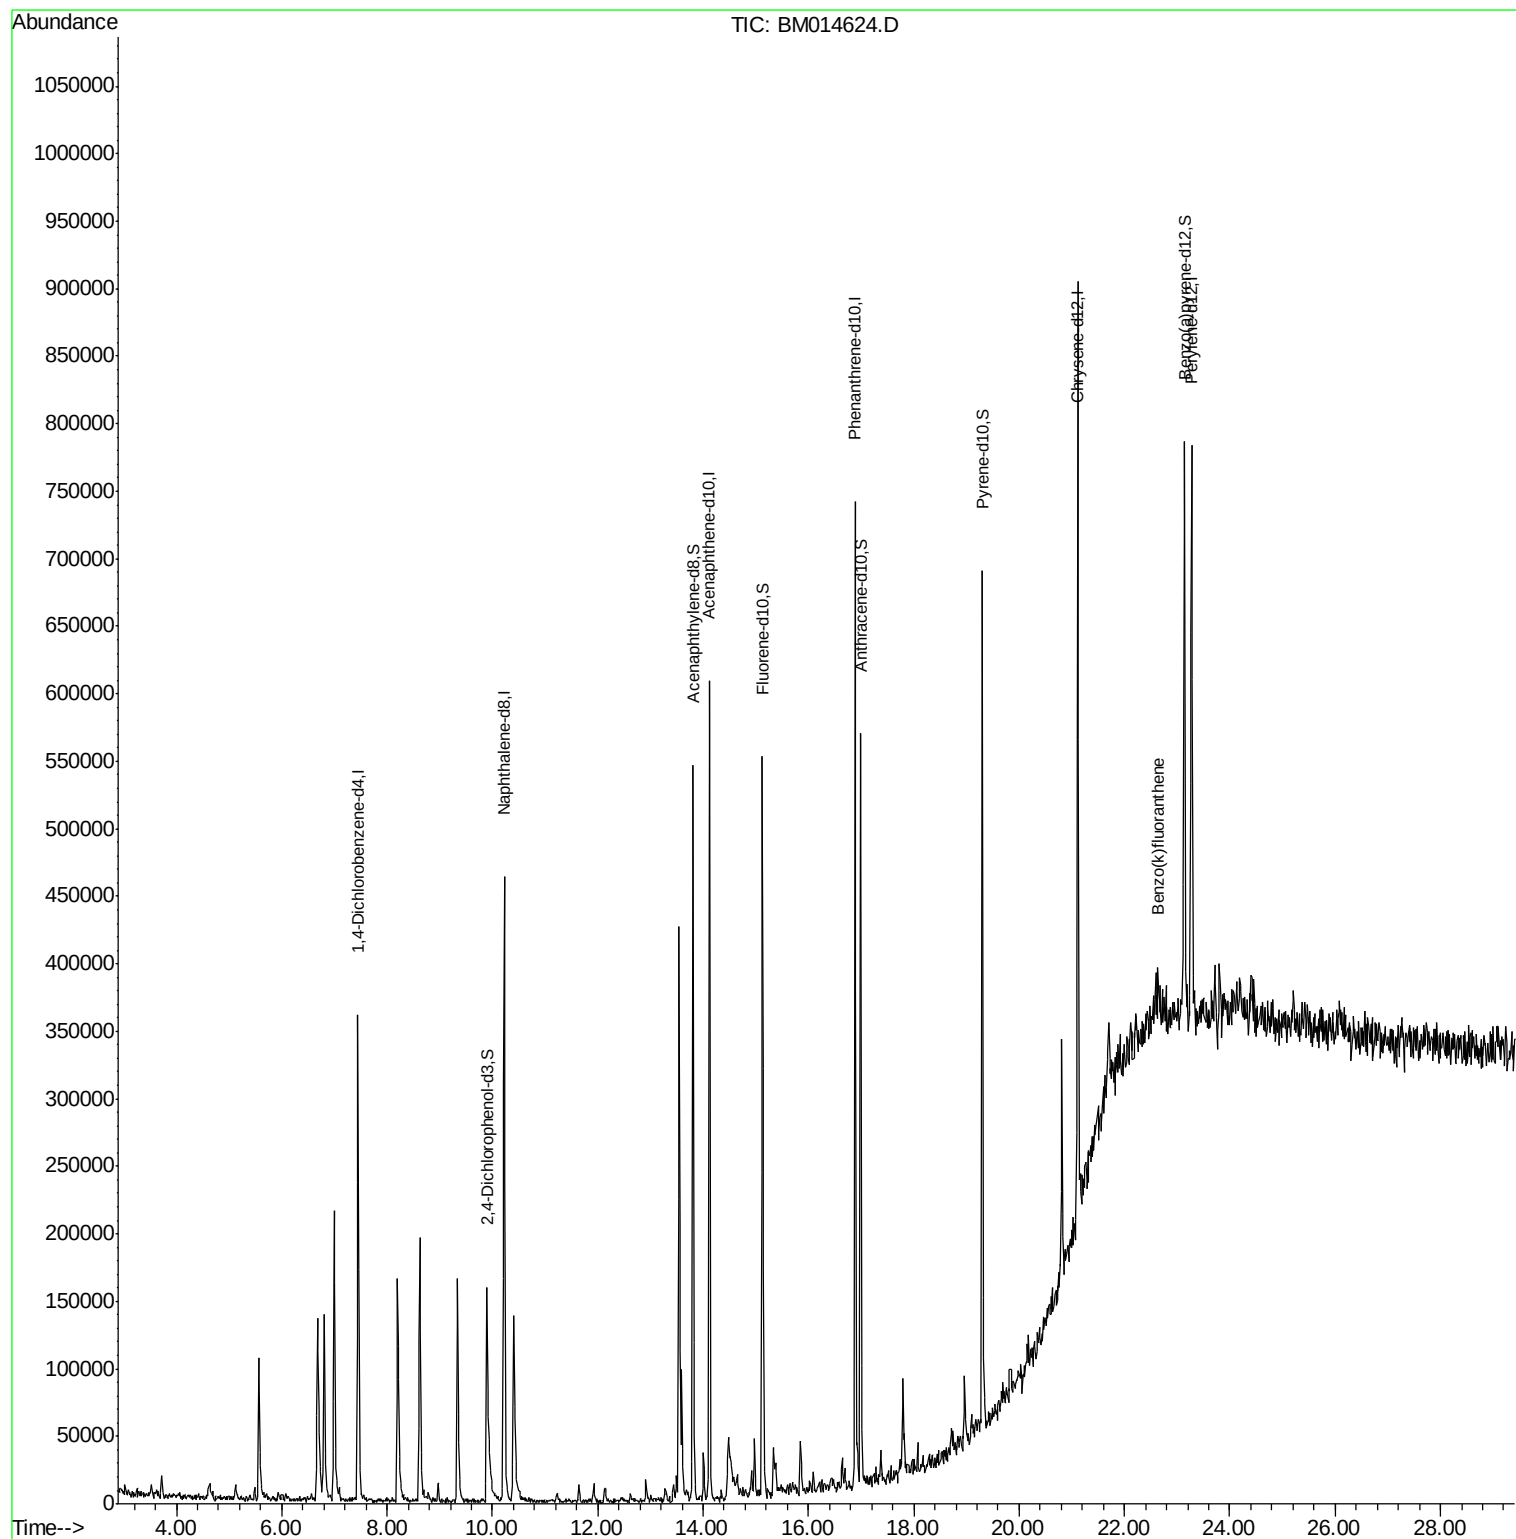

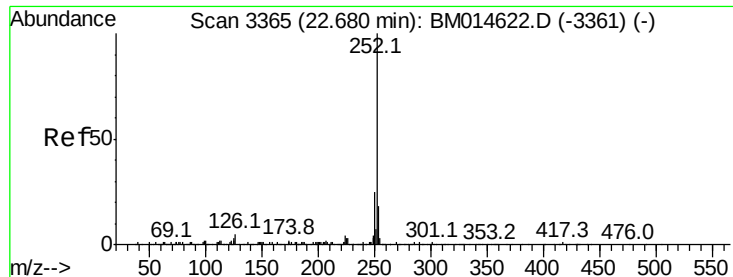

#25

Benzo(k)fluoranthene

Concen: 1.170 ng/ul

RT: 22.64 min Scan# 3359

Delta R.T. -0.04 min

Lab File: BM014624.D

Acq: 17 Mar 2018 02:21

Instrument :

BNA_M

ClientSampleId :

BE8H8

Tot Ion:252 Resp: 18657

Ion Ratio Lower Upper

252 100

253 36.2 17.1 25.7#

125 18.3 3.4 5.2#

