

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031623\
 Data File : BM039016.D
 Acq On : 16 Mar 2023 13:14
 Operator : CG/JU
 Sample : PB151350BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB151350BL

Quant Time: Mar 17 06:31:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 17 05:25:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	344513	20.000	ng	0.00
21) Naphthalene-d8	10.792	136	1423189	20.000	ng	0.00
39) Acenaphthene-d10	14.616	164	849791	20.000	ng	0.00
64) Phenanthrene-d10	17.357	188	1692918	20.000	ng	0.00
76) Chrysene-d12	21.539	240	1177748	20.000	ng	0.00
86) Perylene-d12	23.980	264	1131177	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.528	112	3731315	164.550	ng	0.00
7) Phenol-d6	7.140	99	4809665	163.295	ng	0.00
23) Nitrobenzene-d5	9.145	82	2822655	97.423	ng	0.00
42) 2,4,6-Tribromophenol	16.104	330	1432824	145.749	ng	0.00
45) 2-Fluorobiphenyl	13.245	172	5934408	90.909	ng	0.00
79) Terphenyl-d14	19.986	244	7505274	116.512	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031623\
Data File : BM039016.D
Acq On : 16 Mar 2023 13:14
Operator : CG/JU
Sample : PB151350BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151350BL

Quant Time: Mar 17 06:31:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 17 05:25:34 2023
Response via : Initial Calibration




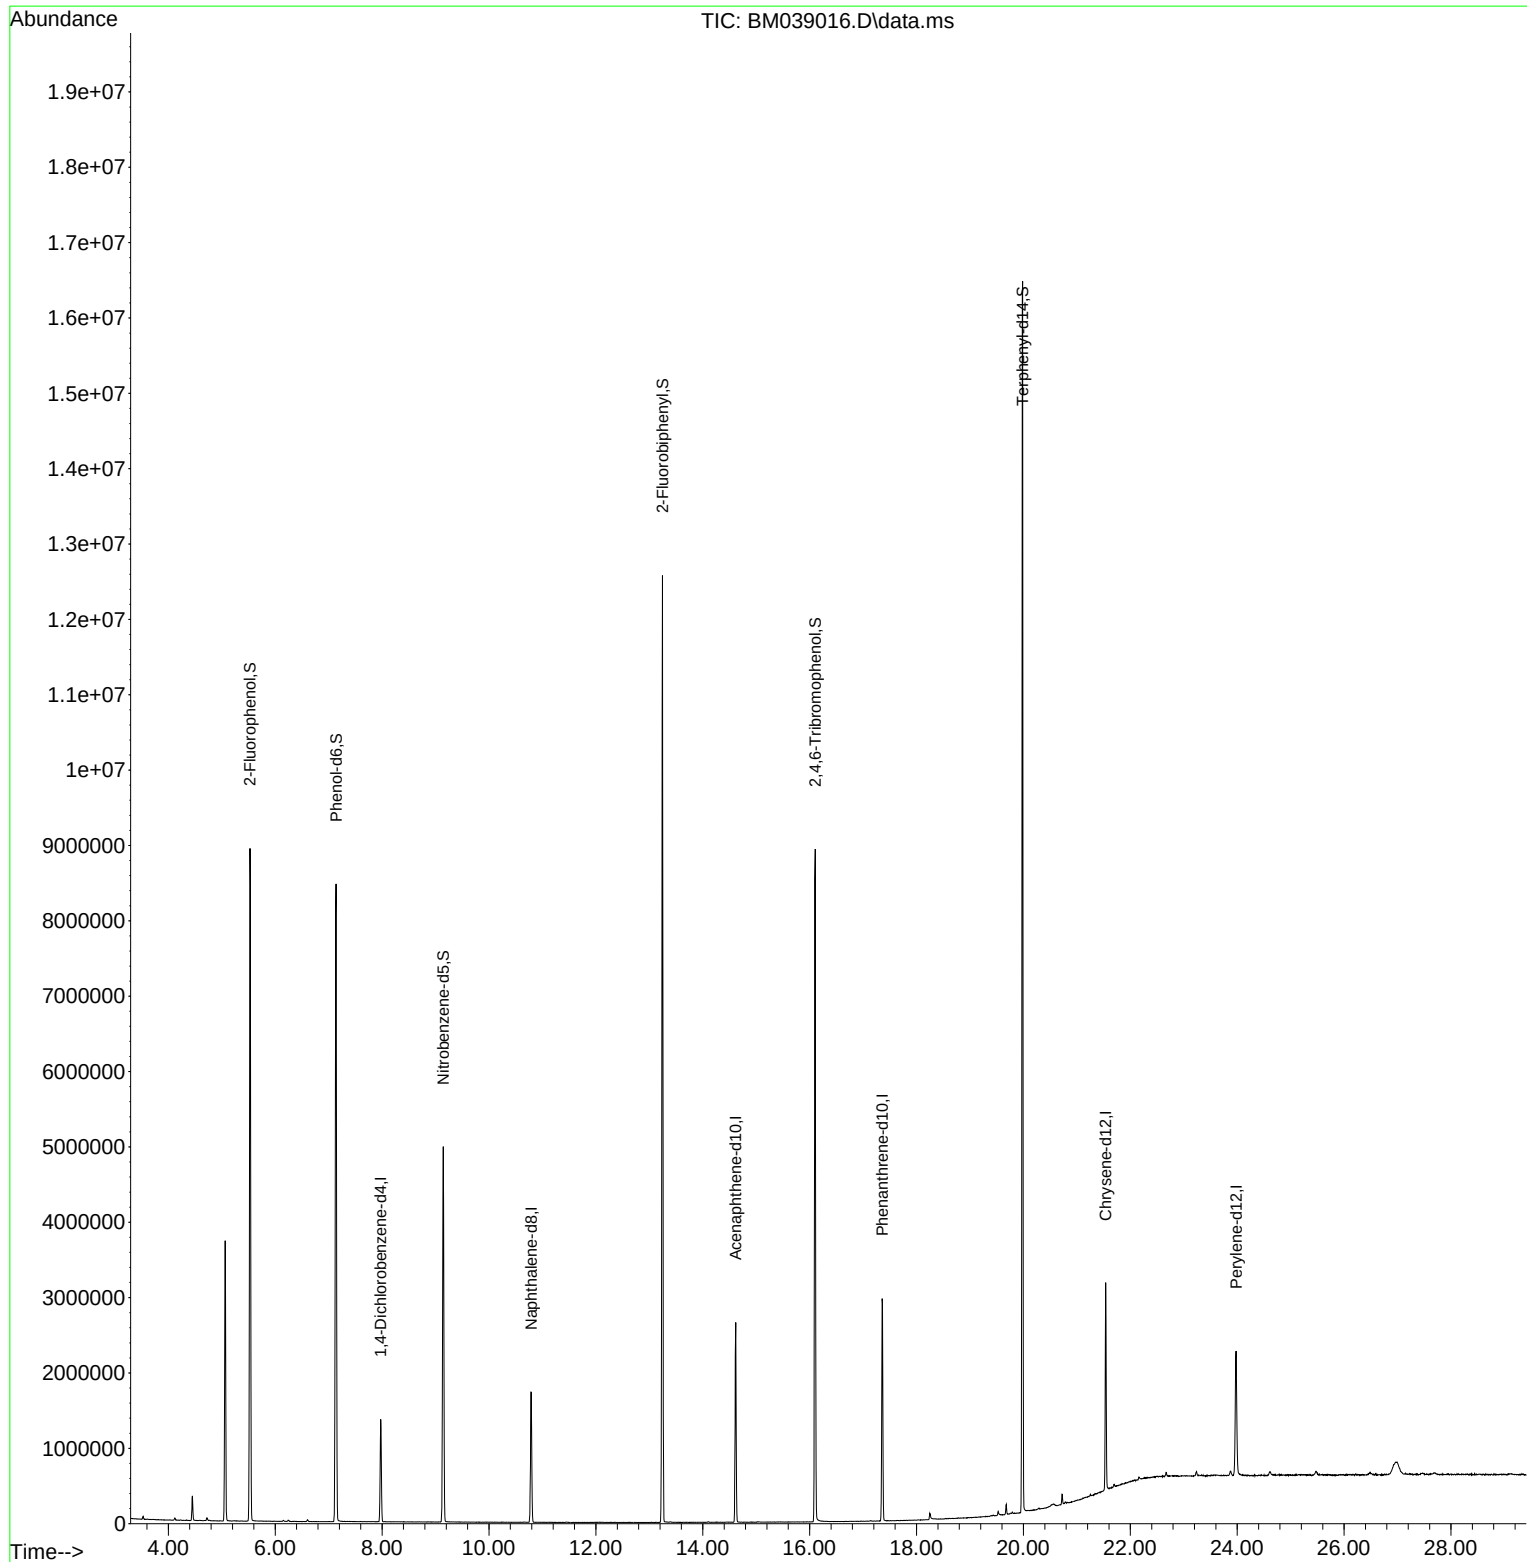


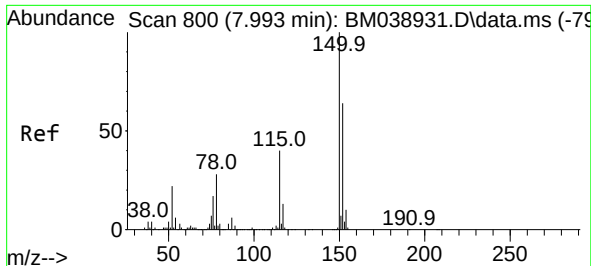

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.975 min Scan# 799
Delta R.T. -0.000 min
Lab File: BM039016.D
Acq: 16 Mar 2023 13:14




Instrument :
BNA_M
ClientSampleId :
PB151350BL


Tgt Ion:152 Resp: 344513
Ion Ratio Lower Upper
152 100
150 157.9 125.1 187.7
115 63.0 49.6 74.4

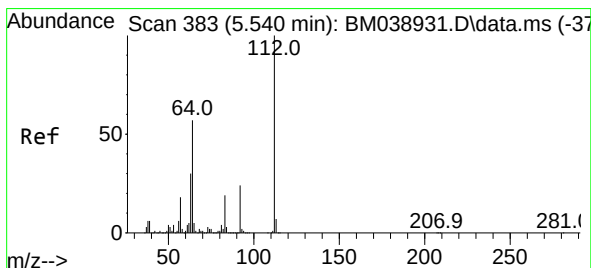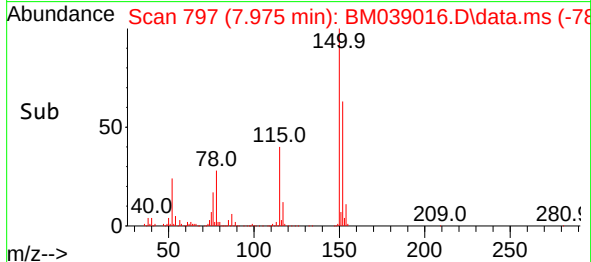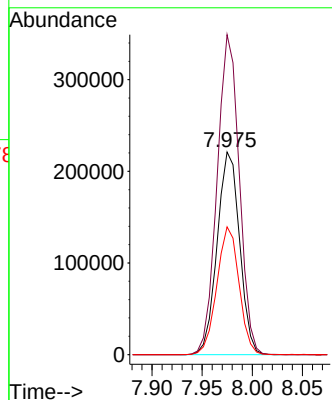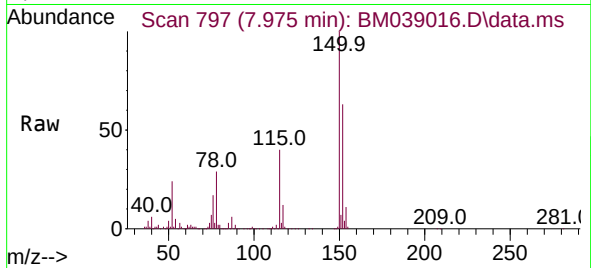

#5
2-Fluorophenol
Concen: 164.550 ng
RT: 5.528 min Scan# 381
Delta R.T. 0.000 min
Lab File: BM039016.D
Acq: 16 Mar 2023 13:14

Tgt Ion:112 Resp: 3731315
Ion Ratio Lower Upper
112 100
64 59.2 45.9 68.9
63 30.5 23.8 35.8


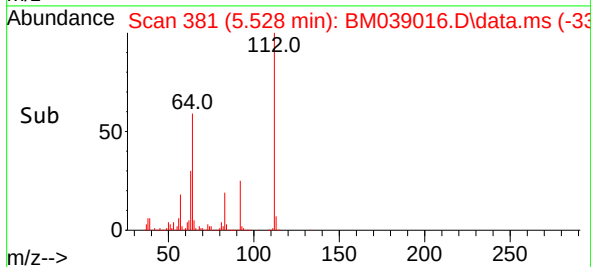
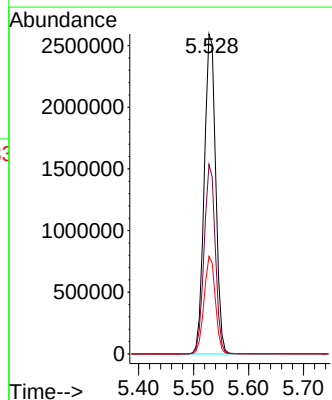
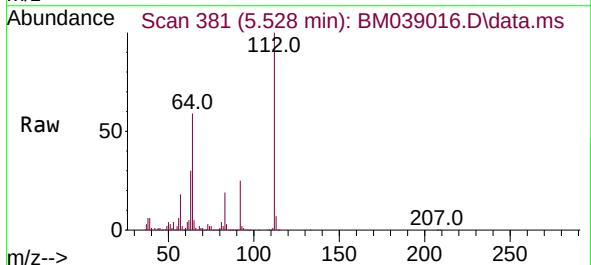


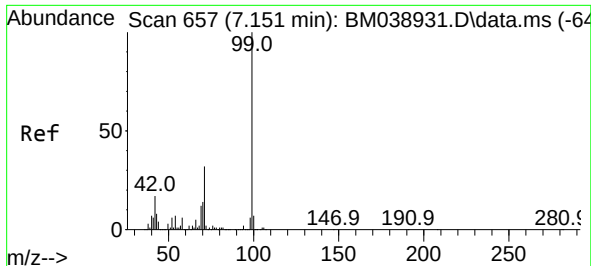

#7
Phenol-d6
Concen: 163.295 ng
RT: 7.140 min Scan# 61
Delta R.T. 0.006 min
Lab File: BM039016.D
Acq: 16 Mar 2023 13:14




Instrument :
BNA_M
ClientSampleId :
PB151350BL


Tgt Ion: 99 Resp: 4809665
Ion Ratio Lower Upper
99 100
42 17.2 13.5 20.3
71 32.5 25.6 38.4

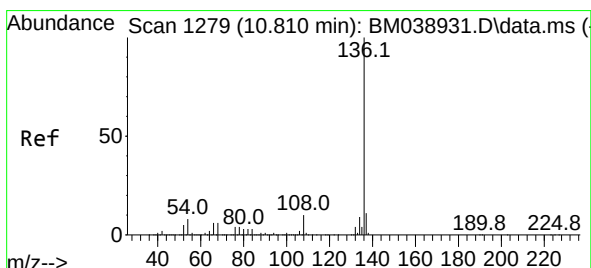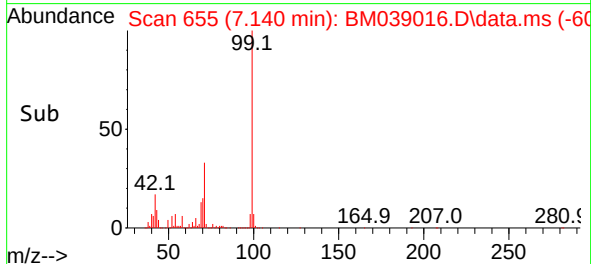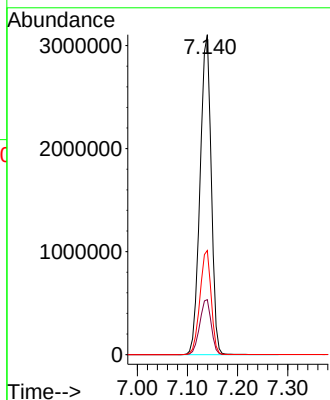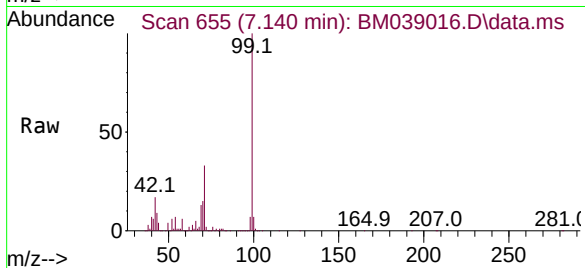

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.792 min Scan# 1276
Delta R.T. 0.000 min
Lab File: BM039016.D
Acq: 16 Mar 2023 13:14

Tgt Ion: 136 Resp: 1423189
Ion Ratio Lower Upper
136 100
137 10.8 8.7 13.1
54 8.3 6.3 9.5
68 6.4 5.0 7.6


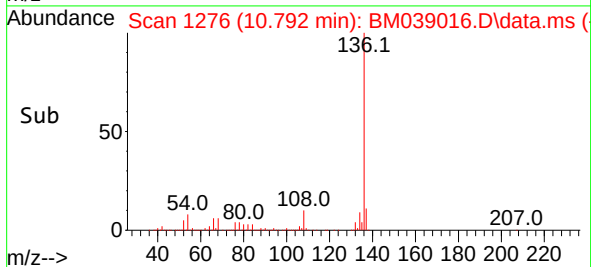
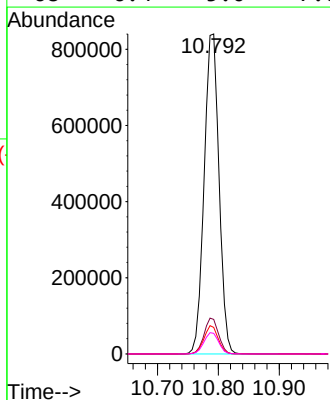
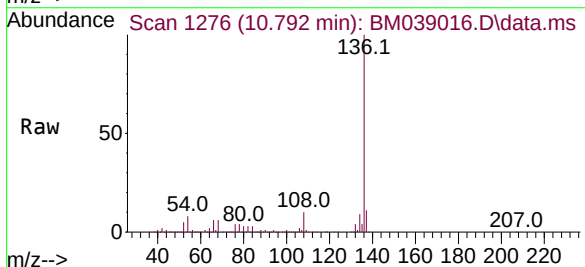


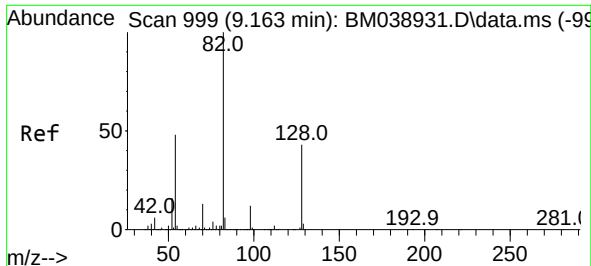

#23
Nitrobenzene-d5
Concen: 97.423 ng
RT: 9.145 min Scan# 999
Delta R.T. 0.000 min
Lab File: BM039016.D
Acq: 16 Mar 2023 13:14




Instrument :
BNA_M
ClientSampleId :
PB151350BL


Tgt Ion: 82 Resp: 2822655
Ion Ratio Lower Upper
82 100
128 42.9 34.4 51.6
54 48.9 38.8 58.2

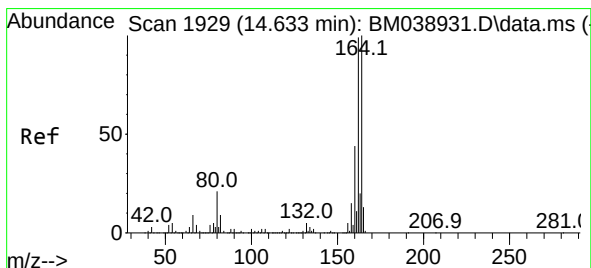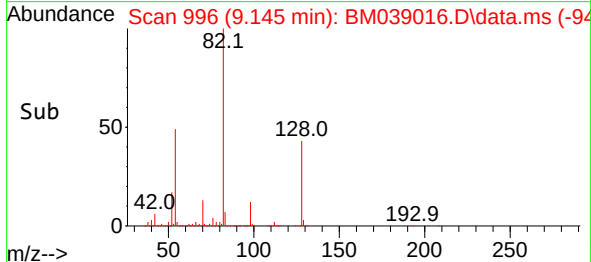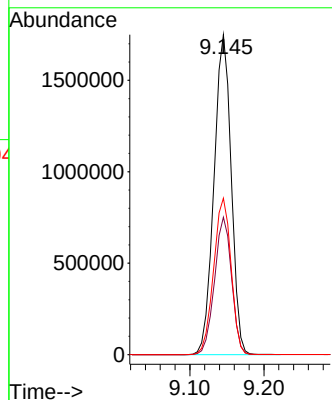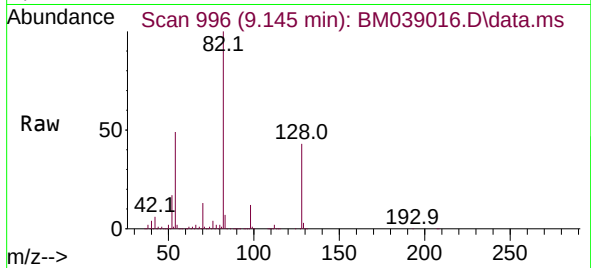

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.616 min Scan# 1926
Delta R.T. 0.000 min
Lab File: BM039016.D
Acq: 16 Mar 2023 13:14

Tgt Ion: 164 Resp: 849791
Ion Ratio Lower Upper
164 100
162 98.6 79.2 118.8
160 44.8 35.5 53.3


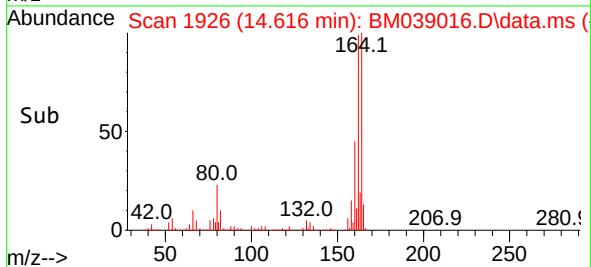
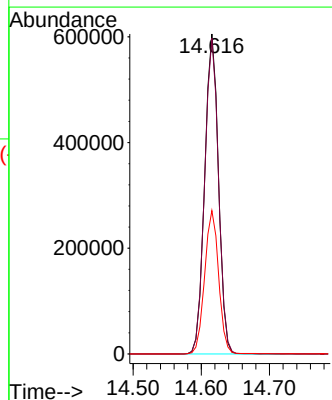
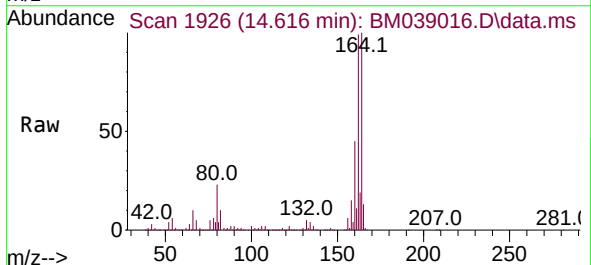


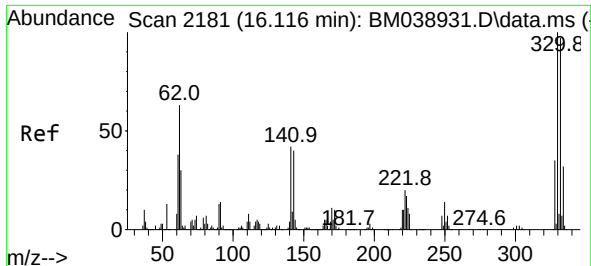

#42
2,4,6-Tribromophenol
Concen: 145.749 ng
RT: 16.104 min Scan# 2181
Delta R.T. 0.000 min
Lab File: BM039016.D
Acq: 16 Mar 2023 13:14




Instrument :
BNA_M
ClientSampleId :
PB151350BL


Tgt Ion:330 Resp: 1432824
Ion Ratio Lower Upper
330 100
332 96.0 77.4 116.0
141 40.9 32.2 48.4

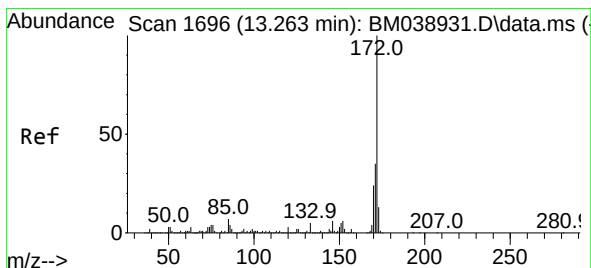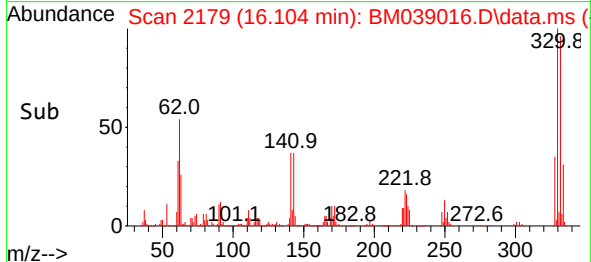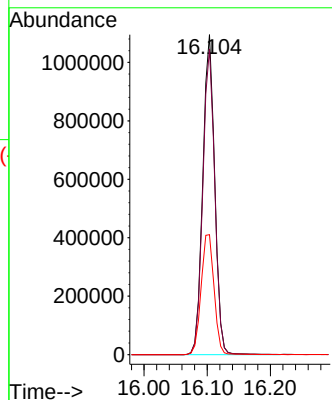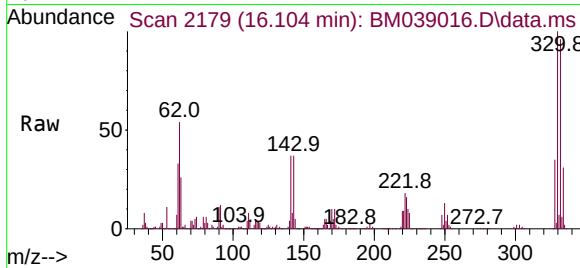

#45
2-Fluorobiphenyl
Concen: 90.909 ng
RT: 13.245 min Scan# 1693
Delta R.T. 0.000 min
Lab File: BM039016.D
Acq: 16 Mar 2023 13:14

Tgt Ion:172 Resp: 5934408
Ion Ratio Lower Upper
172 100
171 35.4 28.2 42.2
170 24.2 19.1 28.7


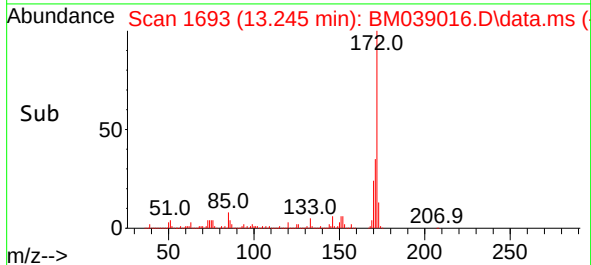
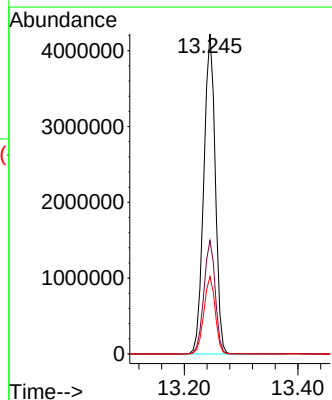
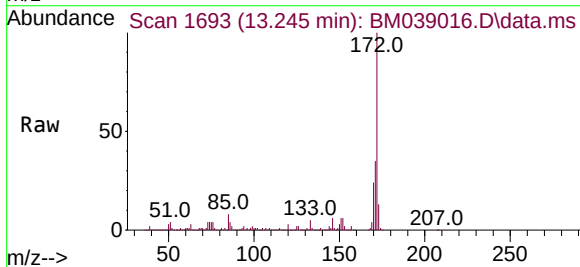


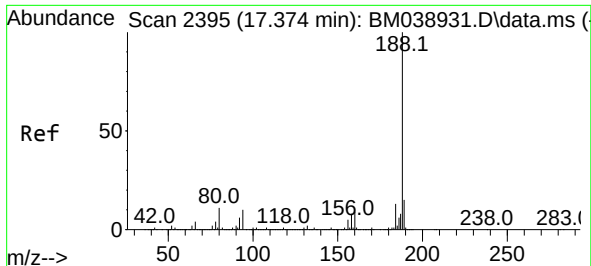

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.357 min Scan# 2392
Delta R.T. -0.006 min
Lab File: BM039016.D
Acq: 16 Mar 2023 13:14




Instrument :
BNA_M
ClientSampleId :
PB151350BL


Tgt Ion:188 Resp: 1692918
Ion Ratio Lower Upper
188 100
94 10.7 7.9 11.9
80 11.9 8.5 12.7

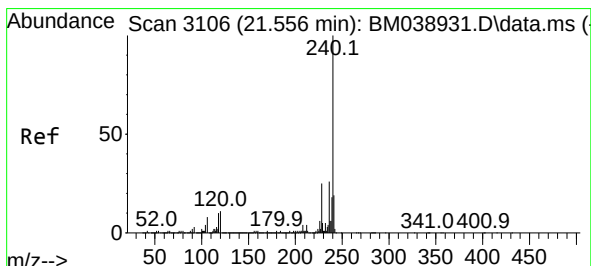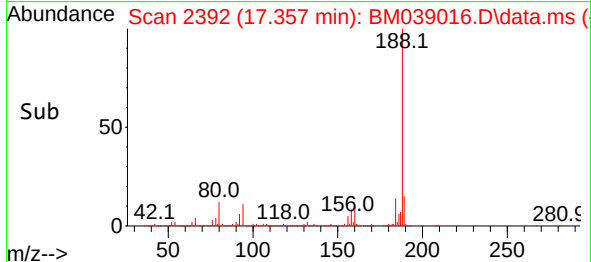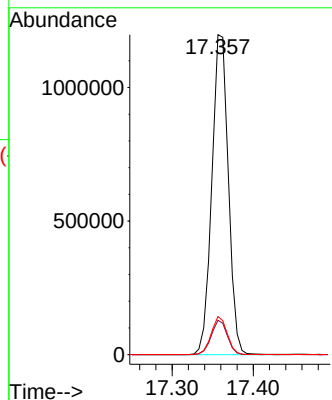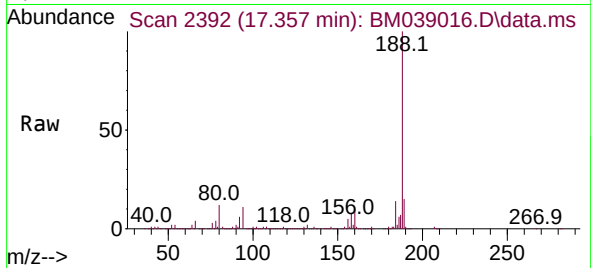

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.539 min Scan# 3103
Delta R.T. 0.000 min
Lab File: BM039016.D
Acq: 16 Mar 2023 13:14

Tgt Ion:240 Resp: 1177748
Ion Ratio Lower Upper
240 100
120 12.8 9.2 13.8
236 26.0 20.8 31.2


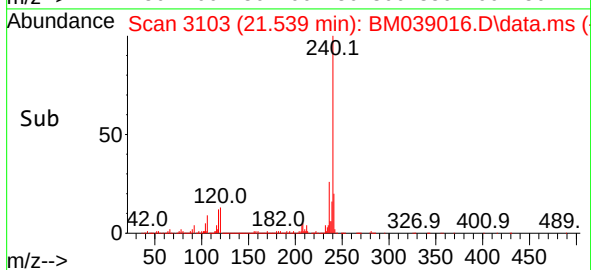
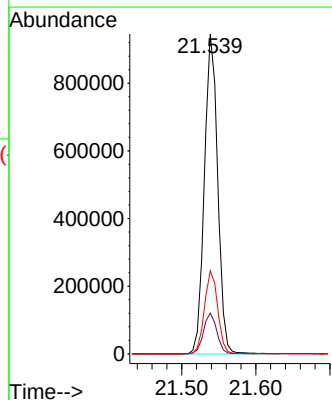
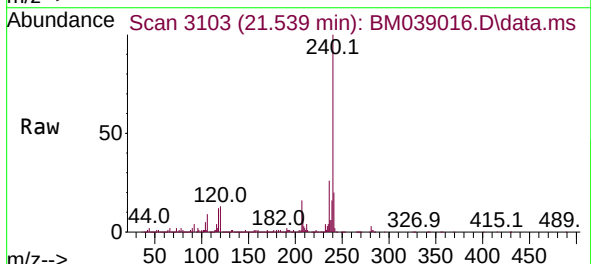


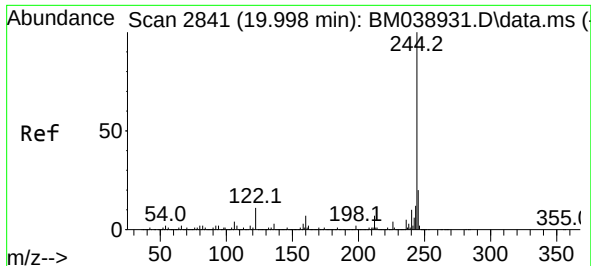

#79
 Terphenyl-d14
 Concen: 116.512 ng
 RT: 19.986 min Scan# 2841
 Delta R.T. 0.006 min
 Lab File: BM039016.D
 Acq: 16 Mar 2023 13:14

Instrument :
 BNA_M
 ClientSampleId :
 PB151350BL

Tgt Ion:244 Resp: 7505274
 Ion Ratio Lower Upper
 244 100
 212 7.2 5.5 8.3
 122 12.2 9.0 13.4

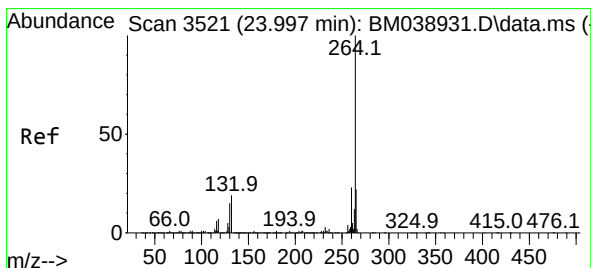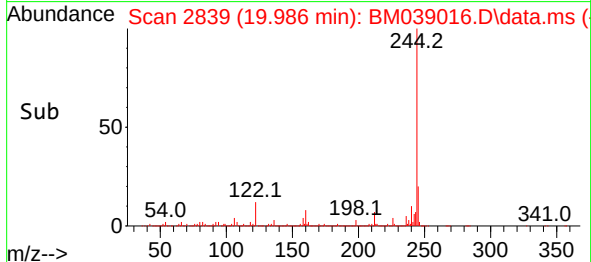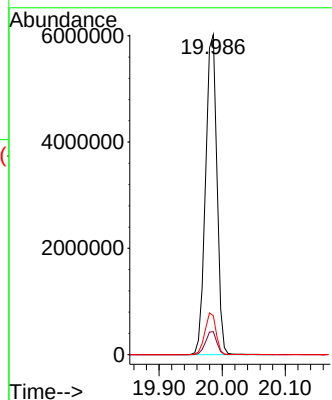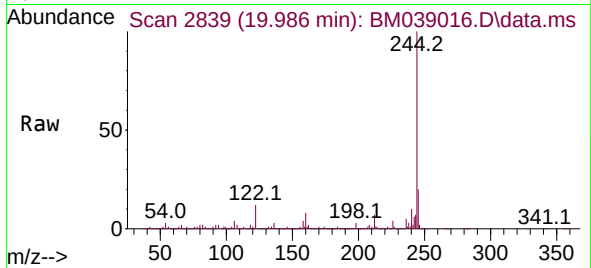

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.980 min Scan# 3518
 Delta R.T. 0.000 min
 Lab File: BM039016.D
 Acq: 16 Mar 2023 13:14

Tgt Ion:264 Resp: 1131177
 Ion Ratio Lower Upper
 264 100
 260 23.8 18.7 28.1
 265 21.8 17.9 26.9

