
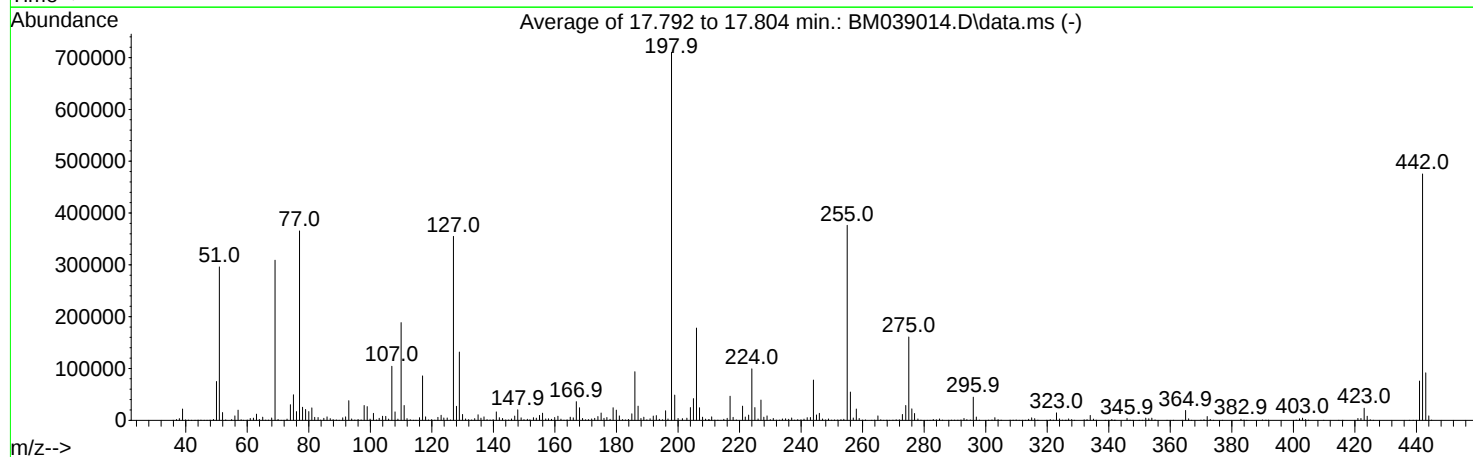


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031623\
 Data File : BM039014.D
 Acq On : 16 Mar 2023 11:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 17 05:25:34 2023

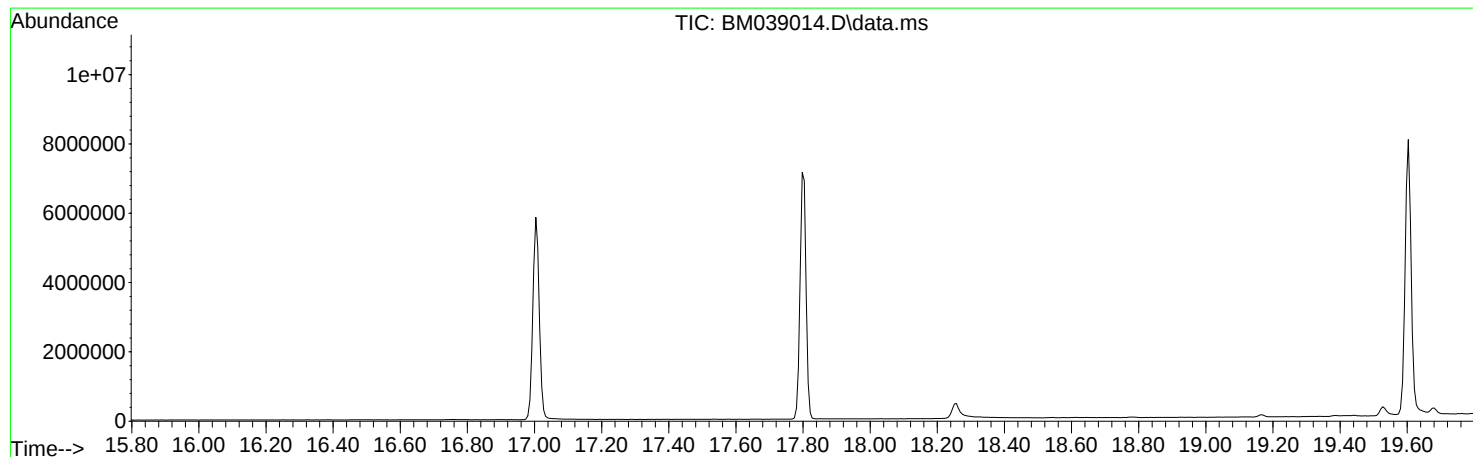




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	296099	PASS
68	69	0.00	2	1.5	4642	PASS
69	198	0.00	100	43.5	308931	PASS
70	69	0.00	2	0.5	1680	PASS
127	198	10	80	50.0	355029	PASS
197	198	0.00	2	0.4	2698	PASS
198	198	100	100	100.0	709952	PASS
199	198	5	9	6.9	48693	PASS
275	198	10	60	22.6	160771	PASS
365	198	1	100	2.7	18855	PASS
441	198	0.01	100	10.7	75736	PASS
442	442	50	100	100.0	475499	PASS
443	442	15	24	19.3	91659	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031623\
Data File : BM039014.D
Acq On : 16 Mar 2023 11:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 17 07:52:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 17 05:25:34 2023
Response via : Initial Calibration

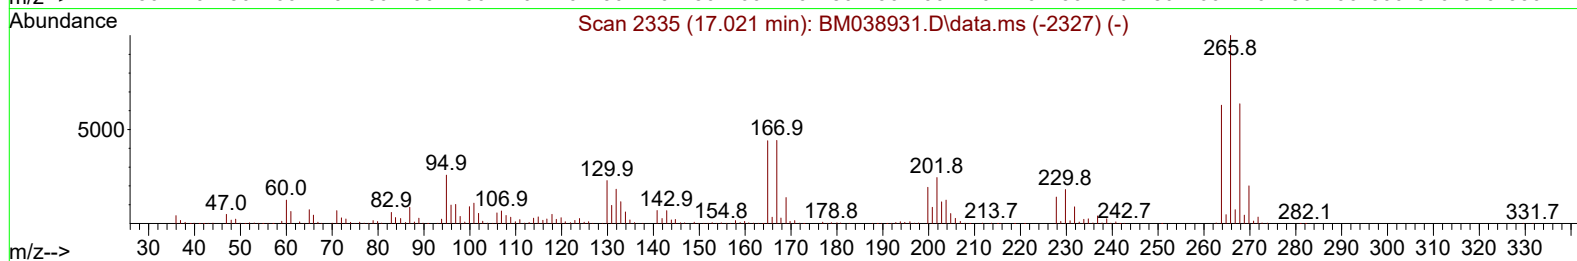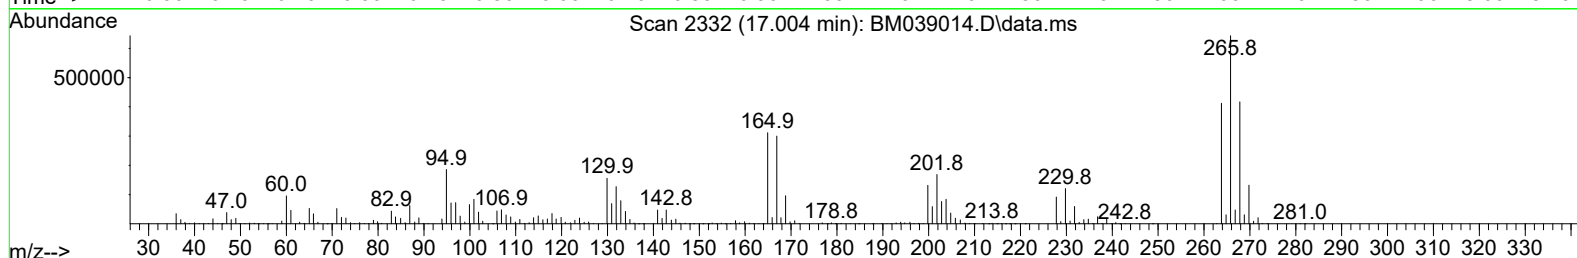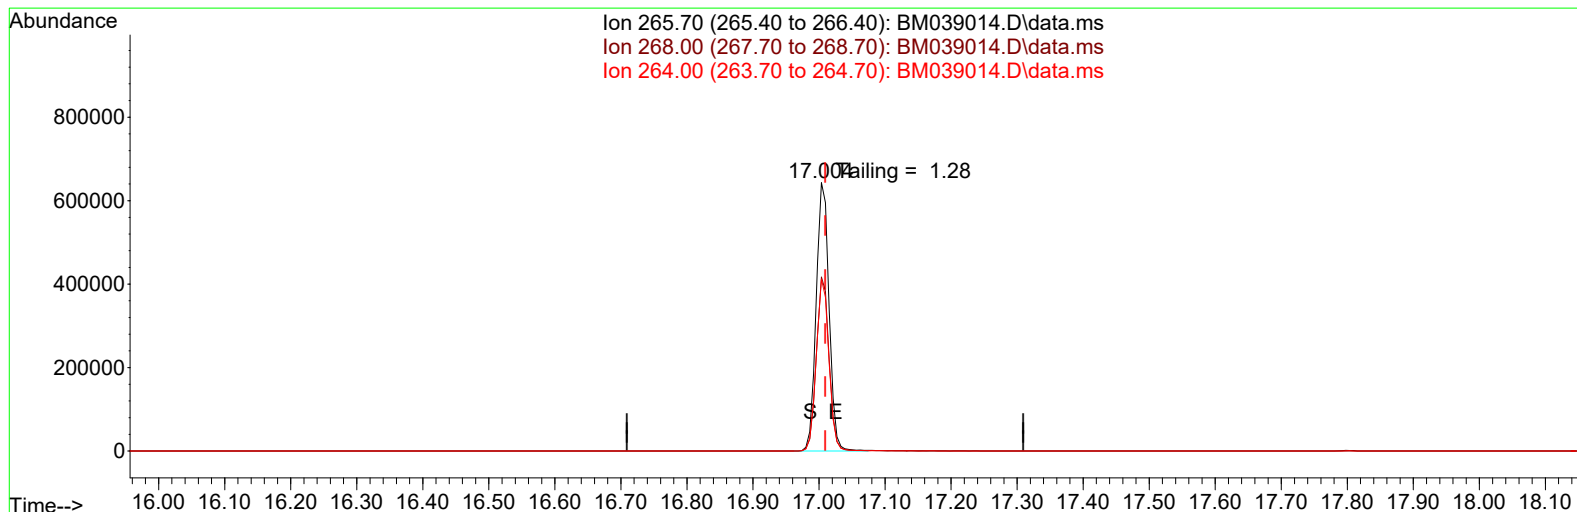

TIC: BM039014.D\data.ms

(70) Pentachlorophenol (C)

17.004min (-0.006) 0.00 ng




response 872429

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.87
264.00	62.90	64.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031623\
 Data File : BM039014.D
 Acq On : 16 Mar 2023 11:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 17 07:52:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 17 05:25:34 2023
 Response via : Initial Calibration

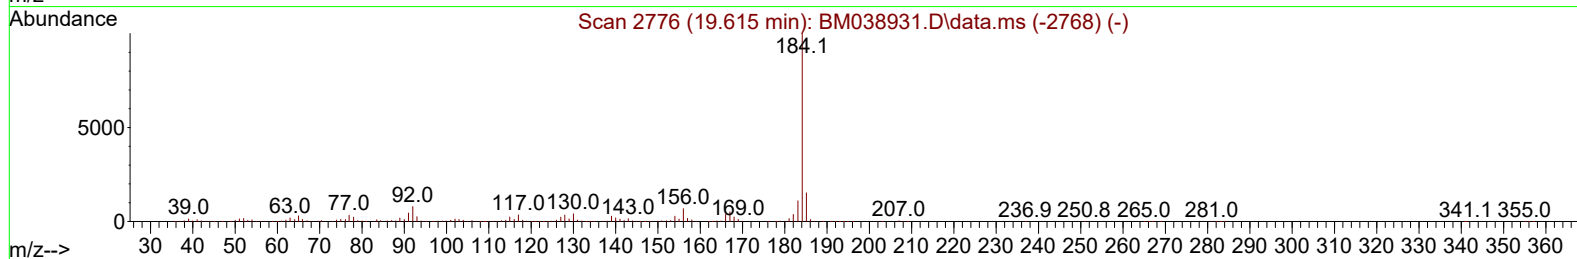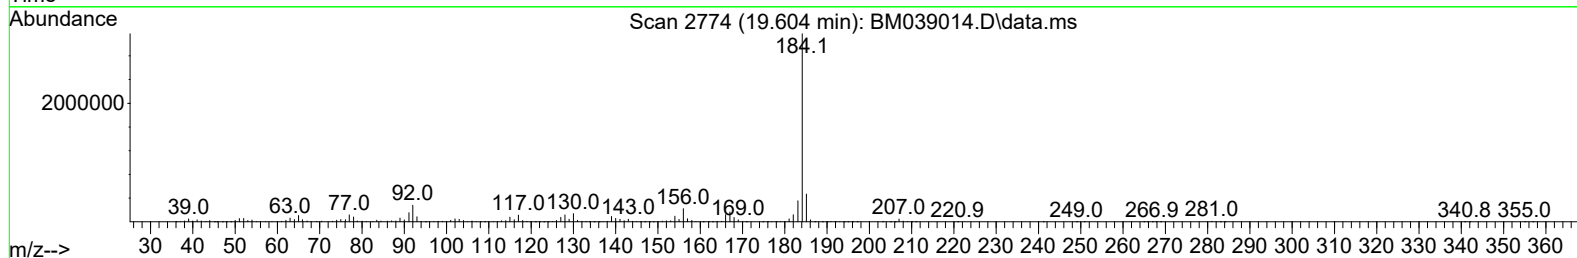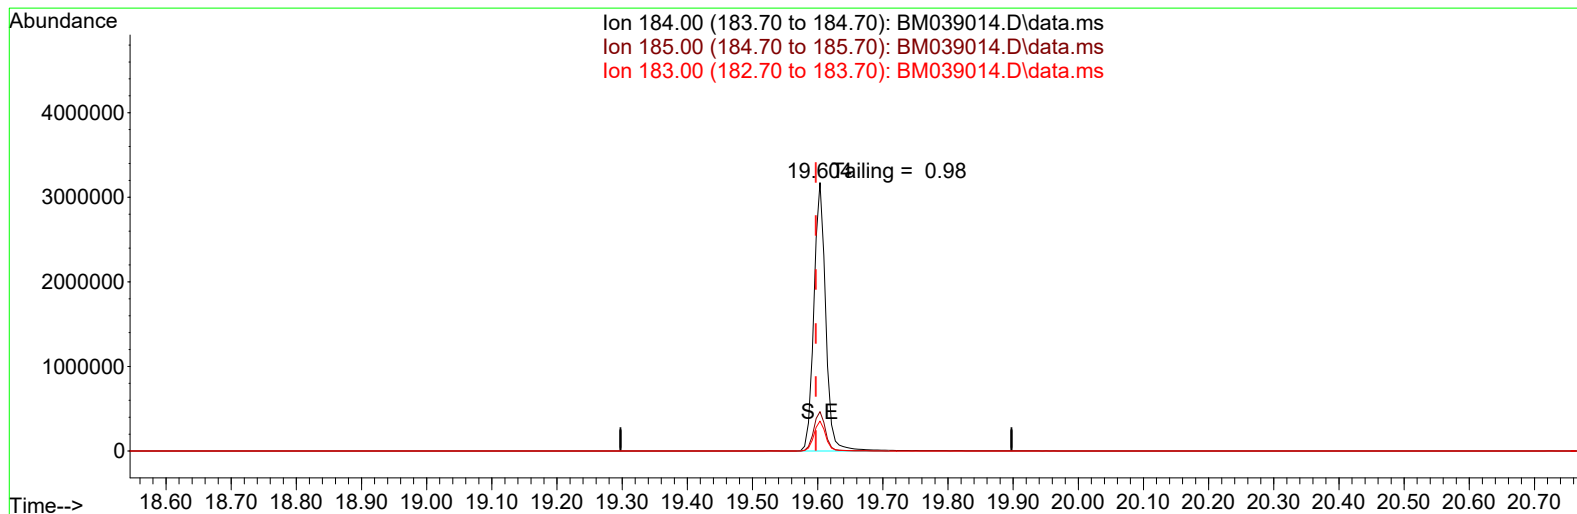

TIC: BM039014.D\data.ms

(77) Benzidine**19.604min (+ 0.006) 185421.89 ng****response 4026936**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.70
183.00	11.00	11.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/16/2023	BNA_M	<u>BM039014.D</u>
Compound Name	Response	Retention Time
DDT	2277481	20.839
DDD	21047	20.451
DDE	562	19.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21609	2299090	0.94

Instrument :
BNA_M
ClientSampleId :
DFTPP