

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
 Data File : BM044650.D
 Acq On : 16 Mar 2024 01:30
 Operator : MA/JU
 Sample : P1779-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AJ6

Quant Time: Mar 16 02:19:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 15 11:12:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.698	152	160865	20.000	ng/u1	0.00
20) Naphthalene-d8	10.475	136	653851	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.339	164	390121	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.098	188	788434	20.000	ng/u1	0.00
79) Chrysene-d12	21.291	240	747165	20.000	ng/u1	0.00
88) Perylene-d12	23.538	264	836194	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.257	96	25732	5.425	ng/uL	0.00
4) Pyridine-d5	3.657	84	131184	9.397	ng/u1	0.00
7) Phenol-d5	6.869	99	110026	6.653	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.045	67	389967	38.173	ng/u1	0.00
11) 2-Chlorophenol-d4	7.228	132	342321	28.166	ng/u1	0.00
15) 4-Methylphenol-d8	8.398	113	207018	15.938	ng/u1	0.00
21) Nitrobenzene-d5	8.857	128	226469	41.132	ng/u1	0.00
24) 2-Nitrophenol-d4	9.569	143	228298	38.463	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.098	165	355779	35.220	ng/u1	0.00
31) 4-Chloroaniline-d4	10.622	131	510531	30.430	ng/u1	0.00
46) Dimethylphthalate-d6	13.763	166	1263042	41.272	ng/u1	0.00
49) Acenaphthylene-d8	14.033	160	1435603	41.019	ng/u1	0.00
54) 4-Nitrophenol-d4	14.563	143	34607	5.453	ng/u1	0.00
60) Fluorene-d10	15.339	176	1128937	43.899	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.468	200	190345	37.192	ng/u1	0.00
73) Anthracene-d10	17.198	188	1800751	47.782	ng/u1	0.00
81) Pyrene-d10	19.497	212	2084782	45.493	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.397	264	2099559	47.770	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.293	88	5080	1.035	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044650.D
Acq On : 16 Mar 2024 01:30
Operator : MA/JU
Sample : P1779-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AJ6

Quant Time: Mar 16 02:19:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 15 11:12:49 2024
Response via : Initial Calibration

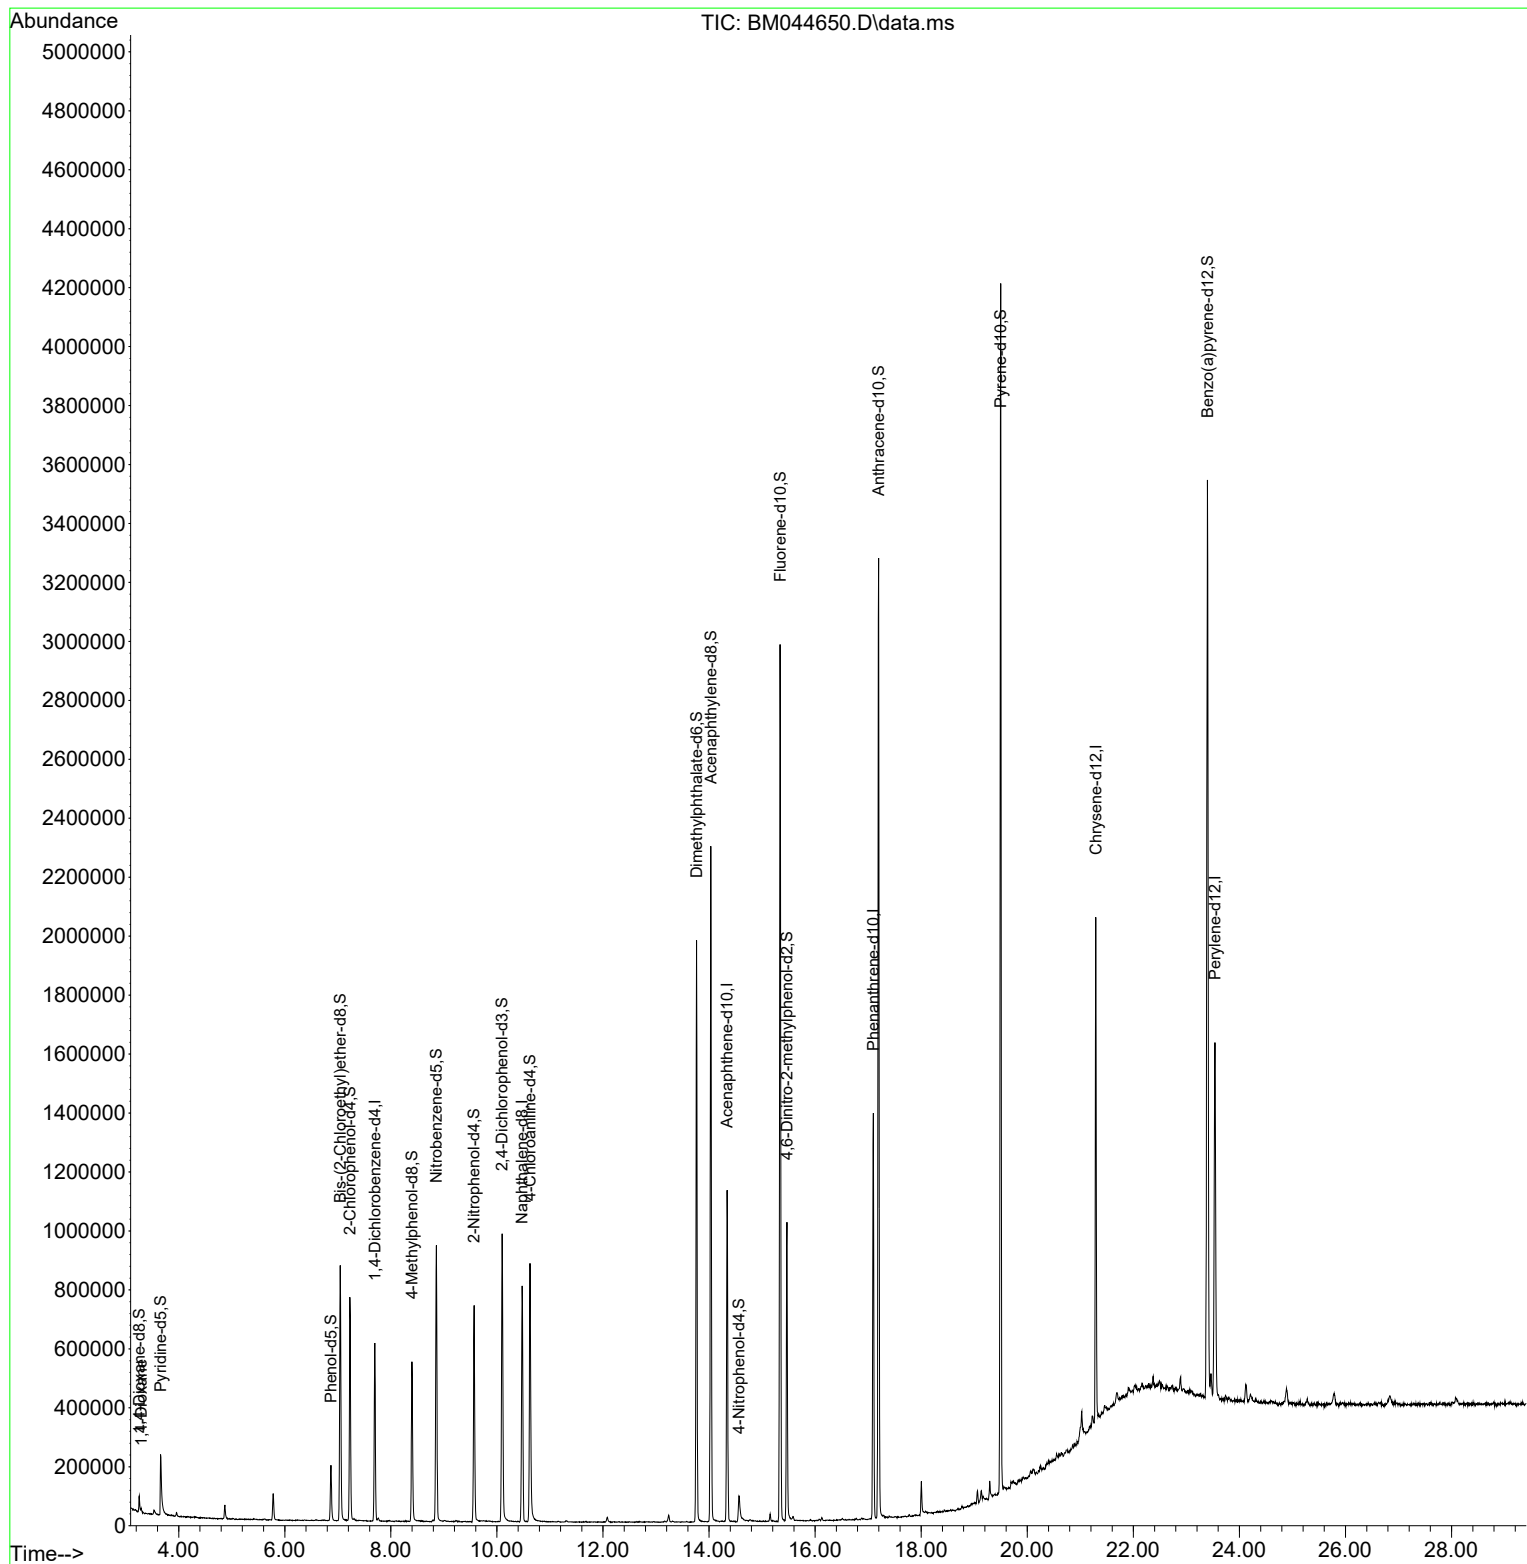

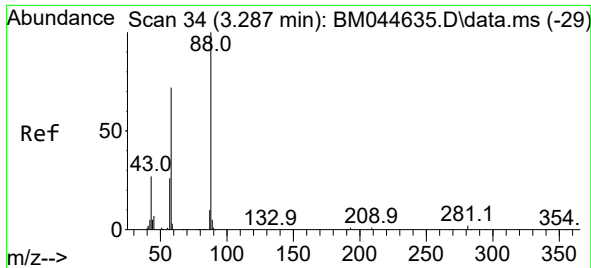

#2
 1,4-Dioxane
 Concen: 1.035 ng/uL
 RT: 3.293 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BM044650.D
 Acq: 16 Mar 2024 01:30

Instrument :
 BNA_M
 ClientSampleId :
 C0AJ6

Tgt Ion: 88 Resp: 5080
 Ion Ratio Lower Upper
 88 100
 43 34.3 23.8 35.6
 58 77.2 61.6 92.4

