

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
 Data File : BM044625.D
 Acq On : 15 Mar 2024 10:18
 Operator : MA/JU
 Sample : PB159597BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK597

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044625.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.257	25	29	36	rVB	66421	84055	1.93%	0.185%
2	3.651	93	96	119	rBV	736917	1188449	27.32%	2.620%
3	3.963	145	149	154	rVB2	12866	18251	0.42%	0.040%
4	6.869	636	643	654	rBV	819395	1355946	31.17%	2.989%
5	7.051	668	674	687	rVB	705380	1132443	26.03%	2.496%
6	7.234	698	705	713	rBV	849126	1345577	30.93%	2.966%
7	7.698	775	784	793	rBV	642204	1036791	23.83%	2.285%
8	8.404	896	904	922	rBV	960929	1589493	36.53%	3.504%
9	8.857	974	981	994	rBV	758356	1274115	29.29%	2.808%
10	9.575	1093	1103	1113	rBV	617874	1037447	23.85%	2.287%
11	10.104	1184	1193	1204	rBV	875576	1501666	34.52%	3.310%
12	10.480	1249	1257	1267	rVB	846917	1417335	32.58%	3.124%
13	10.627	1274	1282	1297	rBV	872032	1638677	37.66%	3.612%
14	12.098	1527	1532	1538	rBV5	9104	20538	0.47%	0.045%
15	13.245	1721	1727	1731	rBV3	13567	21300	0.49%	0.047%
16	13.768	1809	1816	1828	rBV	1497645	2197149	50.50%	4.843%
17	14.039	1854	1862	1875	rBV	1730716	2599429	59.75%	5.730%
18	14.345	1907	1914	1924	rBV	1196294	1753394	40.30%	3.865%
19	14.557	1943	1950	1966	rBV	583437	1072881	24.66%	2.365%
20	15.345	2077	2084	2094	rBV	2251482	3199169	73.53%	7.052%
21	15.468	2099	2105	2118	rVV	802386	1106079	25.42%	2.438%
22	15.580	2121	2124	2132	rVB3	9835	18543	0.43%	0.041%
23	16.133	2214	2218	2225	rBV8	7592	11850	0.27%	0.026%
24	17.098	2375	2382	2392	rBV	1494196	2076031	47.72%	4.576%
25	17.198	2392	2399	2411	rVV	2463191	3488638	80.19%	7.690%
26	17.504	2448	2451	2455	rBV3	3487	5890	0.14%	0.013%
27	18.027	2532	2540	2546	rBV9	10945	28177	0.65%	0.062%
28	19.062	2712	2716	2721	rBV3	28841	37459	0.86%	0.083%
29	19.139	2724	2729	2737	rVV	22886	36727	0.84%	0.081%
30	19.309	2754	2758	2761	rBV5	5759	8192	0.19%	0.018%
31	19.497	2784	2790	2801	rBV	3012436	3999849	91.94%	8.816%
32	21.297	3090	3096	3105	rBV	1639232	2245152	51.60%	4.949%
33	23.403	3447	3454	3461	rBV2	2362605	4350708	100.00%	9.590%
34	23.544	3471	3478	3487	rVB	1325591	2470729	56.79%	5.446%

Sum of corrected areas: 45368129

Instrument :

BNA_M

ClientSampleId :




SBLK597

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044625.D
Acq On : 15 Mar 2024 10:18
Operator : MA/JU
Sample : PB159597BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

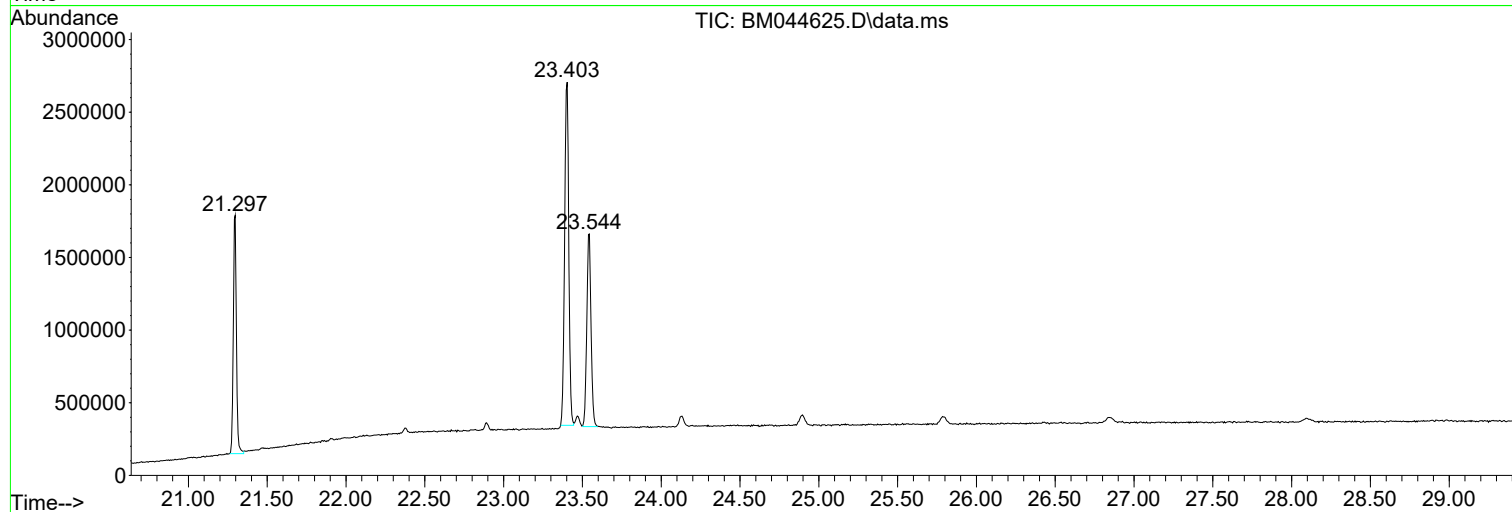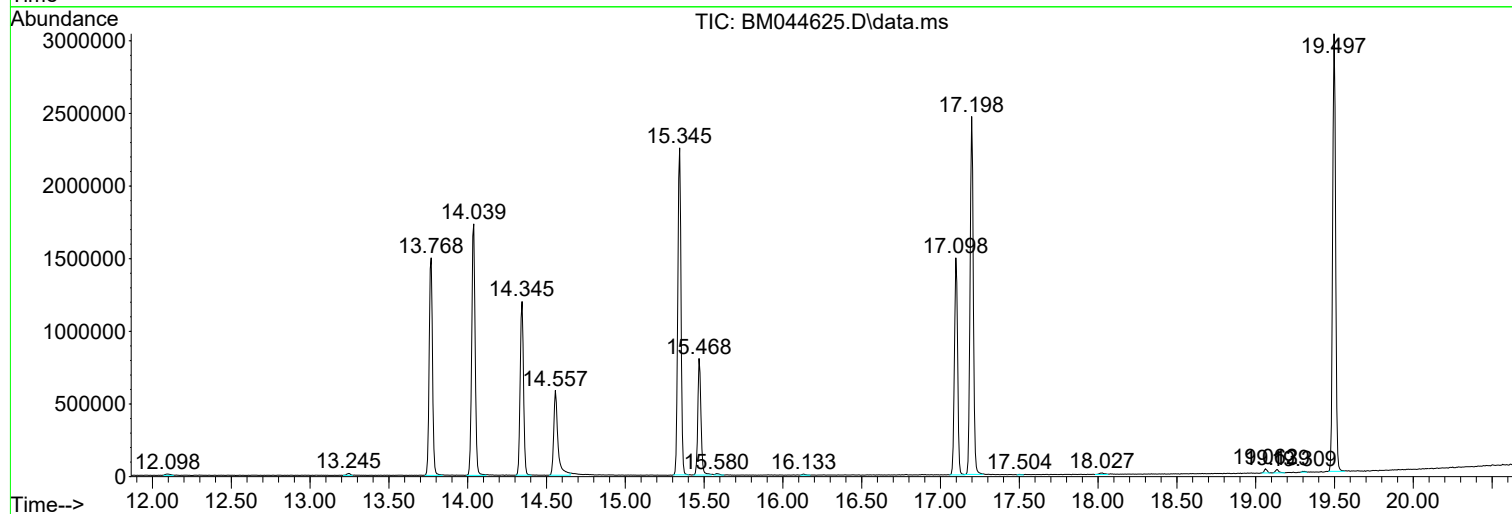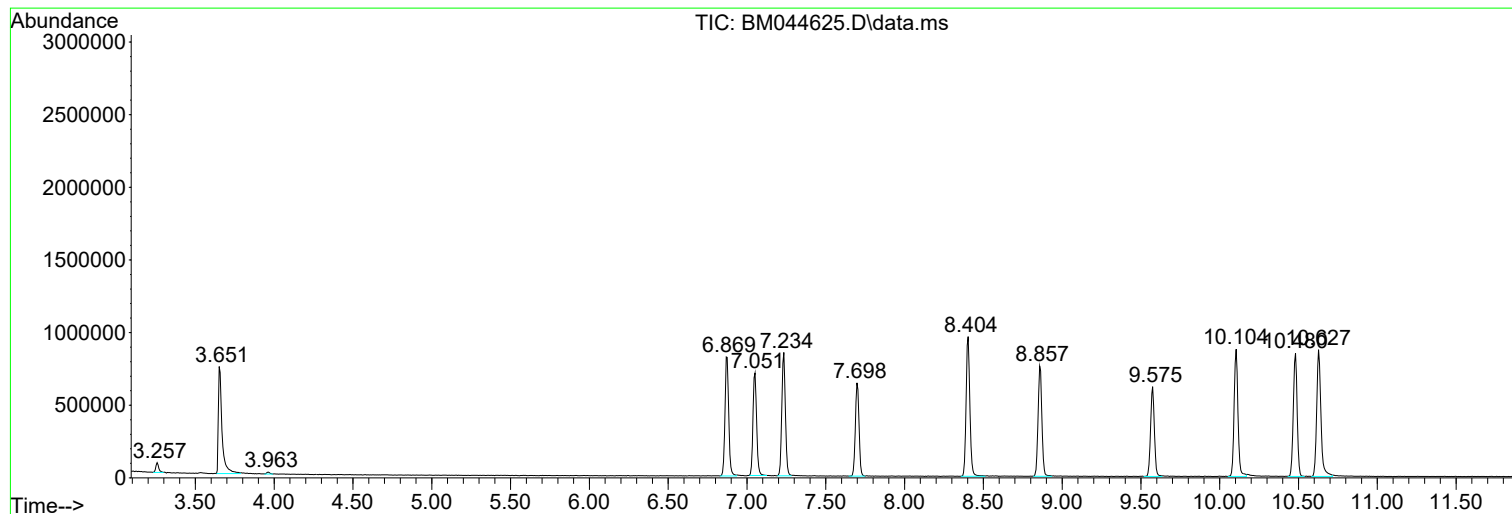

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044625.D
Acq On : 15 Mar 2024 10:18
Operator : MA/JU
Sample : PB159597BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044625.D
Acq On : 15 Mar 2024 10:18
Operator : MA/JU
Sample : PB159597BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc