

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
 Data File : BM044627.D
 Acq On : 15 Mar 2024 11:34
 Operator : MA/JU
 Sample : P1759-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0745

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.257	26	29	38	rVB	51187	69502	1.23%	0.151%
2	3.516	69	73	80	rBV5	12316	21450	0.38%	0.047%
3	3.663	94	98	114	rBV	193554	337505	5.95%	0.732%
4	3.963	145	149	155	rVB2	14583	20853	0.37%	0.045%
5	4.422	224	227	230	rVB4	6506	8532	0.15%	0.019%
6	6.875	637	644	654	rBV	153228	276671	4.88%	0.600%
7	7.051	667	674	687	rBV	738435	1169510	20.63%	2.537%
8	7.234	698	705	714	rBV	600184	955517	16.86%	2.073%
9	7.698	777	784	792	rBV	640837	1033739	18.24%	2.243%
10	8.404	897	904	916	rBV	419588	703715	12.41%	1.527%
11	8.863	974	982	994	rBV	777426	1335311	23.55%	2.897%
12	9.028	1005	1010	1015	rVB6	7141	12307	0.22%	0.027%
13	9.575	1096	1103	1113	rBV	583133	965474	17.03%	2.095%
14	10.104	1186	1193	1212	rBV	789660	1361286	24.01%	2.953%
15	10.481	1249	1257	1264	rBV	867676	1435615	25.32%	3.115%
16	10.628	1274	1282	1308	rBV	826364	1553007	27.39%	3.369%
17	12.098	1525	1532	1539	rVB3	12068	28562	0.50%	0.062%
18	13.245	1721	1727	1734	rBV4	9515	16285	0.29%	0.035%
19	13.769	1809	1816	1828	rBV	1725624	2425185	42.78%	5.261%
20	14.039	1855	1862	1875	rBV	1930236	2902145	51.19%	6.296%
21	14.345	1907	1914	1923	rBV	1253823	1881658	33.19%	4.082%
22	14.574	1945	1953	1968	rBV2	48997	142420	2.51%	0.309%
23	15.151	2047	2051	2056	rBV4	3830	8332	0.15%	0.018%
24	15.345	2077	2084	2095	rBV	2574675	3689052	65.07%	8.003%
25	15.474	2099	2106	2120	rVV	620249	924102	16.30%	2.005%
26	15.586	2120	2125	2128	rVB3	10295	13415	0.24%	0.029%
27	16.133	2214	2218	2223	rVB6	8892	13240	0.23%	0.029%
28	16.886	2339	2346	2351	rBV7	5502	13287	0.23%	0.029%
29	17.098	2375	2382	2390	rBV	1523566	2224747	39.24%	4.827%
30	17.198	2393	2399	2415	rVV2	2833798	4112446	72.54%	8.922%
31	17.504	2448	2451	2456	rBV6	3454	6598	0.12%	0.014%
32	17.798	2494	2501	2504	rBV7	4487	9194	0.16%	0.020%
33	18.009	2532	2537	2547	rBV2	36905	71490	1.26%	0.155%
34	18.092	2547	2551	2556	rVB2	6662	10702	0.19%	0.023%
35	18.874	2681	2684	2690	rVB8	5746	8889	0.16%	0.019%
36	19.062	2712	2716	2722	rVB4	32034	42002	0.74%	0.091%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044627.D
Acq On : 15 Mar 2024 11:34
Operator : MA/JU
Sample : P1759-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0745

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

37	19.133	2724	2728	2733	rBV	29260	41152	0.73%	0.089%
38	19.298	2752	2756	2765	rBV6	21801	41801	0.74%	0.091%
39	19.498	2784	2790	2799	rVV	3527421	4866519	85.85%	10.558%
40	19.745	2829	2832	2836	rVB2	16469	18488	0.33%	0.040%
41	21.021	3046	3049	3058	rBV3	71787	118208	2.09%	0.256%
42	21.297	3090	3096	3106	rBV	1953503	2544674	44.89%	5.521%
43	23.403	3447	3454	3462	rBV2	3102451	5668950	100.00%	12.299%
44	23.544	3471	3478	3489	rVB	1616880	2990433	52.75%	6.488%




Sum of corrected areas: 46093970

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044627.D
Acq On : 15 Mar 2024 11:34
Operator : MA/JU
Sample : P1759-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0745

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

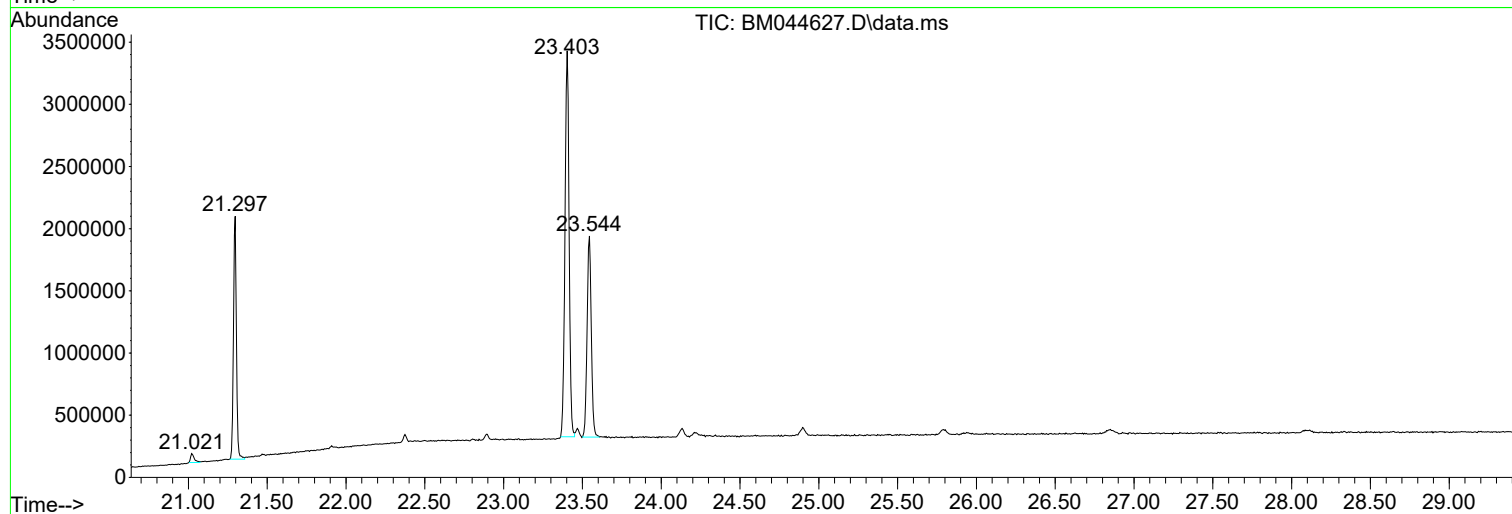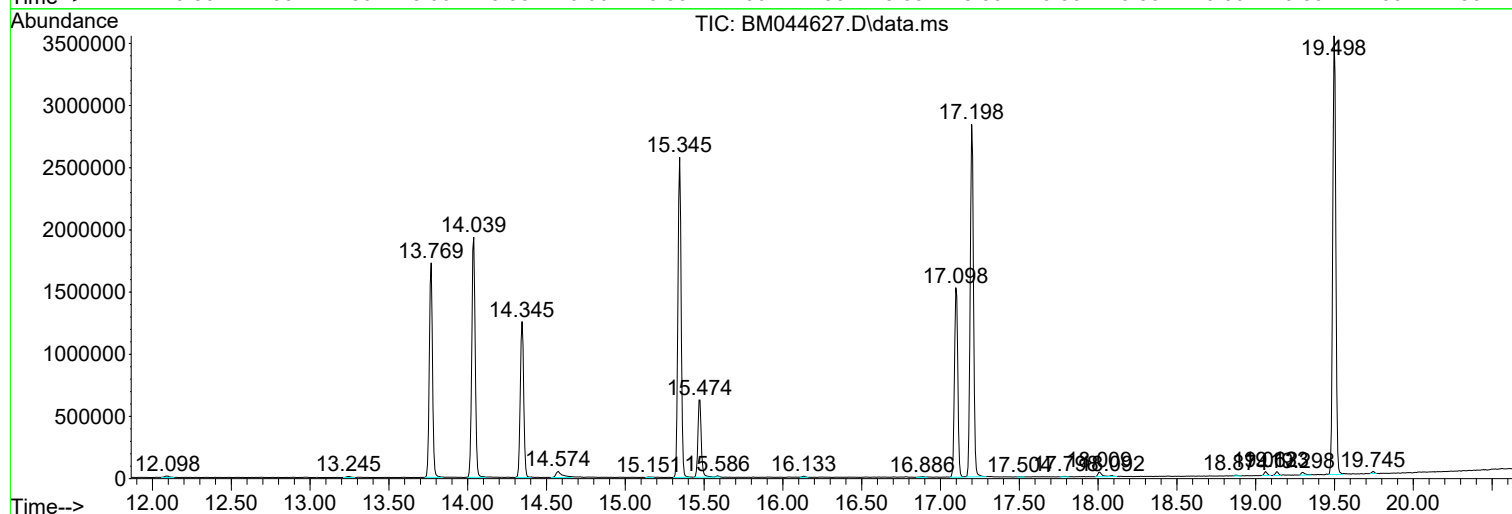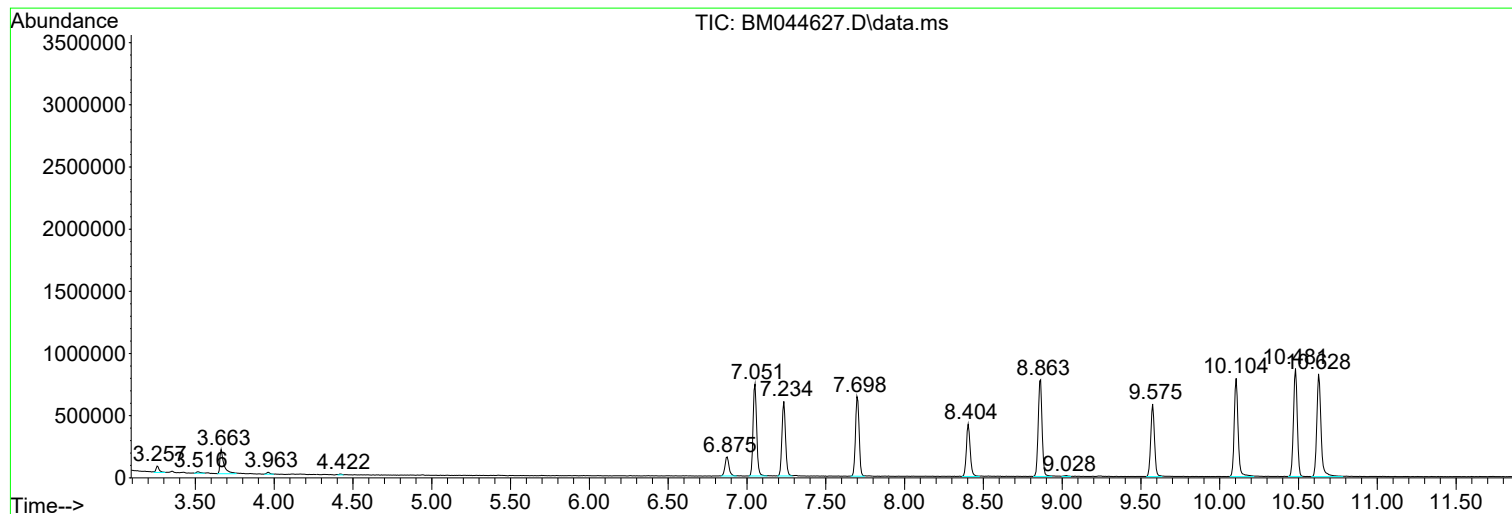

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044627.D
Acq On : 15 Mar 2024 11:34
Operator : MA/JU
Sample : P1759-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0745

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044627.D
Acq On : 15 Mar 2024 11:34
Operator : MA/JU
Sample : P1759-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0745

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------