

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
 Data File : BM044636.D
 Acq On : 15 Mar 2024 17:04
 Operator : MA/JU
 Sample : PB159597BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK597

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044636.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	36	rVB	73827	94262	1.84%	0.176%
2	3.652	93	96	120	rBV	890949	1385302	27.09%	2.589%
3	3.958	145	148	155	rVB2	15670	22070	0.43%	0.041%
4	6.869	637	643	659	rBV	969726	1568229	30.66%	2.931%
5	7.046	667	673	688	rVB	810889	1314770	25.71%	2.457%
6	7.234	697	705	715	rBV	950131	1552276	30.35%	2.901%
7	7.698	777	784	792	rBV	755870	1181878	23.11%	2.209%
8	8.398	896	903	913	rBV	1103417	1862850	36.42%	3.481%
9	8.857	974	981	994	rBV	882355	1491168	29.15%	2.787%
10	9.575	1095	1103	1116	rBV	709403	1228559	24.02%	2.296%
11	10.104	1184	1193	1204	rBV	1007374	1772020	34.65%	3.312%
12	10.481	1249	1257	1266	rBV	970774	1655307	32.36%	3.093%
13	10.628	1274	1282	1308	rBV	1051263	1956531	38.25%	3.656%
14	12.092	1524	1531	1537	rBV2	11824	25899	0.51%	0.048%
15	13.239	1720	1726	1733	rBV	22750	39664	0.78%	0.074%
16	13.763	1807	1815	1825	rBV	1811925	2598987	50.81%	4.857%
17	14.033	1853	1861	1872	rBV	2006211	3112100	60.85%	5.816%
18	14.345	1907	1914	1923	rBV	1398188	2091531	40.89%	3.909%
19	14.557	1943	1950	1974	rBV	726023	1364252	26.67%	2.550%
20	15.345	2077	2084	2093	rBV	2667403	3823331	74.75%	7.145%
21	15.469	2098	2105	2118	rBV	891255	1272681	24.88%	2.378%
22	15.586	2121	2125	2129	rVB4	10709	16089	0.31%	0.030%
23	15.916	2176	2181	2183	rBV6	3782	6225	0.12%	0.012%
24	16.133	2214	2218	2223	rVB4	8243	12597	0.25%	0.024%
25	16.780	2324	2328	2334	rVB8	4759	6825	0.13%	0.013%
26	17.098	2376	2382	2392	rBV	1763688	2431102	47.53%	4.543%
27	17.198	2392	2399	2417	rVV	2928257	4125642	80.66%	7.710%
28	18.021	2534	2539	2542	rBV6	8400	12717	0.25%	0.024%
29	19.062	2711	2716	2722	rBV3	32343	48206	0.94%	0.090%
30	19.133	2724	2728	2732	rBV	28566	42486	0.83%	0.079%
31	19.451	2779	2782	2784	rBV4	7466	8196	0.16%	0.015%
32	19.498	2784	2790	2800	rVV	3638249	4759396	93.05%	8.895%
33	21.292	3090	3095	3105	rBV	1950425	2613044	51.09%	4.883%
34	23.397	3446	3453	3460	rBV2	2805305	5114631	100.00%	9.558%
35	23.539	3471	3477	3489	rVB	1516970	2898390	56.67%	5.417%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044636.D
Acq On : 15 Mar 2024 17:04
Operator : MA/JU
Sample : PB159597BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK597

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 53509213

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044636.D
Acq On : 15 Mar 2024 17:04
Operator : MA/JU
Sample : PB159597BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

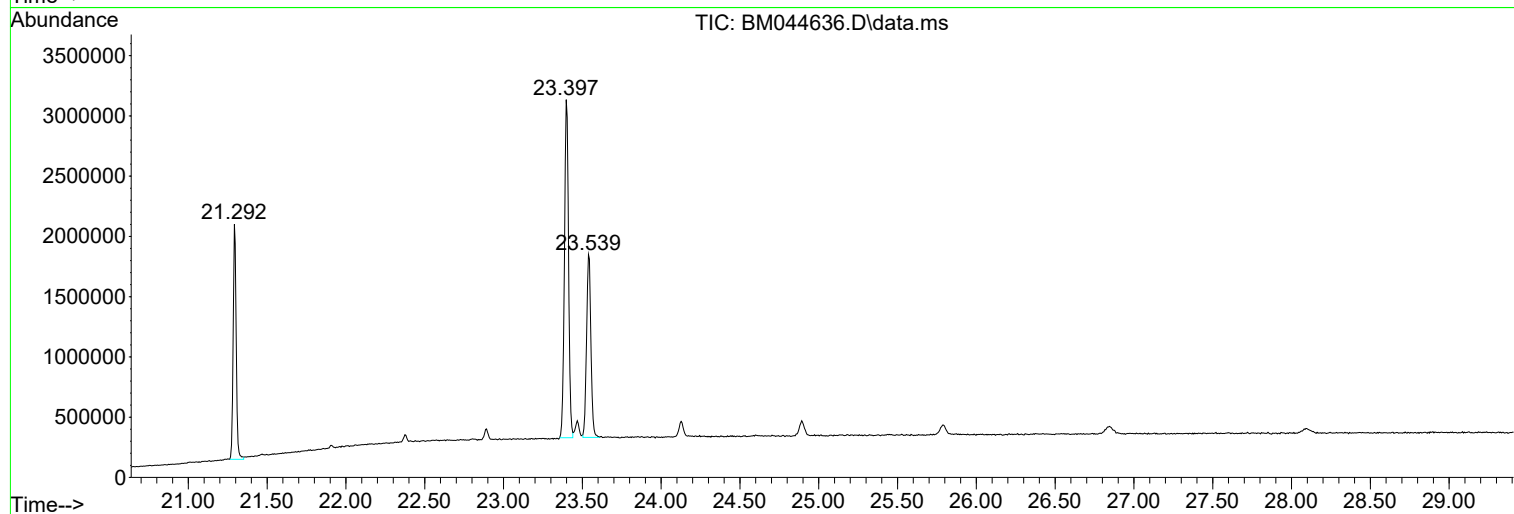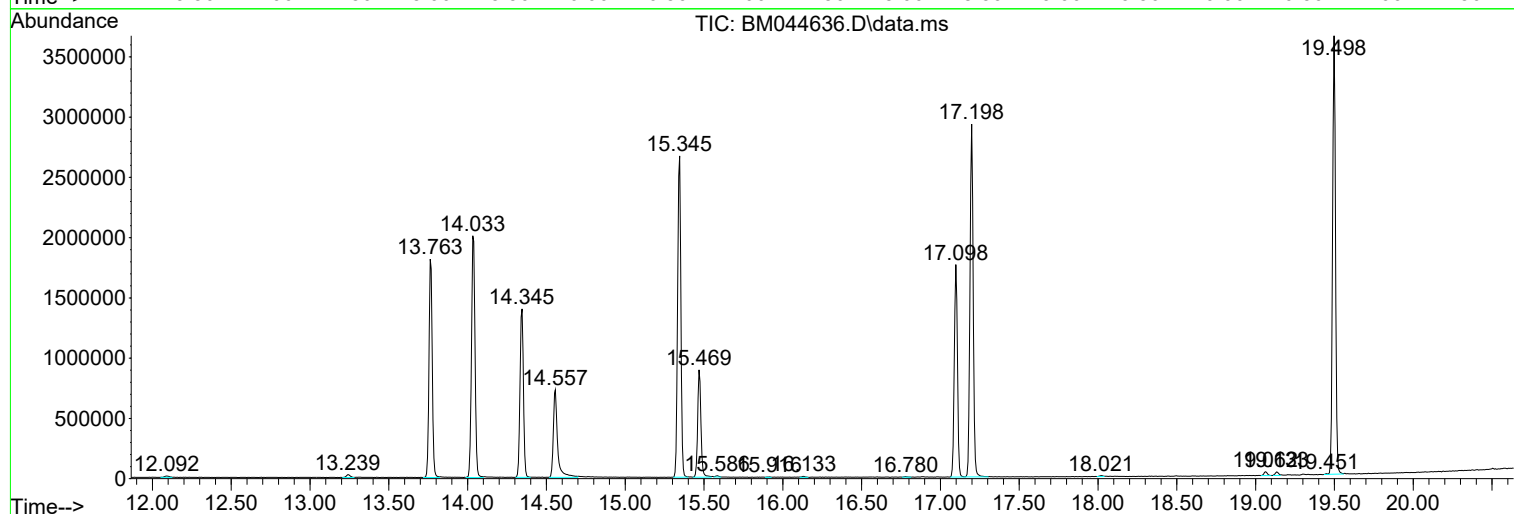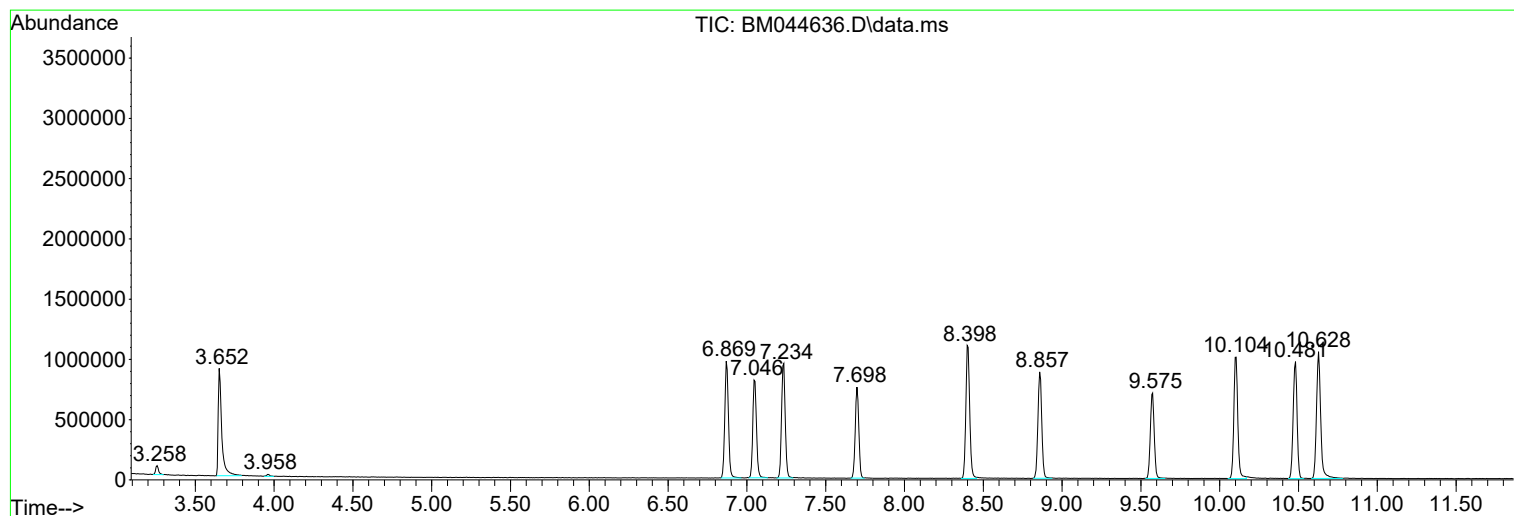

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044636.D
Acq On : 15 Mar 2024 17:04
Operator : MA/JU
Sample : PB159597BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044636.D
Acq On : 15 Mar 2024 17:04
Operator : MA/JU
Sample : PB159597BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc