

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044637.D
Acq On : 15 Mar 2024 17:40
Operator : MA/JU
Sample : PB159595BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK595

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BM044637.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.257	25	29	38	rVB	63066	78807	2.06%	0.191%
2	3.651	93	96	122	rBV	695764	1116031	29.22%	2.704%
3	3.963	145	149	153	rVB	10961	13780	0.36%	0.033%
4	6.869	637	643	661	rBV	763827	1249462	32.71%	3.027%
5	7.045	667	673	686	rBV	648188	1048584	27.46%	2.540%
6	7.234	698	705	717	rBV	751857	1235917	32.36%	2.994%
7	7.698	777	784	794	rVB	599048	943831	24.71%	2.287%
8	7.969	828	830	833	rBV4	3554	4962	0.13%	0.012%
9	8.398	897	903	918	rBV	866797	1481430	38.79%	3.589%
10	8.857	974	981	991	rBV	713305	1180807	30.92%	2.861%
11	9.569	1096	1102	1114	rBV	557408	951481	24.91%	2.305%
12	10.104	1183	1193	1215	rBV	775139	1430757	37.46%	3.466%
13	10.480	1249	1257	1264	rBV	750034	1300531	34.05%	3.151%
14	10.628	1273	1282	1297	rBV	816586	1542206	40.38%	3.736%
15	12.098	1525	1532	1538	rBV3	9695	19753	0.52%	0.048%
16	13.239	1721	1726	1733	rVB2	17473	29600	0.78%	0.072%
17	13.763	1808	1815	1829	rBV	1372850	2025735	53.04%	4.908%
18	14.033	1854	1861	1870	rBV	1657765	2439272	63.87%	5.910%
19	14.345	1907	1914	1925	rBV	1107496	1617032	42.34%	3.918%
20	14.557	1942	1950	1973	rBV	497033	1005747	26.33%	2.437%
21	15.345	2076	2084	2096	rBV	2033231	3018628	79.04%	7.313%
22	15.468	2099	2105	2116	rBV	649697	919783	24.08%	2.228%
23	15.586	2121	2125	2131	rVB7	9402	15756	0.41%	0.038%
24	16.133	2213	2218	2222	rVB5	6598	10444	0.27%	0.025%
25	16.774	2325	2327	2331	rBV6	3362	4559	0.12%	0.011%
26	16.892	2340	2347	2350	rBV6	2529	4460	0.12%	0.011%
27	17.098	2375	2382	2392	rBV	1348948	1865146	48.84%	4.519%
28	17.198	2392	2399	2416	rVV	2248494	3183563	83.36%	7.713%
29	18.021	2532	2539	2540	rBV7	6847	10254	0.27%	0.025%
30	19.062	2712	2716	2720	rBV3	25776	35382	0.93%	0.086%
31	19.133	2724	2728	2734	rBV	21825	37064	0.97%	0.090%
32	19.498	2784	2790	2801	rBV	2675204	3622440	94.85%	8.776%
33	21.297	3090	3096	3103	rBV	1403704	1924072	50.38%	4.662%
34	23.397	3446	3453	3461	rBV2	2039289	3819249	100.00%	9.253%
35	23.538	3471	3477	3488	rVB	1082838	2088538	54.68%	5.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044637.D
Acq On : 15 Mar 2024 17:40
Operator : MA/JU
Sample : PB159595BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK595

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 41275063

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044637.D
Acq On : 15 Mar 2024 17:40
Operator : MA/JU
Sample : PB159595BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK595

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

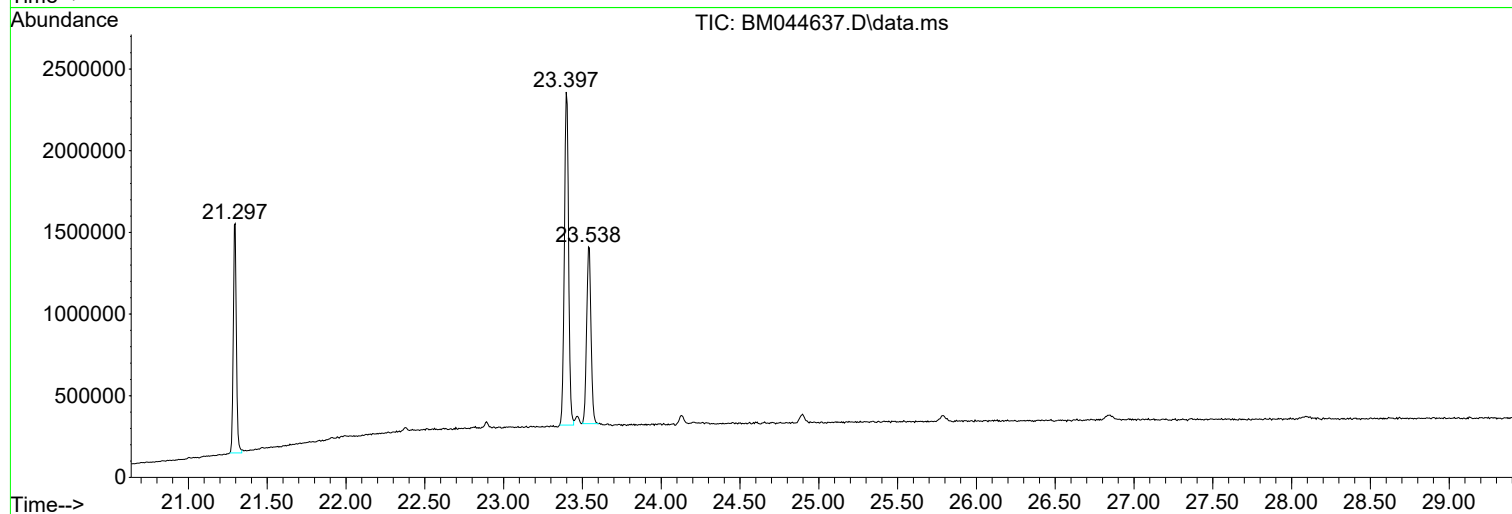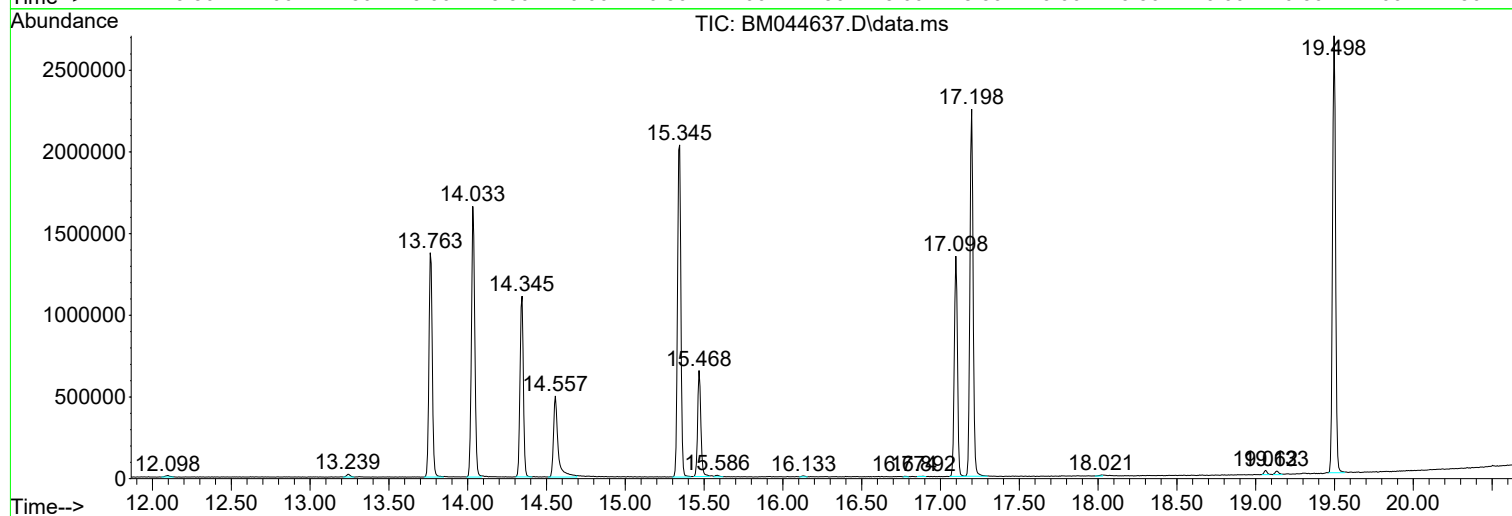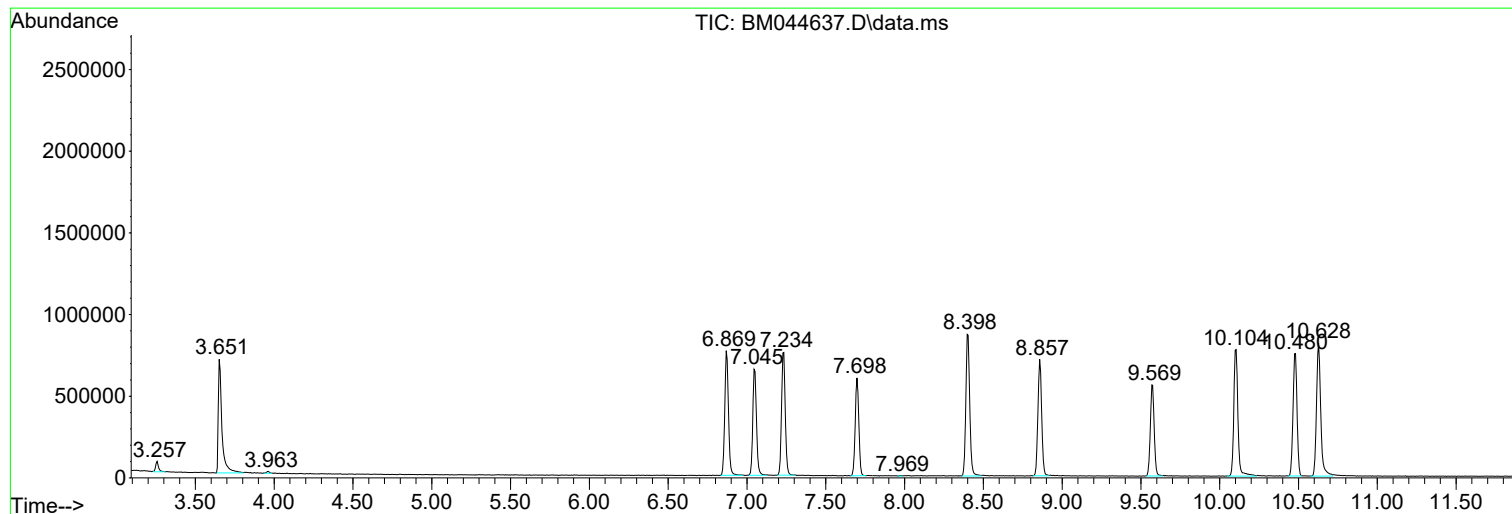

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044637.D
Acq On : 15 Mar 2024 17:40
Operator : MA/JU
Sample : PB159595BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK595

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044637.D
Acq On : 15 Mar 2024 17:40
Operator : MA/JU
Sample : PB159595BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK595

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc