

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
 Data File : BM044647.D
 Acq On : 15 Mar 2024 23:42
 Operator : MA/JU
 Sample : PB159622BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK622

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044647.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.257	25	29	37	rVB	66186	87872	2.12%	0.198%
2	3.651	92	96	118	rBV	761892	1216353	29.31%	2.734%
3	3.963	145	149	154	rVB3	12318	19153	0.46%	0.043%
4	6.869	636	643	652	rBV	860392	1376389	33.16%	3.094%
5	7.045	667	673	689	rVB	747137	1176077	28.34%	2.643%
6	7.228	697	704	715	rBV	866947	1375017	33.13%	3.091%
7	7.557	757	760	762	rBV4	4068	4715	0.11%	0.011%
8	7.698	777	784	795	rBV	603230	965882	23.27%	2.171%
9	8.398	896	903	916	rBV	1009729	1633182	39.35%	3.671%
10	8.857	974	981	995	rBV	792188	1318226	31.76%	2.963%
11	9.569	1094	1102	1114	rBV	626780	1068320	25.74%	2.401%
12	10.098	1183	1192	1211	rBV	893384	1574701	37.94%	3.539%
13	10.475	1249	1256	1267	rVB	777942	1313555	31.65%	2.952%
14	10.627	1272	1282	1302	rBV	868861	1692771	40.78%	3.805%
15	12.092	1524	1531	1538	rVB2	10595	23340	0.56%	0.052%
16	13.239	1720	1726	1736	rBV3	17697	30526	0.74%	0.069%
17	13.763	1808	1815	1825	rBV	1602351	2246350	54.12%	5.049%
18	14.033	1854	1861	1875	rBV	1795250	2696851	64.98%	6.062%
19	14.339	1906	1913	1928	rVB	1100692	1627705	39.22%	3.659%
20	14.551	1941	1949	1967	rBV	565764	1079492	26.01%	2.426%
21	15.339	2076	2083	2094	rBV	2269960	3291679	79.31%	7.399%
22	15.468	2099	2105	2119	rBV	756779	1084325	26.12%	2.437%
23	15.586	2121	2125	2130	rVB7	9171	15966	0.38%	0.036%
24	16.127	2213	2217	2221	rBV5	7319	10200	0.25%	0.023%
25	16.974	2357	2361	2364	rBV6	2440	4268	0.10%	0.010%
26	17.098	2373	2382	2392	rBV	1308625	1852713	44.64%	4.164%
27	17.198	2392	2399	2410	rBV	2399255	3537086	85.22%	7.950%
28	18.021	2533	2539	2541	rBV6	5521	9350	0.23%	0.021%
29	19.062	2712	2716	2722	rVB2	25355	34210	0.82%	0.077%
30	19.133	2724	2728	2735	rVB2	21212	29765	0.72%	0.067%
31	19.450	2779	2782	2783	rBV2	6651	6878	0.17%	0.015%
32	19.497	2783	2790	2798	rVV	2934628	3981364	95.92%	8.949%
33	21.291	3090	3095	3104	rBV	1489333	1890726	45.55%	4.250%
34	23.397	3446	3453	3461	rBV2	2259041	4150563	100.00%	9.329%
35	23.538	3470	3477	3487	rVB	1059348	2064634	49.74%	4.641%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044647.D
Acq On : 15 Mar 2024 23:42
Operator : MA/JU
Sample : PB159622BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK622

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 44490204

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044647.D
Acq On : 15 Mar 2024 23:42
Operator : MA/JU
Sample : PB159622BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK622

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

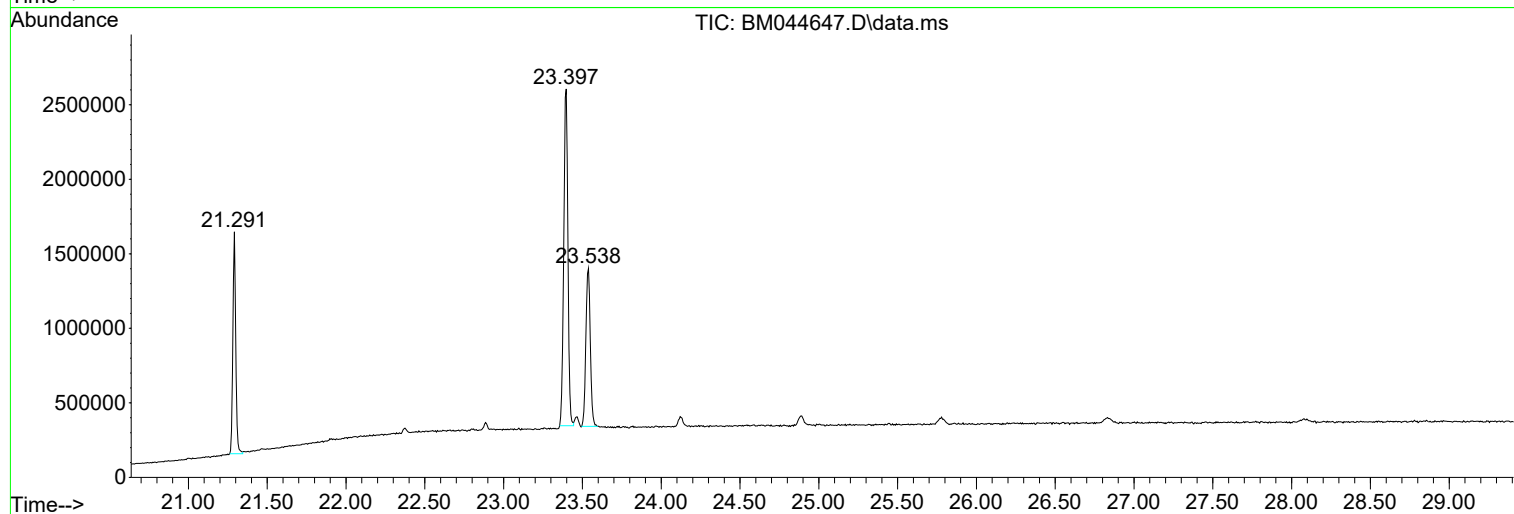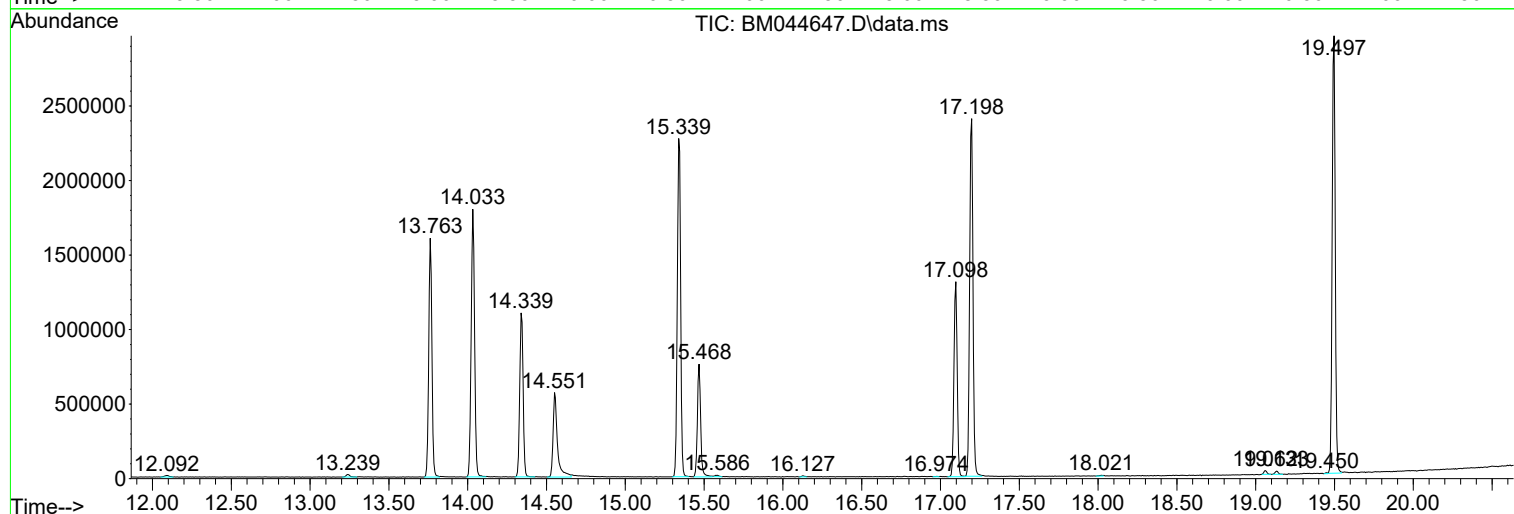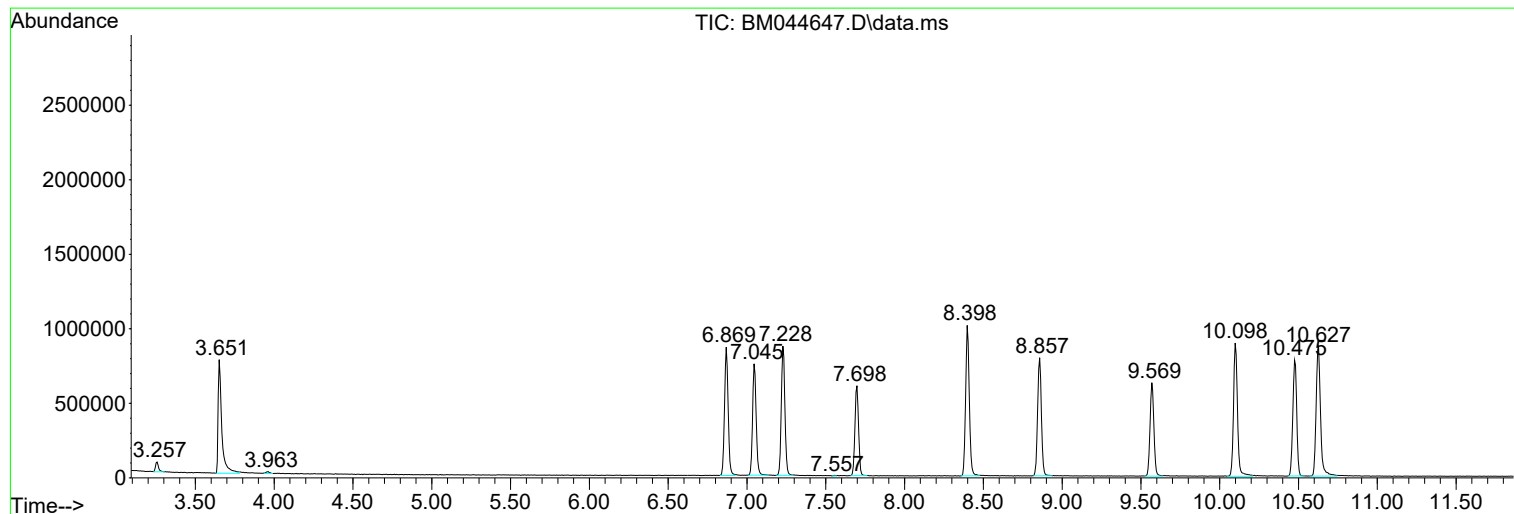

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044647.D
Acq On : 15 Mar 2024 23:42
Operator : MA/JU
Sample : PB159622BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK622

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044647.D
Acq On : 15 Mar 2024 23:42
Operator : MA/JU
Sample : PB159622BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK622

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc