

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
 Data File : BM044651.D
 Acq On : 16 Mar 2024 02:06
 Operator : MA/JU
 Sample : P1779-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044651.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.257	25	29	39	rVB	53838	78908	1.44%	0.168%
2	3.663	95	98	118	rVB	147116	272820	4.96%	0.580%
3	3.957	145	148	152	rVB	13061	15141	0.28%	0.032%
4	6.234	532	535	540	rBV7	2865	5597	0.10%	0.012%
5	6.869	636	643	655	rBV	180286	306621	5.58%	0.651%
6	7.045	666	673	683	rBV	875747	1377641	25.06%	2.926%
7	7.228	697	704	715	rBV	744670	1202086	21.86%	2.553%
8	7.698	777	784	791	rBV	605651	966544	17.58%	2.053%
9	7.763	791	795	802	rVB8	5761	11352	0.21%	0.024%
10	8.398	896	903	915	rBV	538217	883879	16.08%	1.878%
11	8.857	973	981	993	rBV	940739	1570966	28.57%	3.337%
12	9.569	1094	1102	1114	rBV	714351	1205989	21.93%	2.562%
13	10.098	1184	1192	1208	rBV	940396	1652791	30.06%	3.511%
14	10.474	1248	1256	1264	rBV	802421	1313949	23.90%	2.791%
15	10.622	1273	1281	1303	rBV	792971	1531138	27.85%	3.252%
16	11.833	1481	1487	1495	rBV2	23664	42276	0.77%	0.090%
17	12.080	1522	1529	1536	rVB	13309	28664	0.52%	0.061%
18	13.239	1721	1726	1732	rVB2	20458	33554	0.61%	0.071%
19	13.763	1808	1815	1828	rBV	1853398	2630158	47.84%	5.587%
20	14.033	1854	1861	1873	rBV	2209263	3247928	59.07%	6.899%
21	14.339	1906	1913	1924	rBV	1100392	1630333	29.65%	3.463%
22	14.568	1946	1952	1966	rBV2	63705	177521	3.23%	0.377%
23	15.151	2045	2051	2057	rBV	18302	26929	0.49%	0.057%
24	15.339	2076	2083	2098	rBV	2834371	4017937	73.08%	8.535%
25	15.468	2098	2105	2113	rBV	933295	1276687	23.22%	2.712%
26	15.580	2121	2124	2129	rVB3	12203	16813	0.31%	0.036%
27	16.127	2213	2217	2223	rBV6	7670	11066	0.20%	0.024%
28	16.892	2341	2347	2348	rBV5	4755	8035	0.15%	0.017%
29	17.098	2375	2382	2391	rBV	1314621	1858857	33.81%	3.949%
30	17.198	2392	2399	2413	rVV	3168770	4598239	83.63%	9.768%
31	17.774	2495	2497	2503	rVB5	8629	12464	0.23%	0.026%
32	18.003	2531	2536	2545	rBV	62834	105083	1.91%	0.223%
33	18.445	2607	2611	2614	rBV5	5264	6270	0.11%	0.013%
34	19.062	2711	2716	2720	rBV2	34593	48792	0.89%	0.104%
35	19.133	2723	2728	2732	rBV	29109	40699	0.74%	0.086%
36	19.292	2751	2755	2760	rBV5	32482	49875	0.91%	0.106%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044651.D
Acq On : 16 Mar 2024 02:06
Operator : MA/JU
Sample : P1779-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AJ8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

37	19.497	2783	2790	2804	rBV	3959724	5234782	95.21%	11.120%
38	21.291	3090	3095	3105	rBV	1526337	1979699	36.01%	4.205%
39	23.397	3446	3453	3460	rBV2	3044101	5498279	100.00%	11.680%
40	23.538	3471	3477	3486	rVB	1105484	2099746	38.19%	4.460%




Sum of corrected areas: 47076108

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044651.D
Acq On : 16 Mar 2024 02:06
Operator : MA/JU
Sample : P1779-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AJ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

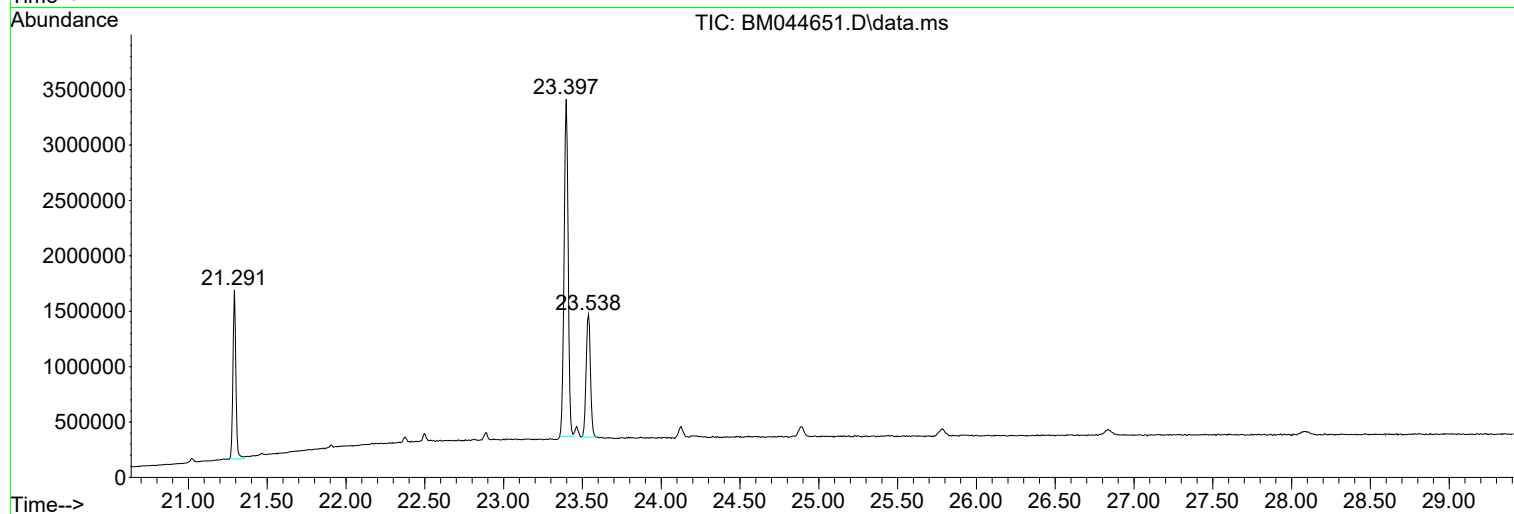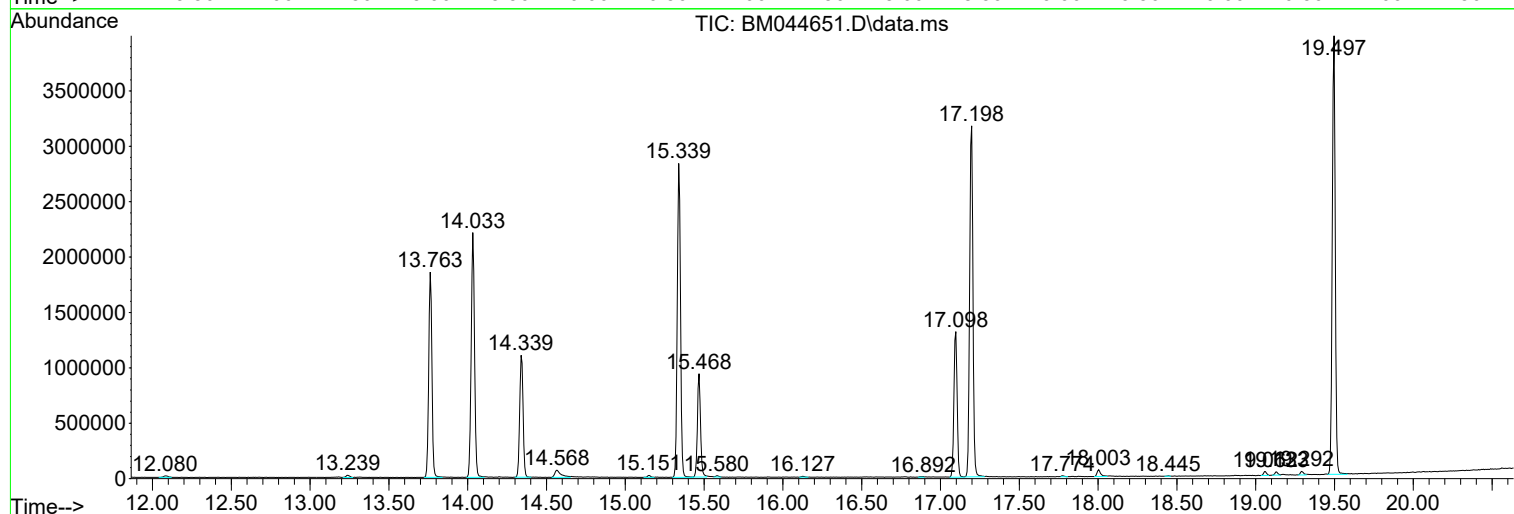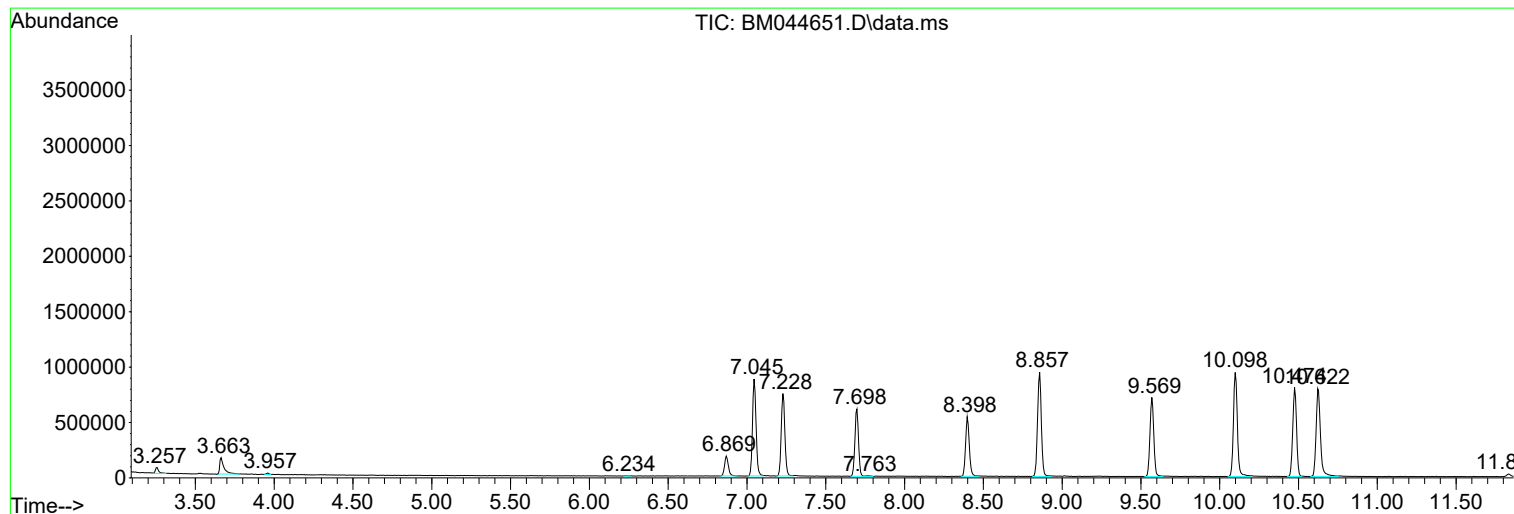

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044651.D
Acq On : 16 Mar 2024 02:06
Operator : MA/JU
Sample : P1779-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AJ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031624\
Data File : BM044651.D
Acq On : 16 Mar 2024 02:06
Operator : MA/JU
Sample : P1779-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AJ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc