

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031716\
 Data File : BM004662.D
 Acq On : 17 Mar 2016 12:30
 Operator : UM/SJ
 Sample : H1779-22
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 18 05:03:11 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM031516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 18 05:01:04 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	69537	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	302511	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.47	164	168611	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.22	188	372293	20.00	ng/ul	0.00
78) Chrysene-d12	21.40	240	404048	20.00	ng/ul	0.00
86) Perylene-d12	23.71	264	388250	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.33	96	4663	2.31	ng/uL	0.00
5) Phenol-d5	7.00	99	91465	16.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	54250	16.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	73917	16.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	69396	15.07	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	32675	15.53	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	33533	14.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	69352	15.56	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	76294	14.30	ng/ul	0.00
44) Dimethylphthalate-d6	13.88	166	220977	16.76	ng/ul	0.00
47) Acenaphthylene-d8	14.17	160	280304	17.34	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	9404	3.69	ng/ul	0.00
58) Fluorene-d10	15.47	176	205247	17.87	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.58	200	6645	3.40	ng/ul	0.00
71) Anthracene-d10	17.32	188	312788	18.25	ng/ul	0.00
79) Pyrene-d10	19.61	212	354209	19.20	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.56	264	363095	20.94	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.93	163	76243	5.70	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031716\
Data File : BM004662.D
Acq On : 17 Mar 2016 12:30
Operator : UM/SJ
Sample : H1779-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 18 05:03:11 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 18 05:01:04 2016
Response via : Initial Calibration

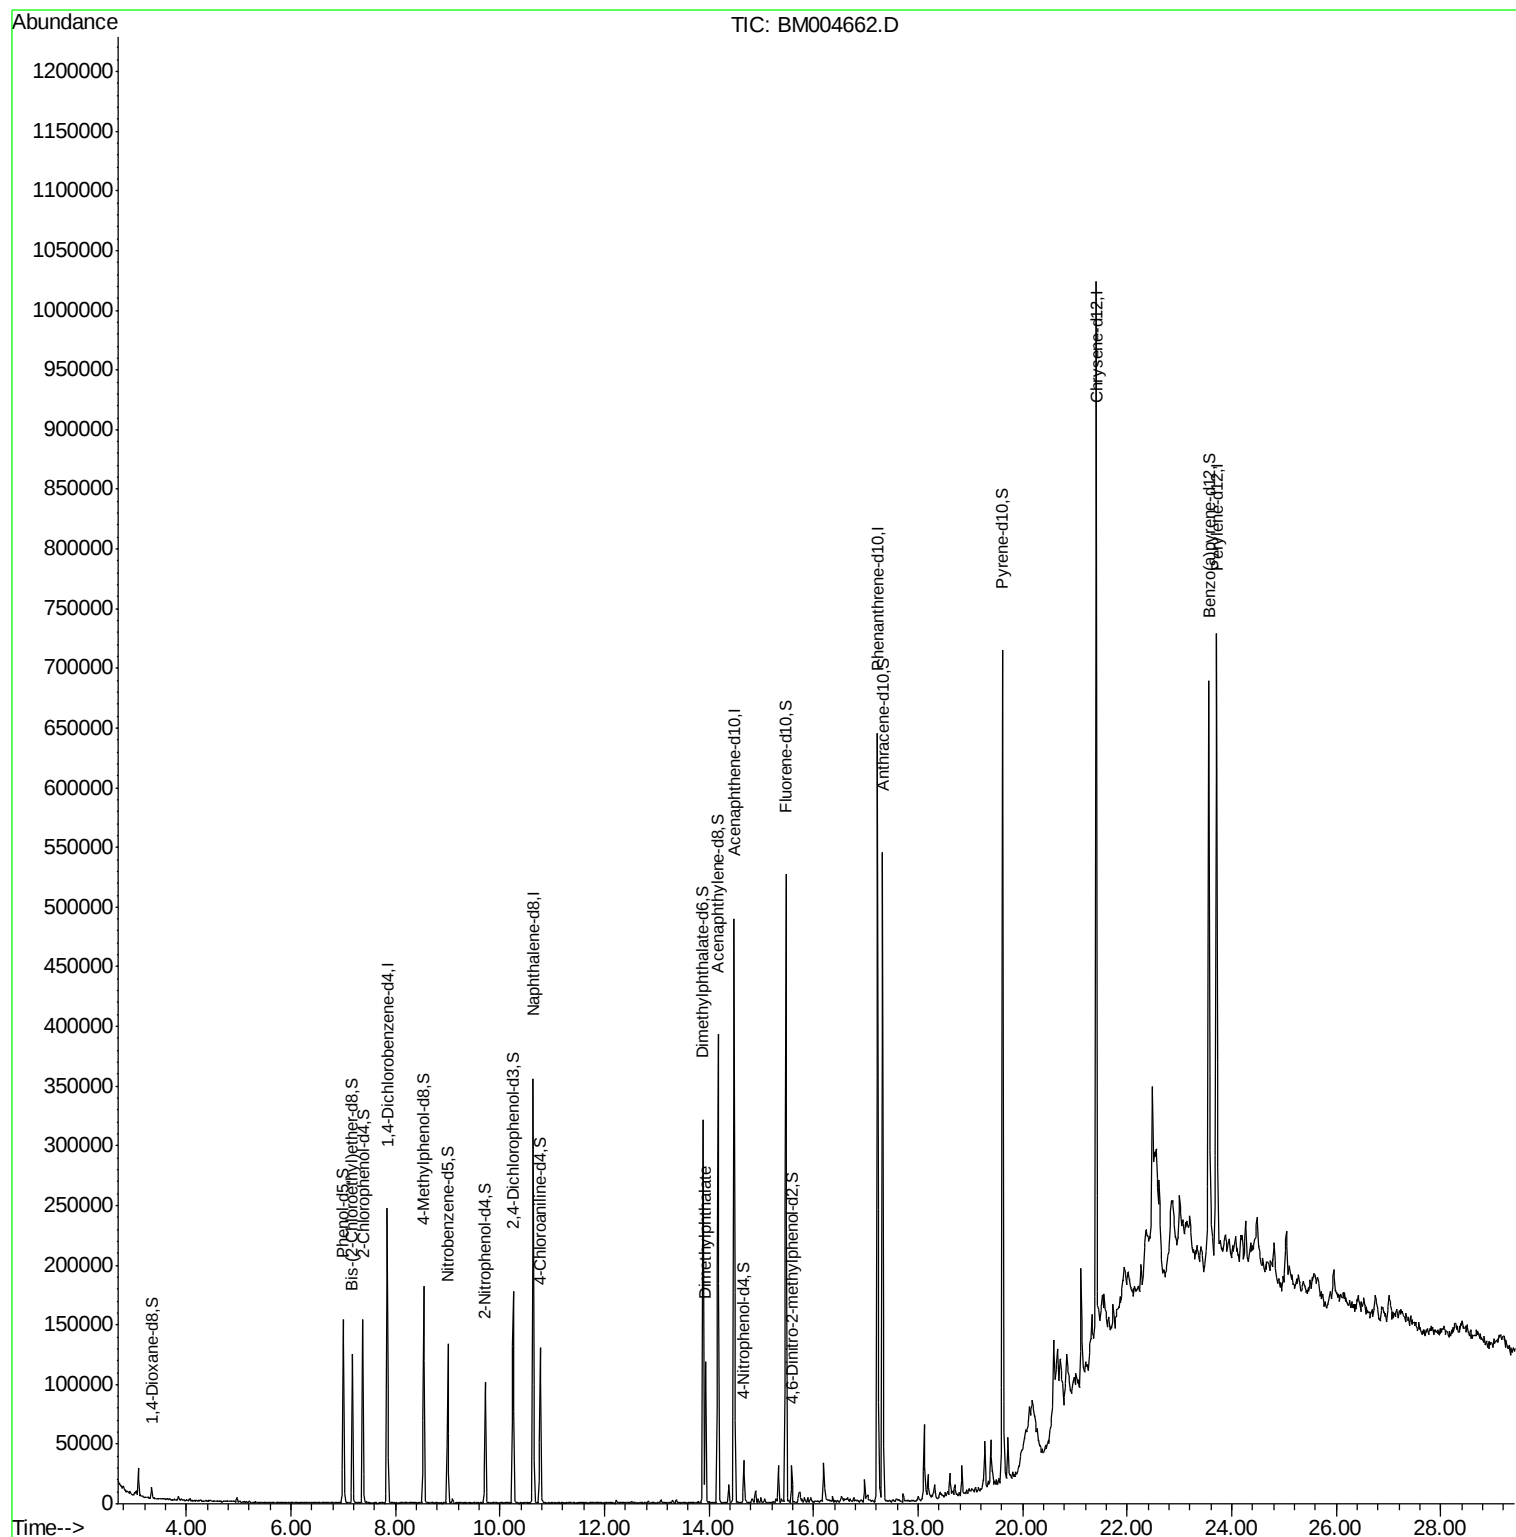


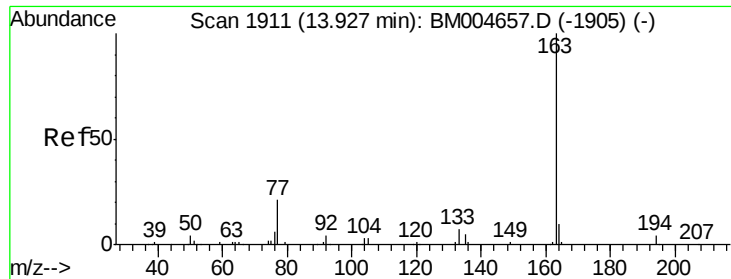

#45
 Dimethylphthalate
 Concen: 5.70 ng/ul
 RT: 13.93 min Scan# 1911
 Delta R.T. -0.00 min
 Lab File: BM004662.D
 Acq: 17 Mar 2016 12:30

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:163 Resp: 76243
 Ion Ratio Lower Upper
 163 100
 194 4.1 3.2 4.8
 164 10.6 7.8 11.8

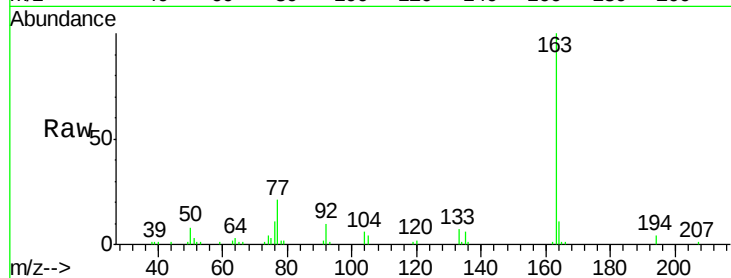

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

